

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062421\
 Data File : P0079120.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jun 2021 16:56
 Operator : DD\AJ
 Sample : M2820-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PIA-124

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 02:28:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.323	3.600	1673337	614976	21.202	20.692
2) SA Decachlor...	9.922	8.777	1290439	569626	20.662	19.116

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062421\
Data File : P0079120.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jun 2021 16:56
Operator : DD\AJ
Sample : M2820-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PIA-124

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 02:28:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

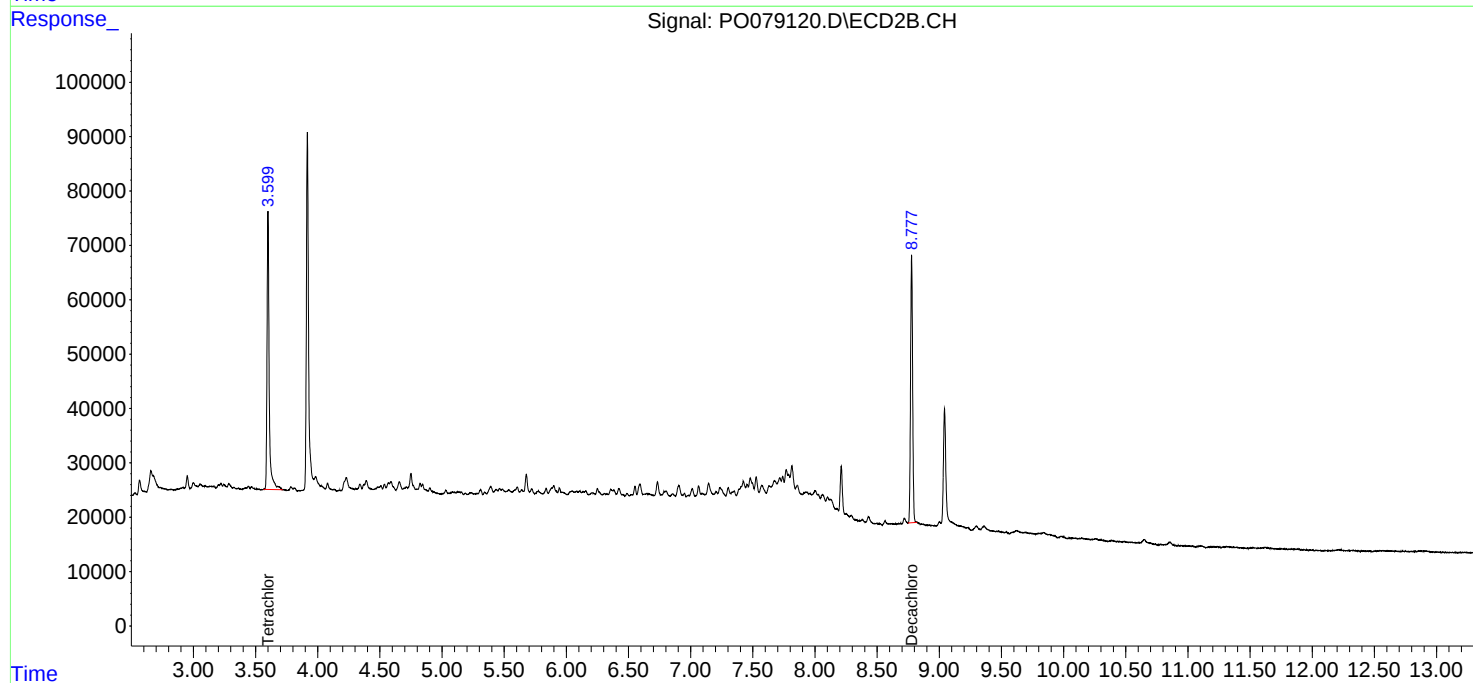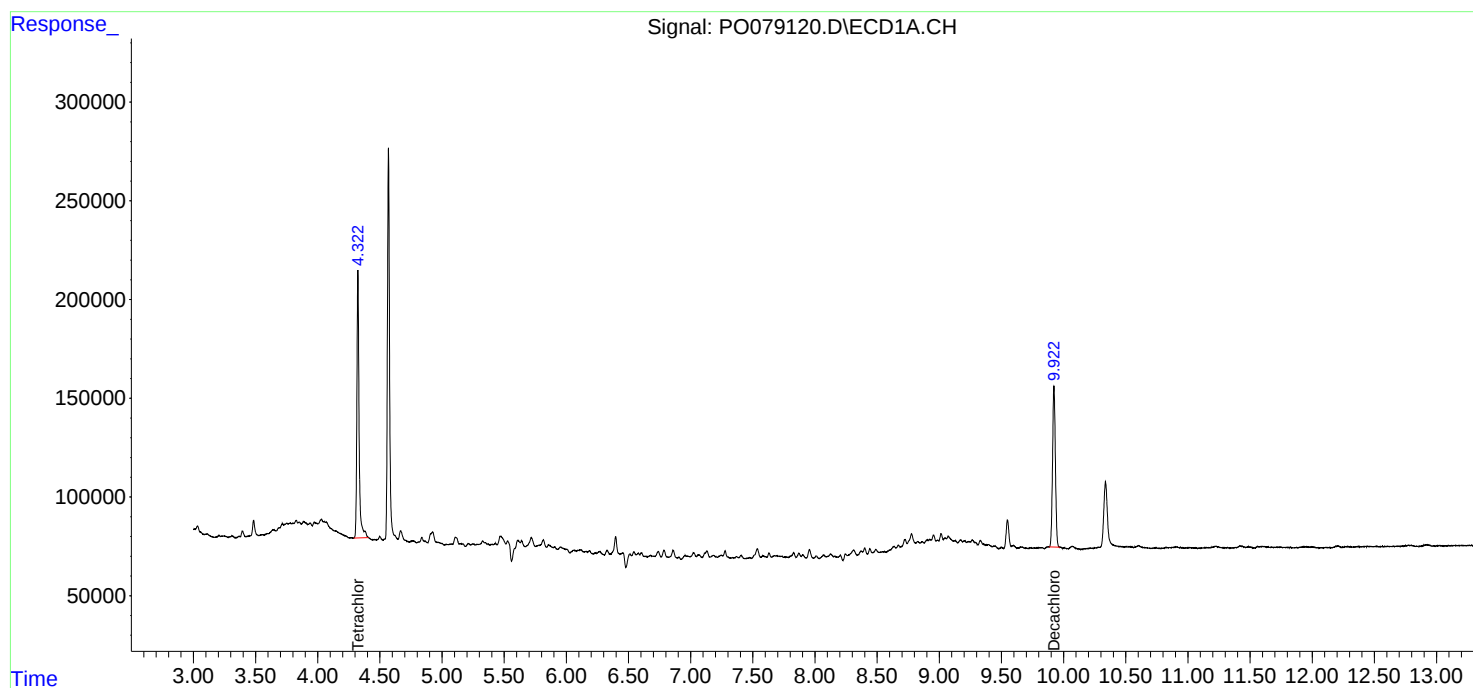


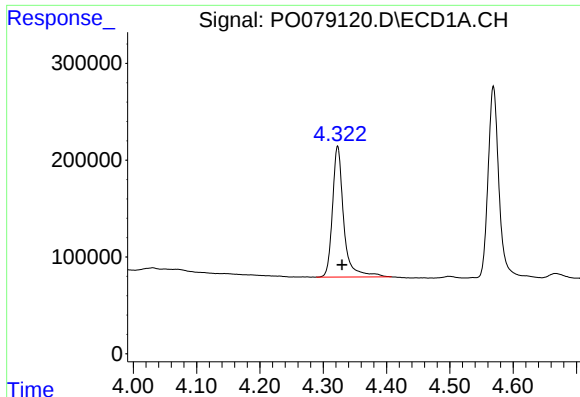

#1 Tetrachloro-m-xylene


R.T.: 4.323 min
Delta R.T.: -0.007 min
Response: 1673337
Conc: 21.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
PIA-124

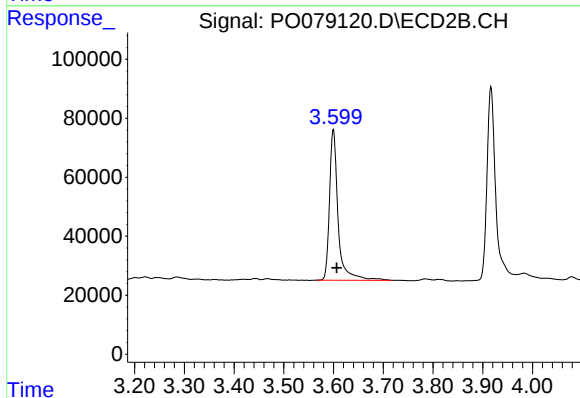


#1 Tetrachloro-m-xylene

R.T.: 3.600 min
Delta R.T.: -0.007 min
Response: 614976
Conc: 20.69 ng/ml

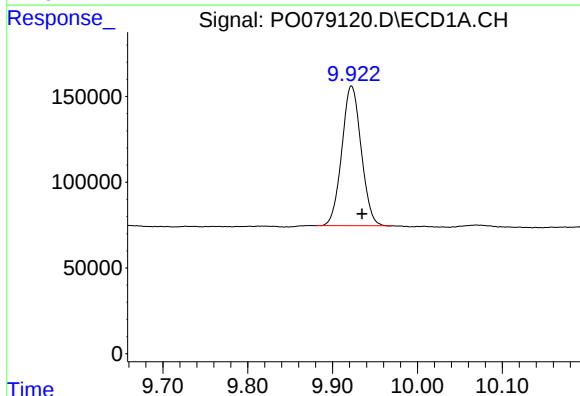

#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: -0.012 min
Response: 1290439
Conc: 20.66 ng/ml

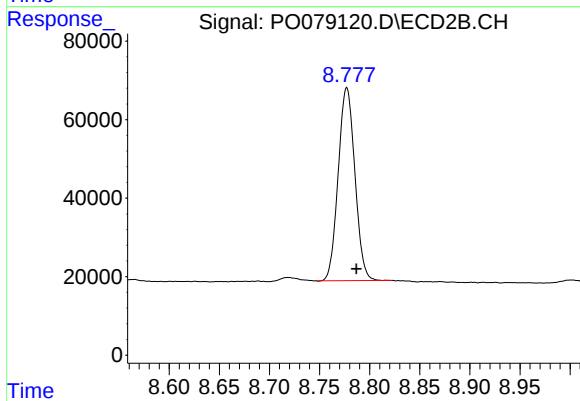

#2 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: -0.010 min
Response: 569626
Conc: 19.12 ng/ml