

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062520\
 Data File : P0069194.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2020 13:17
 Operator : DD\AJ
 Sample : L3099-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUCT-BANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 13:37:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 19 05:15:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.402	3.563	746845	861362	25.246	22.379
2)	SA Decachlor...	10.065	8.771	846690	953895	17.826	17.523
Target Compounds							
45)	L9 AR-1268-5	9.801	0.000	43341	0	2.560	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062520\
Data File : P0069194.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2020 13:17
Operator : DD\AJ
Sample : L3099-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DUCT-BANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 13:37:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

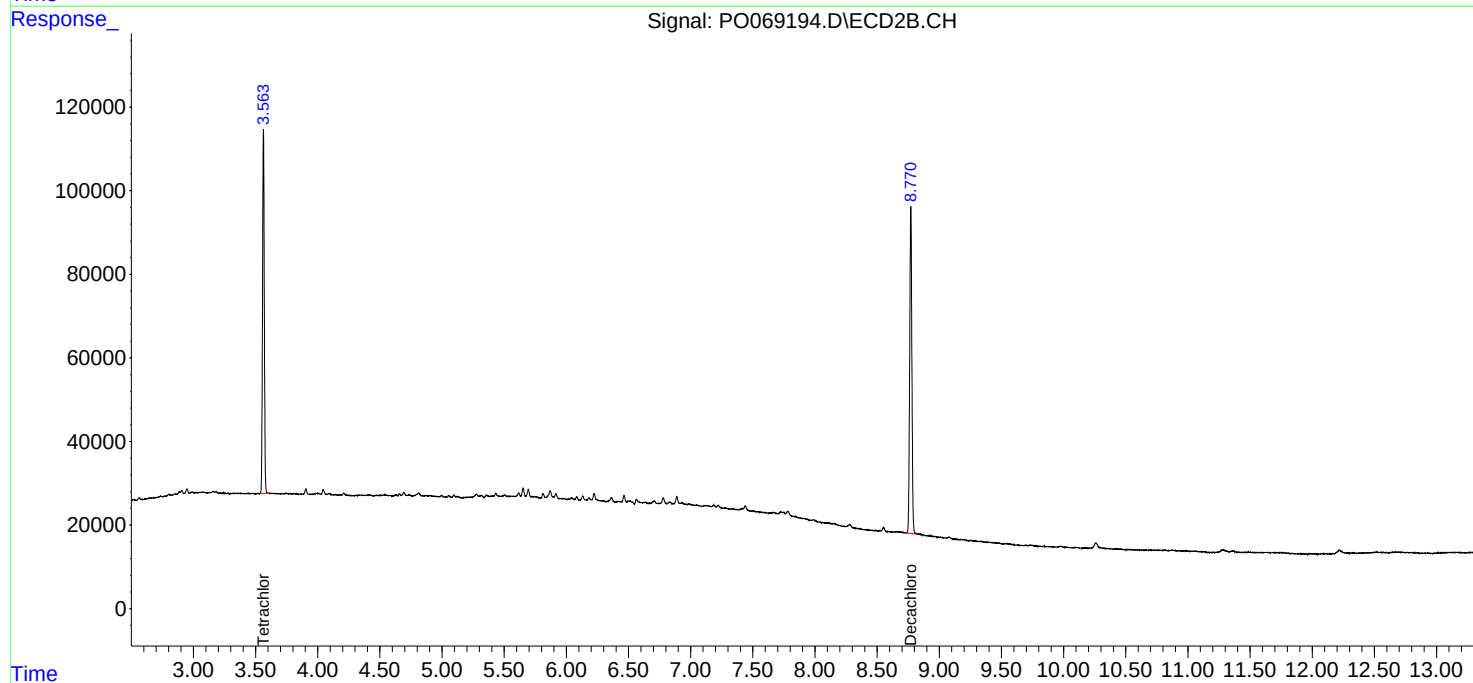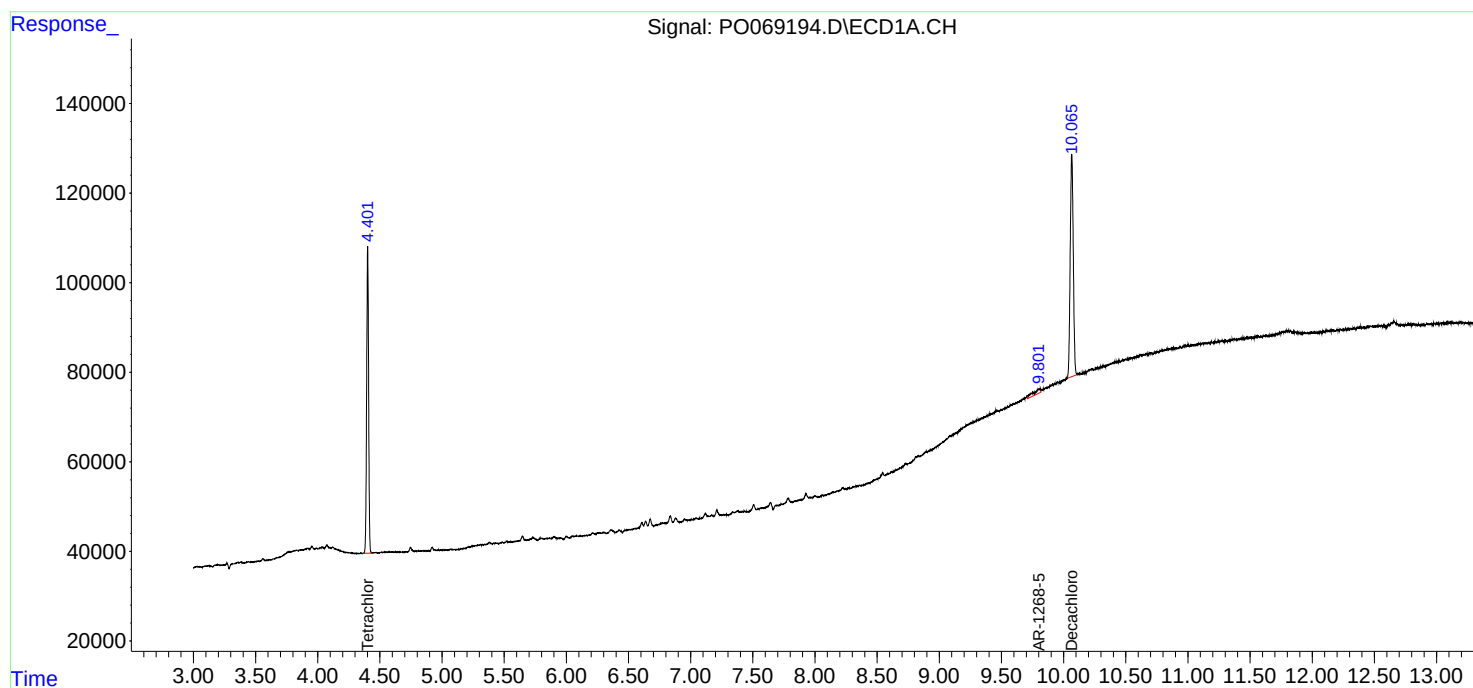


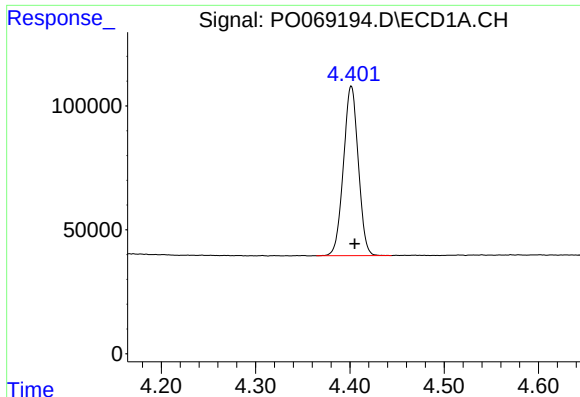

#1 Tetrachloro-m-xylene


R.T.: 4.402 min
Delta R.T.: -0.003 min
Response: 746845
Conc: 25.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUCT-BANK

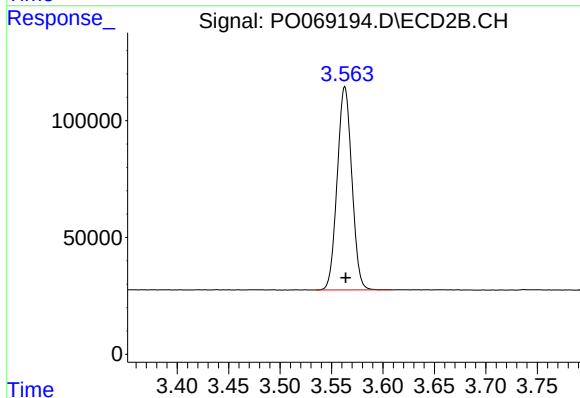


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.001 min
Response: 861362
Conc: 22.38 ng/ml

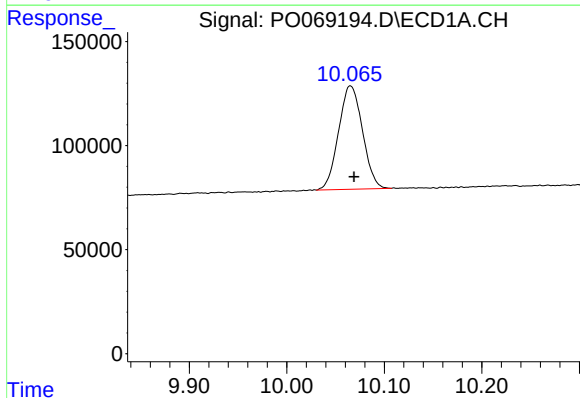


#2 Decachlorobiphenyl

R.T.: 10.065 min
Delta R.T.: -0.004 min
Response: 846690
Conc: 17.83 ng/ml

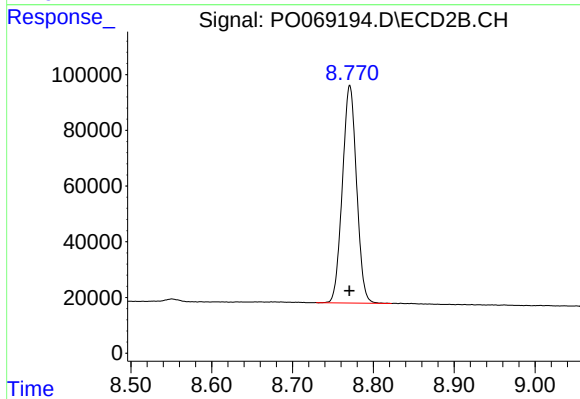

#2 Decachlorobiphenyl


R.T.: 8.771 min
Delta R.T.: 0.000 min
Response: 953895
Conc: 17.52 ng/ml

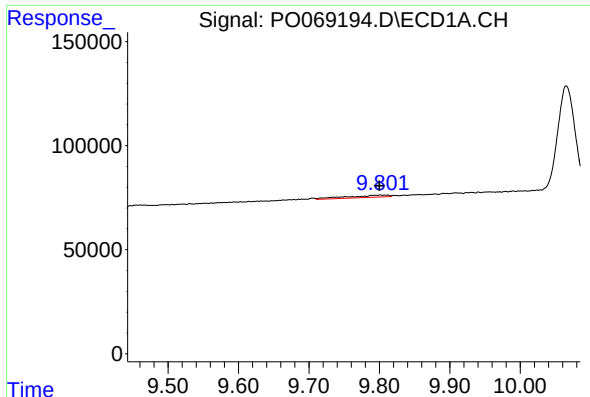

#45 AR-1268-5

R.T.: 9.801 min
Delta R.T.: 0.001 min
Response: 43341
Conc: 2.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUCT-BANK

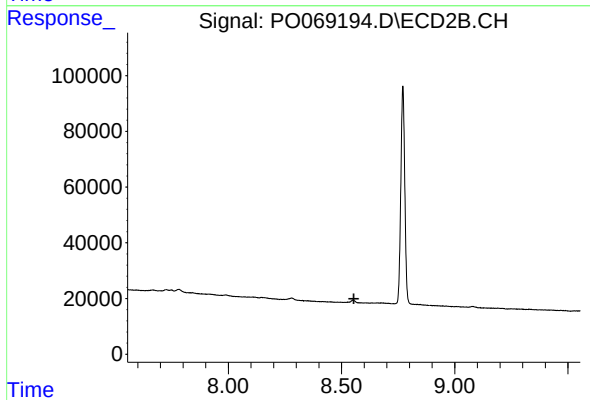

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.554 min
Response: 0
Conc: N.D.