Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062520\
Data File : PO069213.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2020 18:46
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:09:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
	System Monitoring Compounds							
1)	SA Tetrachlo...	4.402	3.564	638281	751701	21.576	19.530	
2)	SA Decachlor...	10.066	8.771	803772	873796	16.923	16.052	
	Target Compounds							
20)	L4 AR-1242-5	6.617	5.675	128472	84982	143.974	76.363	#
24)	L5 AR-1248-4	6.617	0.000	128472	0	85.422	N.D.	#
25)	L5 AR-1248-5	6.617	5.675	128472	84982	88.718	58.742	#
26)	L6 AR-1254-1	6.617	5.675	128472	84982	84.802	36.146	#
32)	L7 AR-1260-2	7.595	0.000	182338	0	77.905	N.D.	#
45)	L9 AR-1268-5	9.798	0.000	18986	0	1.121	N.D.	#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062520\
Data File : PO069213.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2020 18:46
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument : ECD_O
ClientSampleId : I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:09:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

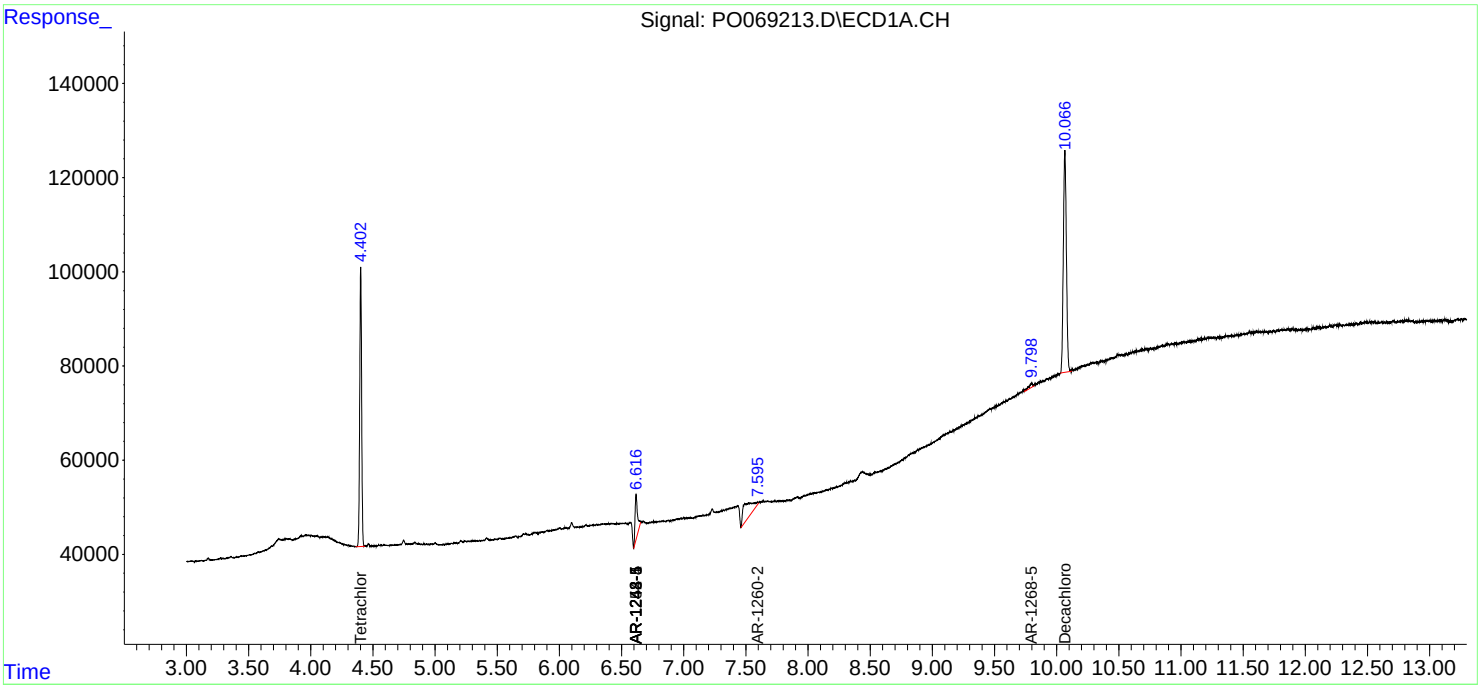

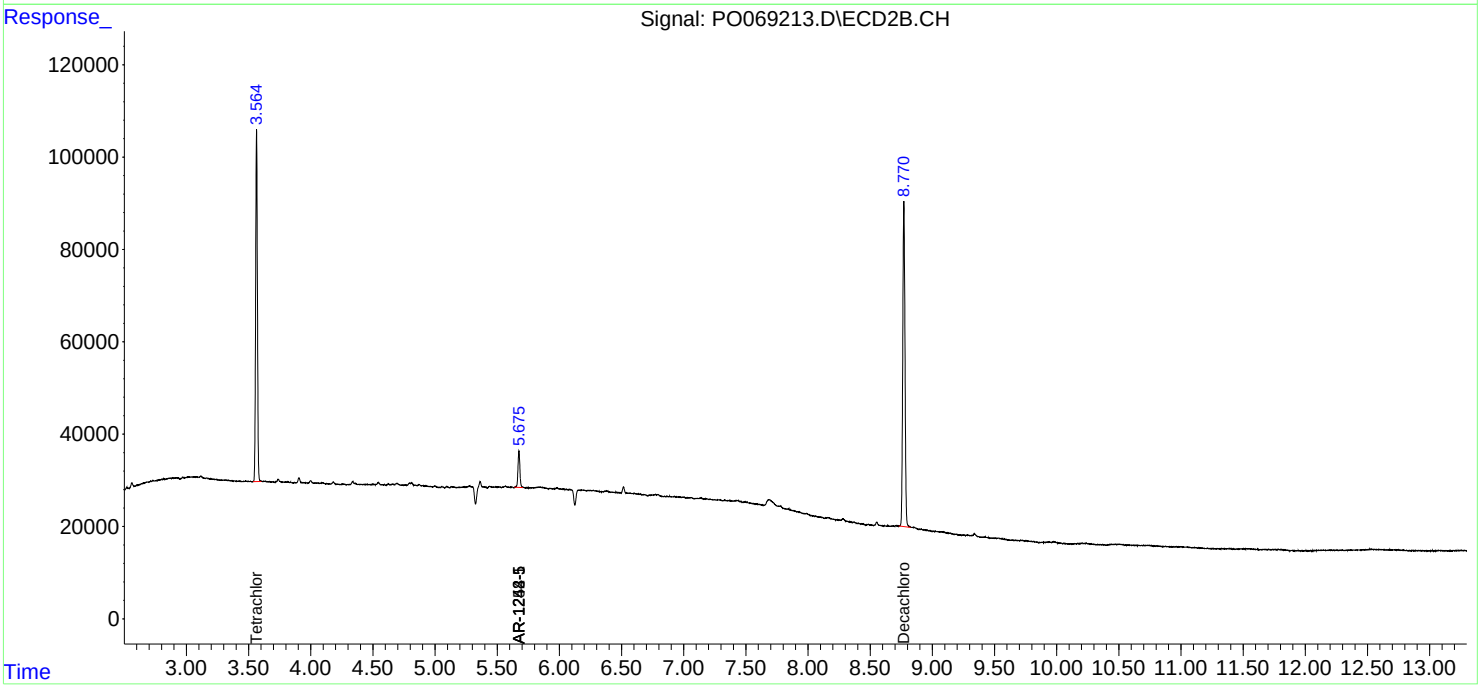

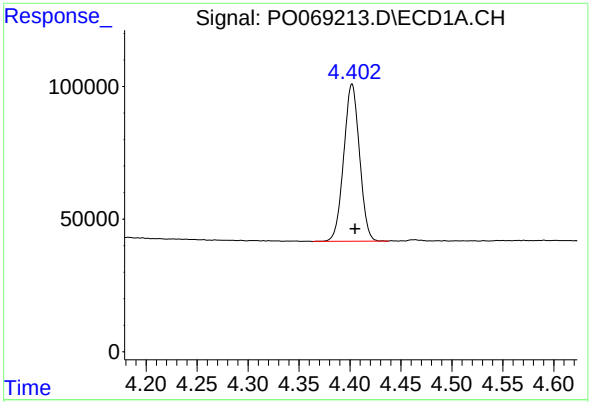

#1 Tetrachloro-m-xylene

R.T.: 4.402 min
Delta R.T.: -0.003 min
Response: 638281
Conc: 21.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

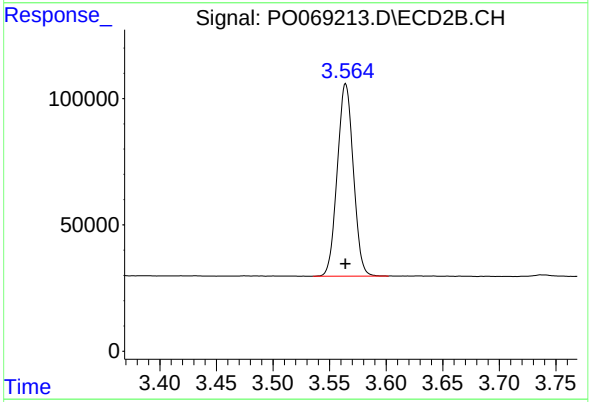

#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 751701
Conc: 19.53 ng/ml

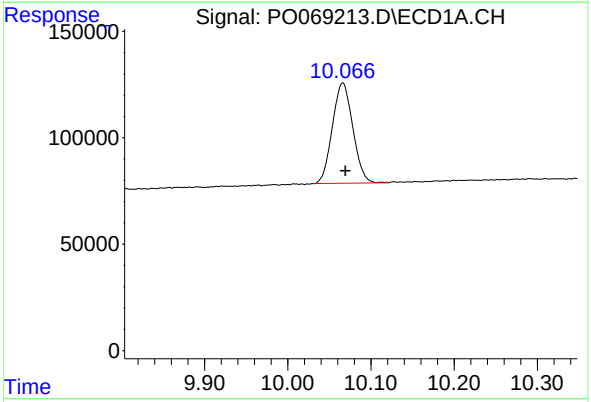

#2 Decachlorobiphenyl

R.T.: 10.066 min
Delta R.T.: -0.003 min
Response: 803772
Conc: 16.92 ng/ml

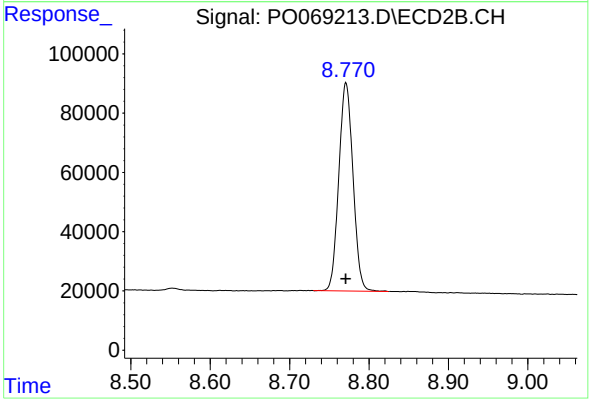

#2 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: 0.000 min
Response: 873796
Conc: 16.05 ng/ml

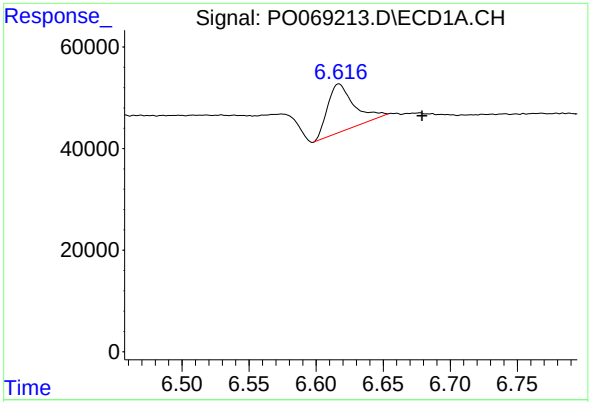

#20 AR-1242-5

R.T.: 6.617 min
Delta R.T.: -0.062 min
Response: 128472
Conc: 143.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

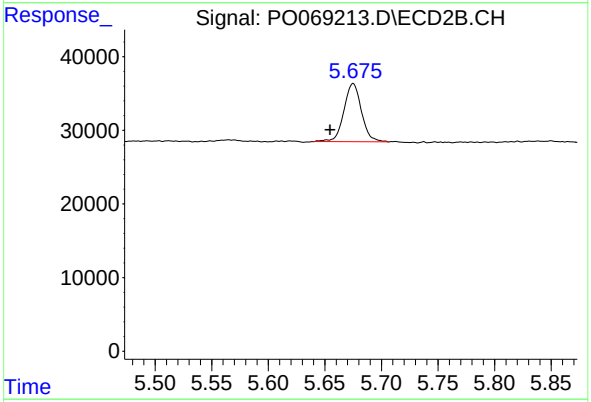

#20 AR-1242-5

R.T.: 5.675 min
Delta R.T.: 0.021 min
Response: 84982
Conc: 76.36 ng/ml

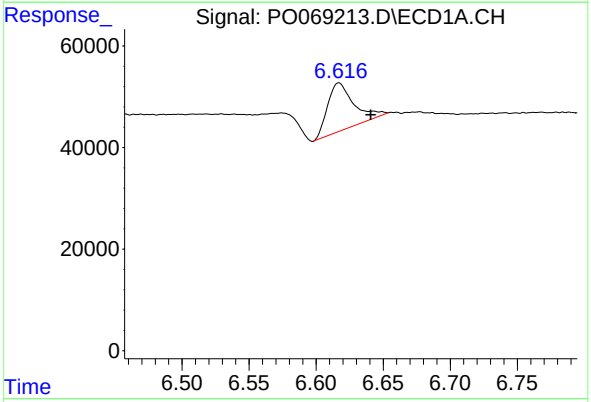

#24 AR-1248-4

R.T.: 6.617 min
Delta R.T.: -0.024 min
Response: 128472
Conc: 85.42 ng/ml

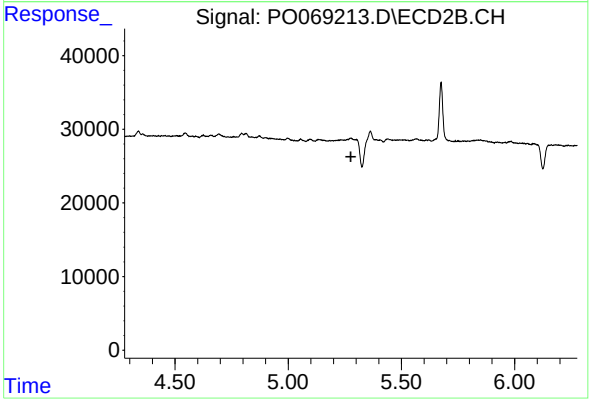

#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

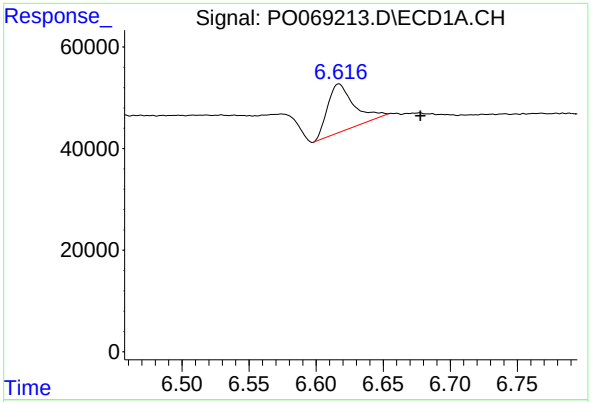

#25 AR-1248-5

R.T.: 6.617 min
Delta R.T.: -0.061 min
Response: 128472
Conc: 88.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

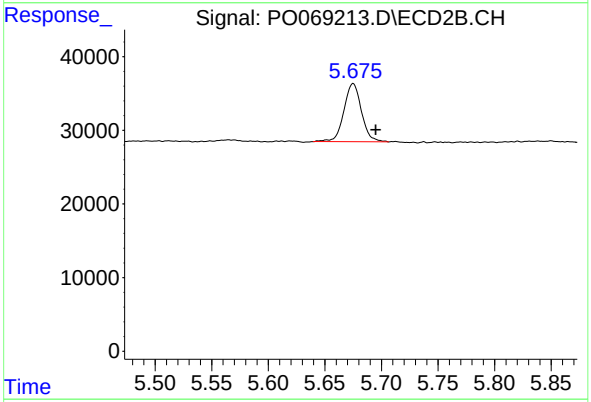

#25 AR-1248-5

R.T.: 5.675 min
Delta R.T.: -0.020 min
Response: 84982
Conc: 58.74 ng/ml

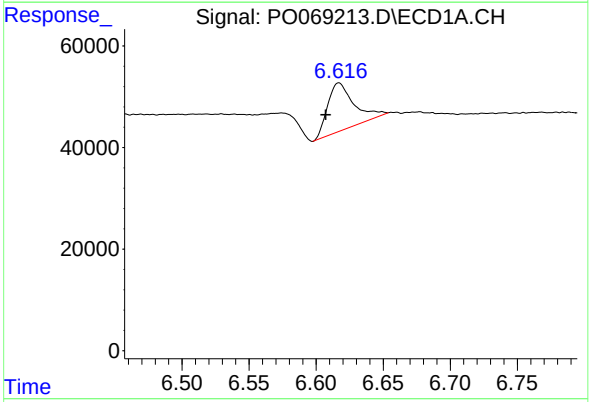

#26 AR-1254-1

R.T.: 6.617 min
Delta R.T.: 0.010 min
Response: 128472
Conc: 84.80 ng/ml

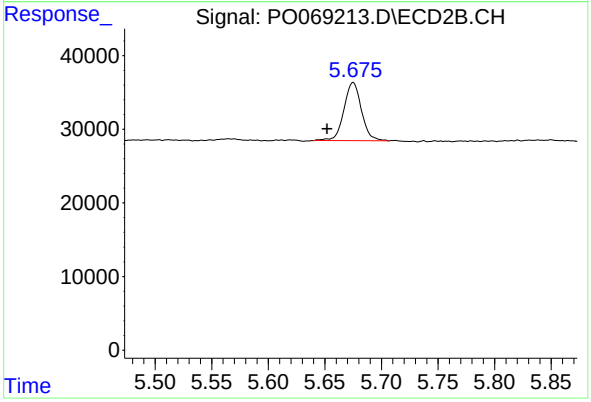

#26 AR-1254-1

R.T.: 5.675 min
Delta R.T.: 0.023 min
Response: 84982
Conc: 36.15 ng/ml

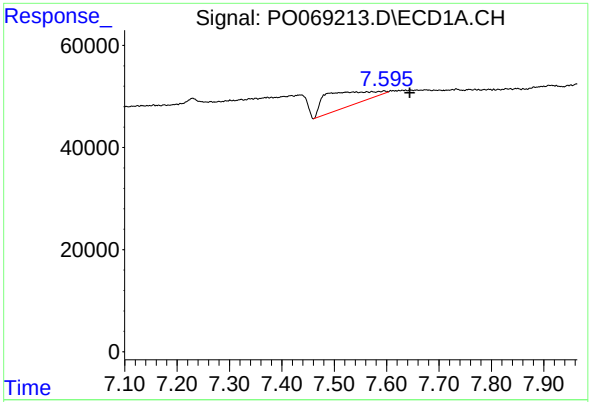

#32 AR-1260-2

R.T.: 7.595 min
Delta R.T.: -0.049 min
Response: 182338
Conc: 77.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

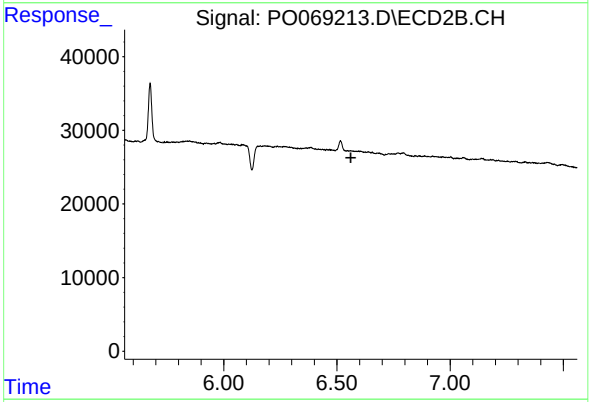

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.562 min
Response: 0
Conc: N.D.

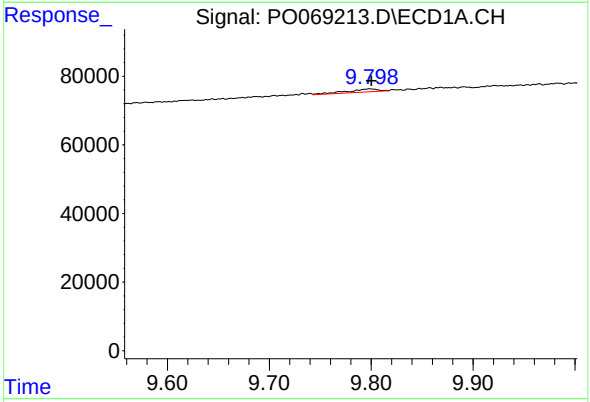

#45 AR-1268-5

R.T.: 9.798 min
Delta R.T.: -0.002 min
Response: 18986
Conc: 1.12 ng/ml

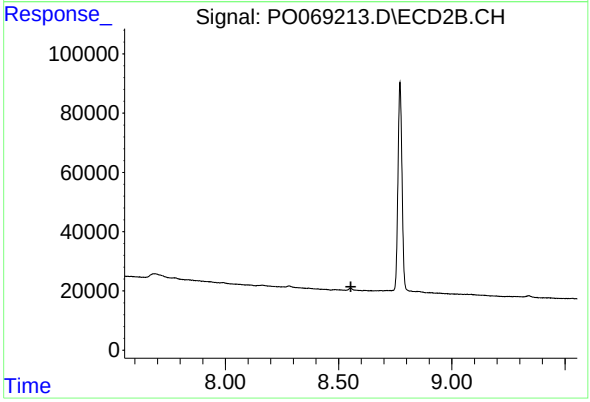

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.554 min
Response: 0
Conc: N.D.