

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062520\
 Data File : P0069205.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2020 16:29
 Operator : DD\AJ
 Sample : L3085-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 31063

Manual Integrations
 APPROVED

Ankita
 6/26/2020 8:53:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 16:51:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 19 05:15:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.401	3.564	630028	720791	21.297	18.727
2) SA Decachlor...	10.065	8.770	865134	925922	18.215	17.009
Target Compounds						
26) L6 AR-1254-1	6.603	5.651	126751	188858	83.666m	80.328
27) L6 AR-1254-2	6.833	5.812	186799	124335	77.881	58.953m
28) L6 AR-1254-3	7.210	6.224	226109	242707	85.165	70.388
29) L6 AR-1254-4	7.506	6.464	99236	90202	46.535	38.681
30) L6 AR-1254-5	7.929	6.889	105864	130966	47.229	40.451

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062520\
Data File : PO069205.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2020 16:29
Operator : DD\AJ
Sample : L3085-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
31063


Manual Integrations
APPROVED

Ankita
6/26/2020 8:53:06 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 16:51:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

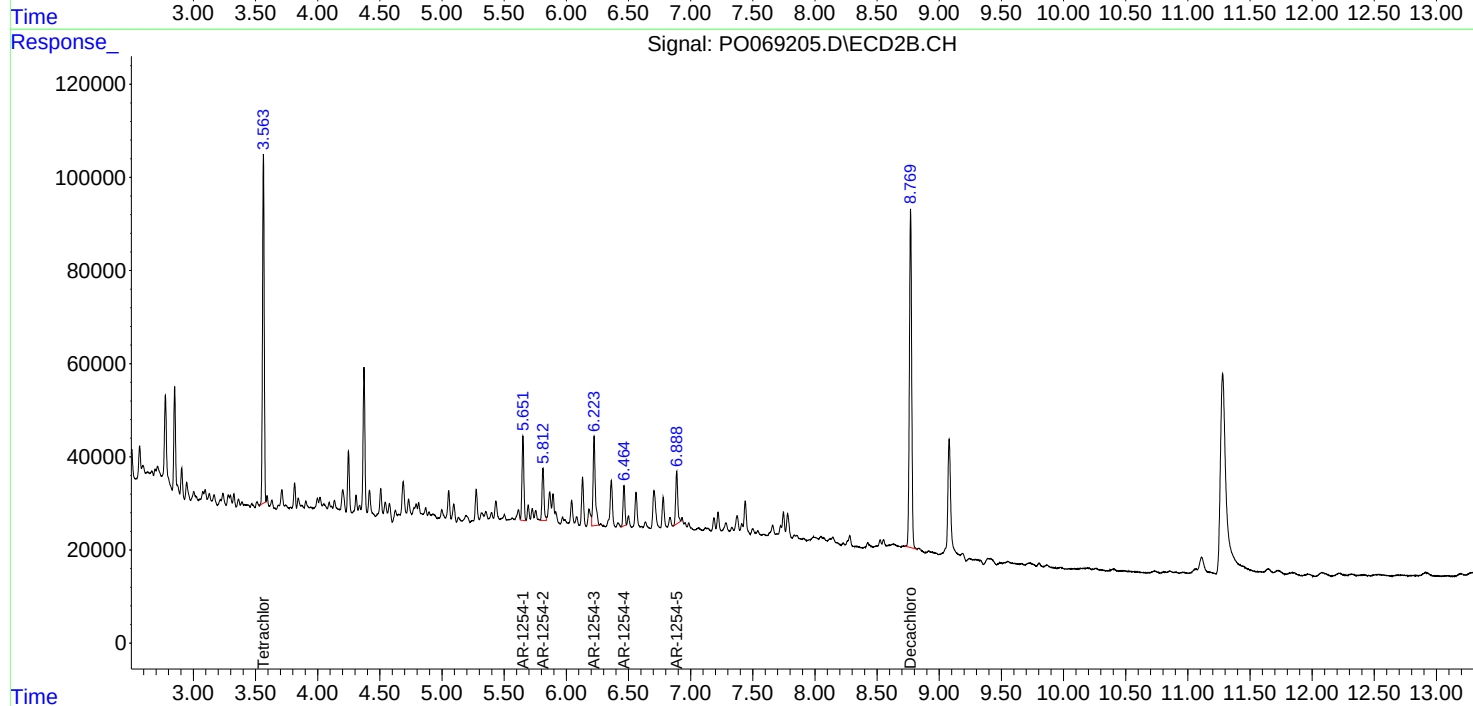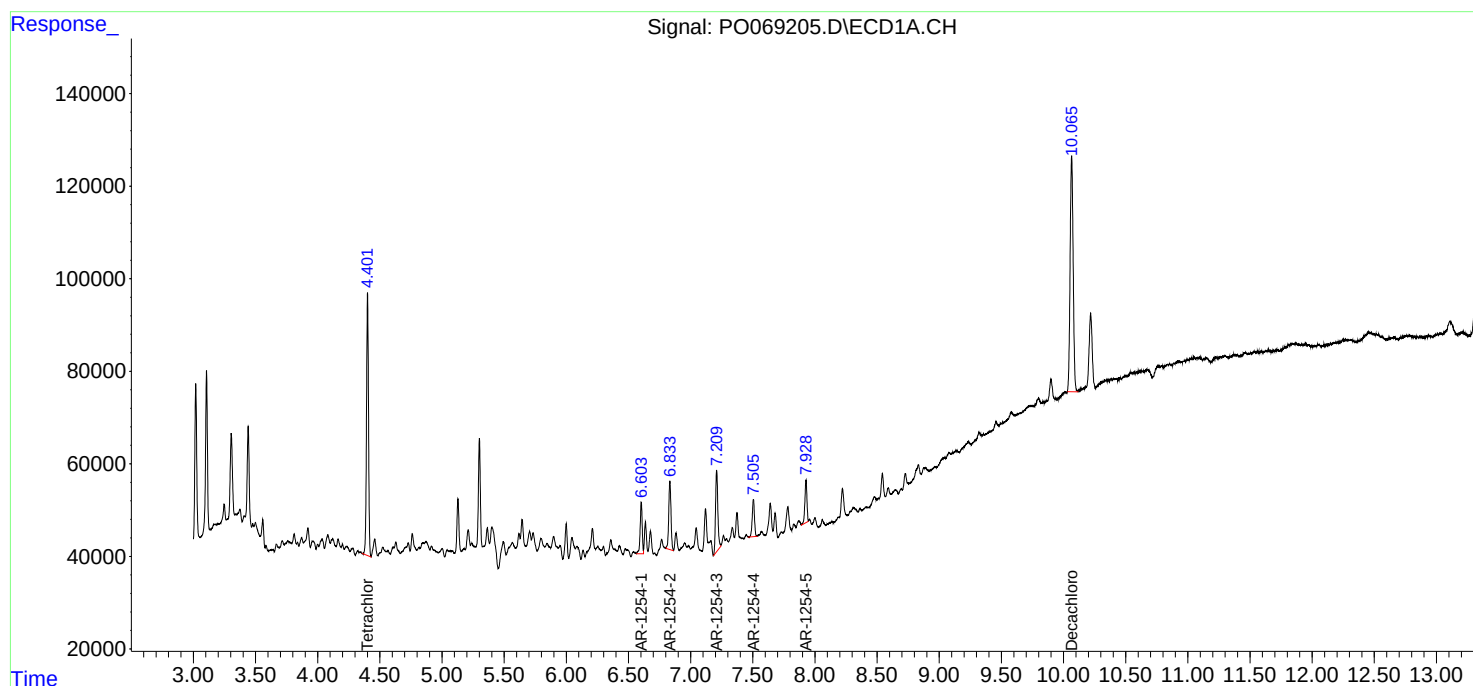

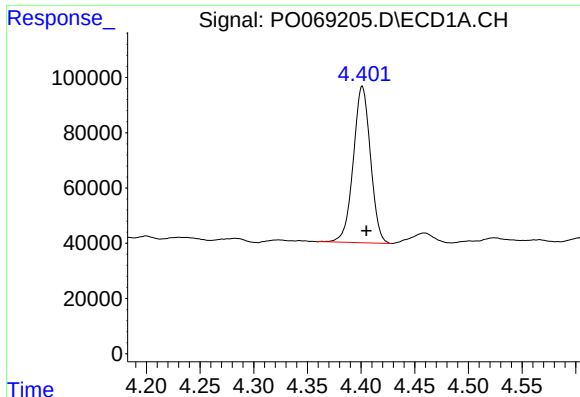


#1 Tetrachloro-m-xylene

R.T.: 4.401 min
Delta R.T.: -0.004 min
Response: 630028
Conc: 21.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
31063


Manual Integrations
APPROVED

Ankita
6/26/2020 8:53:06 AM

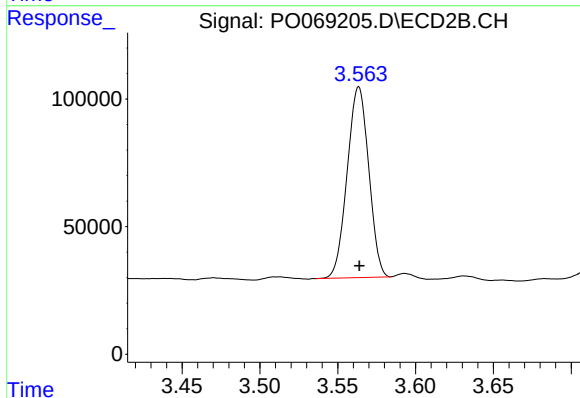


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 720791
Conc: 18.73 ng/ml

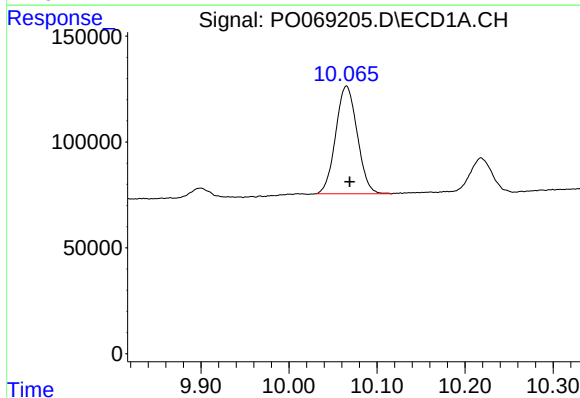


#2 Decachlorobiphenyl

R.T.: 10.065 min
Delta R.T.: -0.004 min
Response: 865134
Conc: 18.21 ng/ml

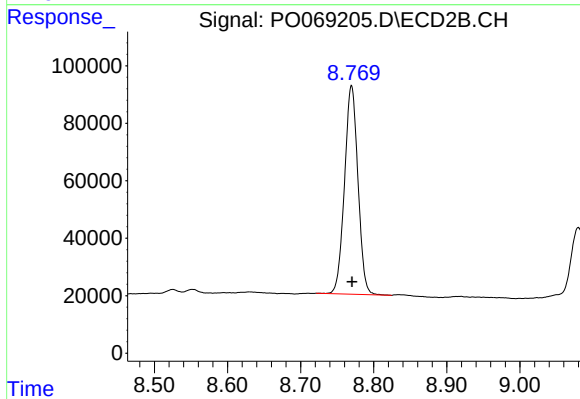

#2 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: 0.000 min
Response: 925922
Conc: 17.01 ng/ml

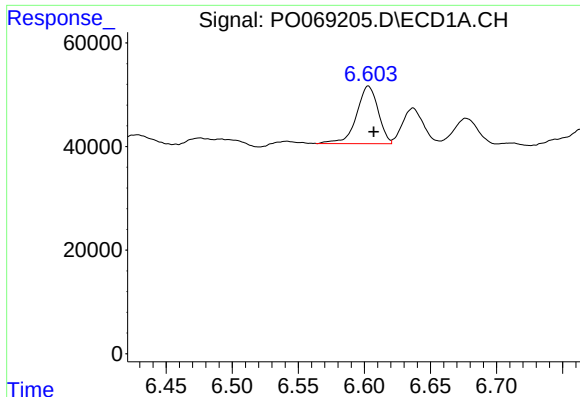


#26 AR-1254-1

R.T.: 6.603 min
Delta R.T.: -0.005 min
Response: 126751
Conc: 83.67 ng/ml m

Instrument :
ECD_O
ClientSampleId :
31063


Manual Integrations
APPROVED

Ankita
6/26/2020 8:53:06 AM

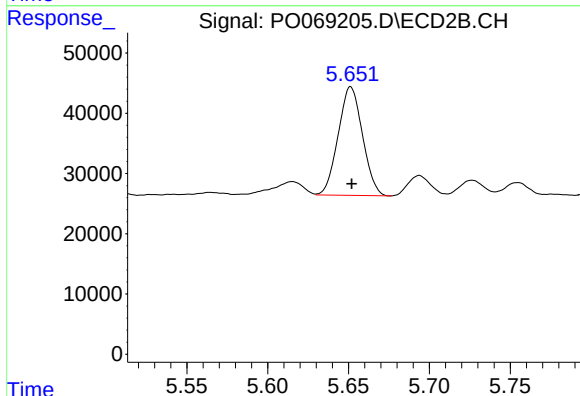


#26 AR-1254-1

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 188858
Conc: 80.33 ng/ml

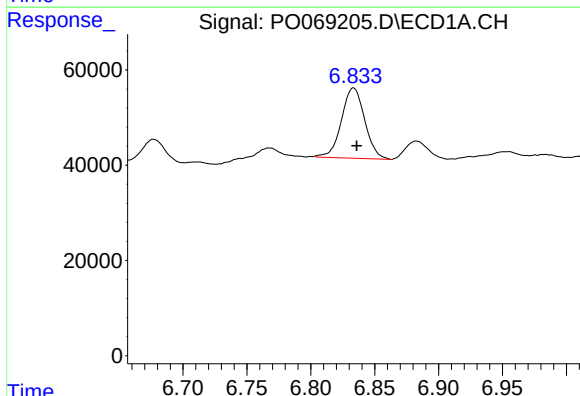


#27 AR-1254-2

R.T.: 6.833 min
Delta R.T.: -0.002 min
Response: 186799
Conc: 77.88 ng/ml

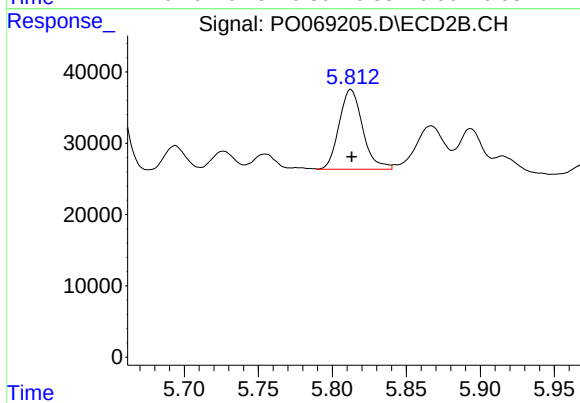

#27 AR-1254-2

R.T.: 5.812 min
Delta R.T.: 0.000 min
Response: 124335
Conc: 58.95 ng/ml m

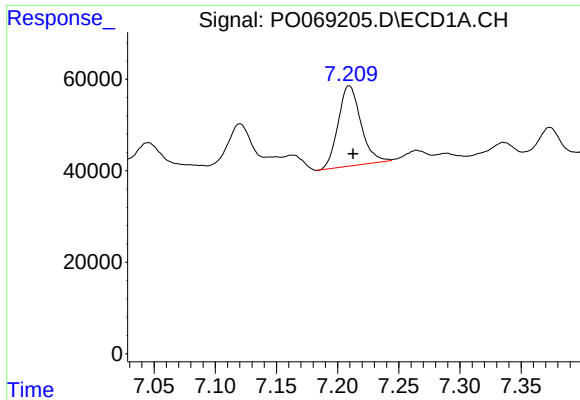


#28 AR-1254-3

R.T.: 7.210 min
Delta R.T.: -0.003 min
Response: 226109
Conc: 85.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
31063


Manual Integrations
APPROVED

Ankita
6/26/2020 8:53:06 AM

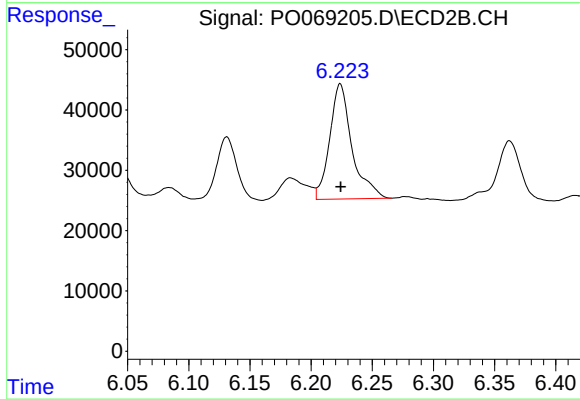


#28 AR-1254-3

R.T.: 6.224 min
Delta R.T.: 0.000 min
Response: 242707
Conc: 70.39 ng/ml

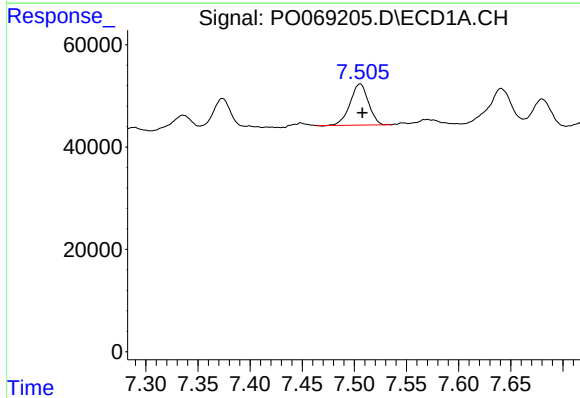


#29 AR-1254-4

R.T.: 7.506 min
Delta R.T.: -0.002 min
Response: 99236
Conc: 46.54 ng/ml

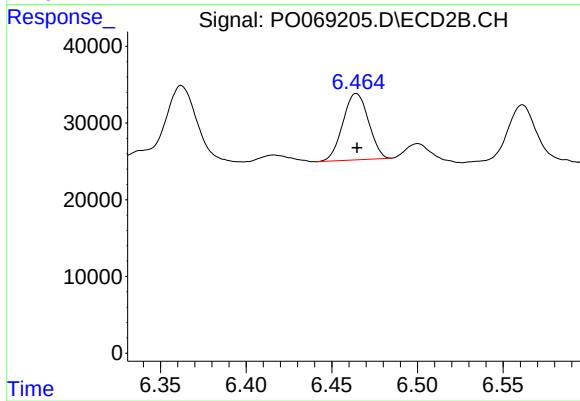

#29 AR-1254-4

R.T.: 6.464 min
Delta R.T.: 0.000 min
Response: 90202
Conc: 38.68 ng/ml

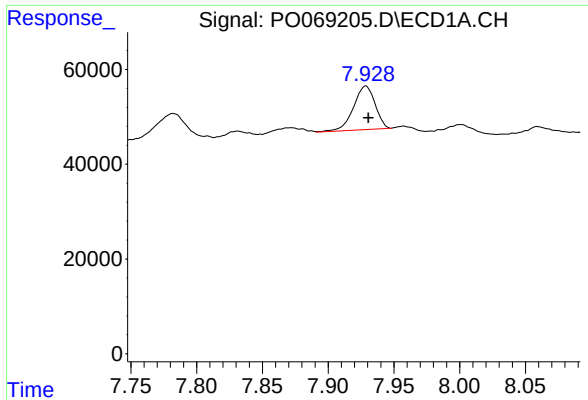


#30 AR-1254-5

R.T.: 7.929 min
Delta R.T.: -0.002 min
Response: 105864
Conc: 47.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
31063

Manual Integrations
APPROVED

Ankita
6/26/2020 8:53:06 AM

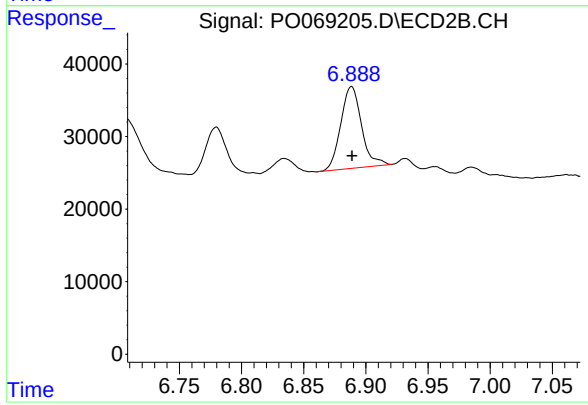

#30 AR-1254-5

R.T.: 6.889 min
Delta R.T.: 0.000 min
Response: 130966
Conc: 40.45 ng/ml