

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062520\
 Data File : P0069206.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2020 16:46
 Operator : DD\AJ
 Sample : L3085-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 31064

Manual Integrations
 APPROVED

Ankita
 6/26/2020 8:53:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 17:46:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 19 05:15:02 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.400	3.563	423303	464823	14.309m	12.077m
2)	SA Decachlor...	10.065	8.770	508387	574104	10.704	10.546
Target Compounds							
26)	L6 AR-1254-1	6.602	5.651	93304	139507	61.588m	59.337
27)	L6 AR-1254-2	6.833	5.812	133587	105998	55.696	50.259
28)	L6 AR-1254-3	7.210	6.224	155610	174451	58.611	50.593
29)	L6 AR-1254-4	7.504	6.464	74121	73355	34.758m	31.457m
30)	L6 AR-1254-5	7.928	6.887	70354	98452	31.387m	30.408

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062520\
Data File : PO069206.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2020 16:46
Operator : DD\AJ
Sample : L3085-02
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
31064


Manual Integrations
APPROVED

Ankita
6/26/2020 8:53:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 17:46:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 19 05:15:02 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

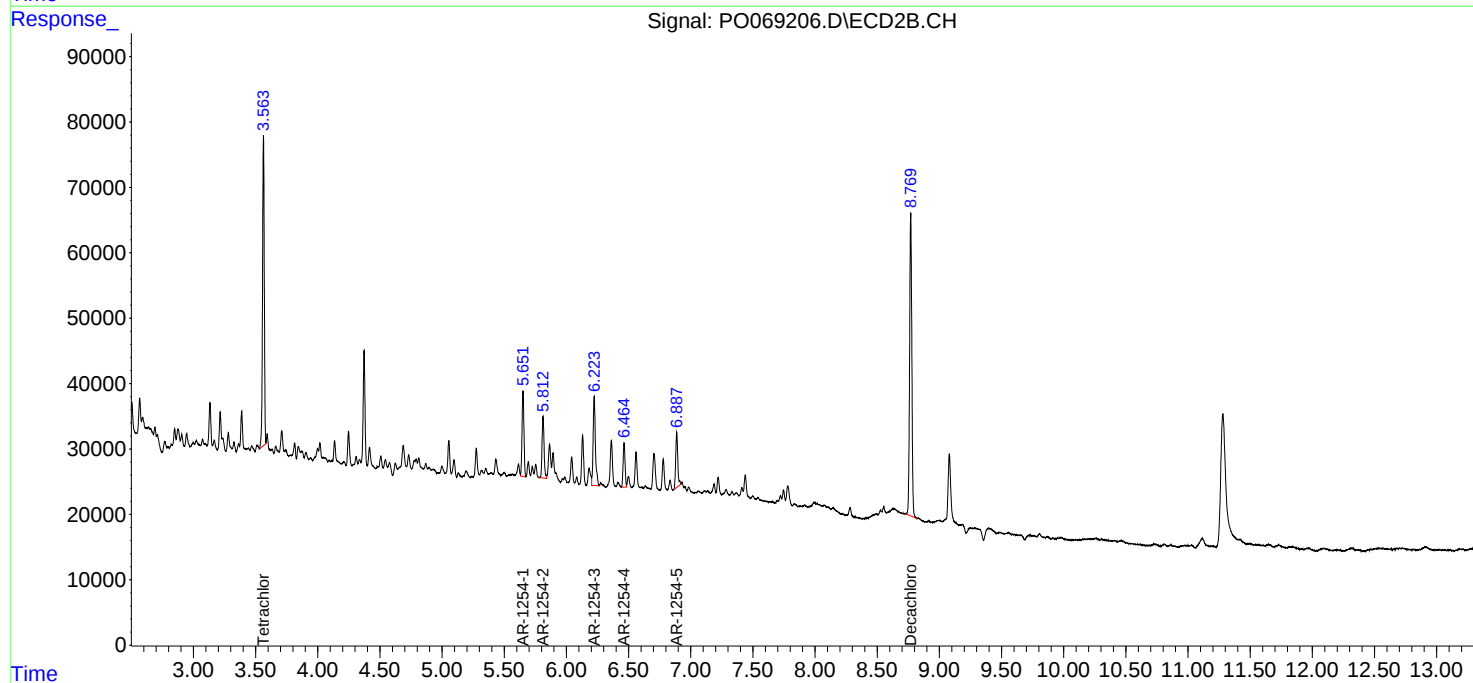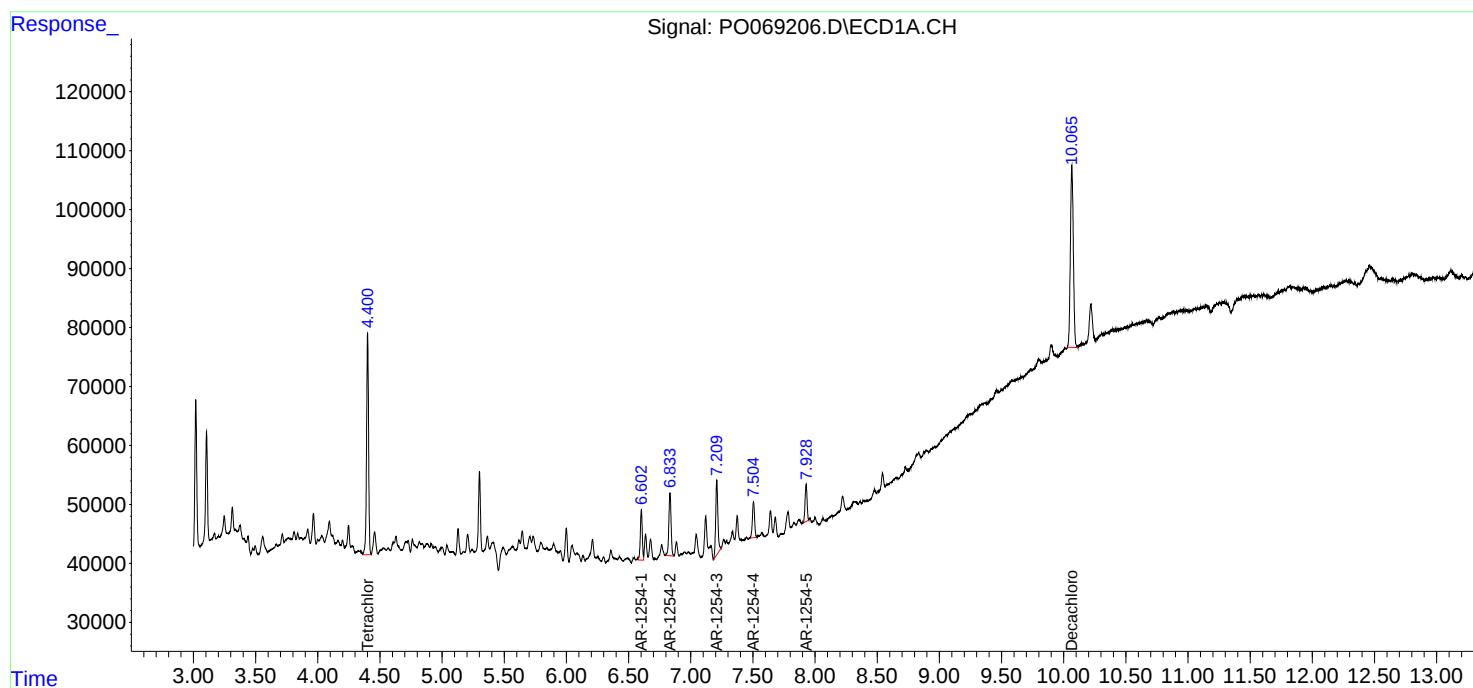

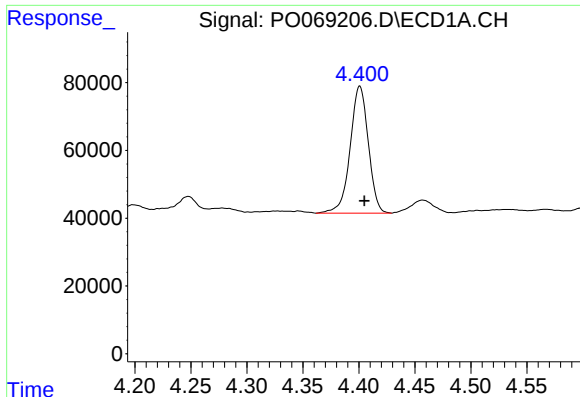


#1 Tetrachloro-m-xylene

R.T.: 4.400 min
Delta R.T.: -0.005 min
Response: 423303
Conc: 14.31 ng/ml m

Instrument :
ECD_O
ClientSampleId :
31064


Manual Integrations
APPROVED

Ankita
6/26/2020 8:53:08 AM

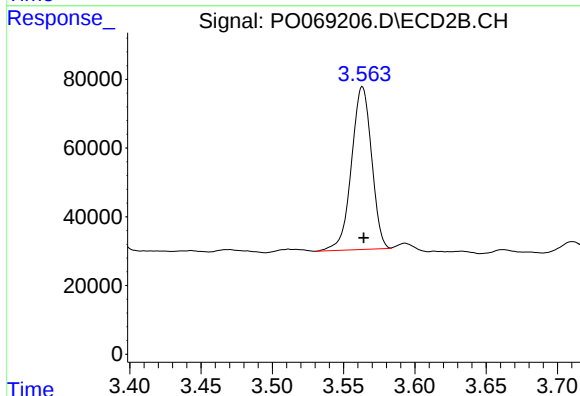


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.001 min
Response: 464823
Conc: 12.08 ng/ml m

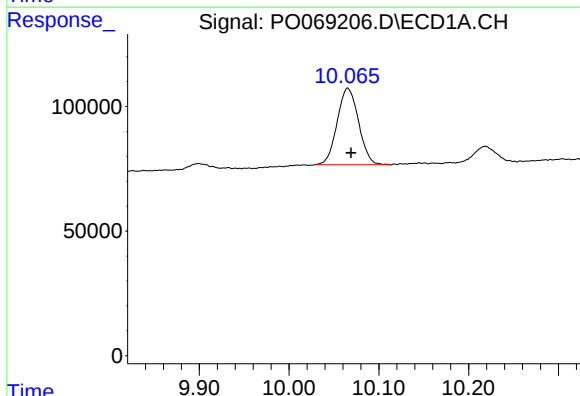


#2 Decachlorobiphenyl

R.T.: 10.065 min
Delta R.T.: -0.004 min
Response: 508387
Conc: 10.70 ng/ml

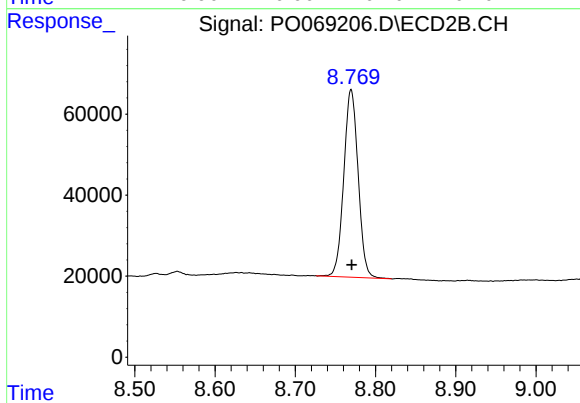

#2 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: 0.000 min
Response: 574104
Conc: 10.55 ng/ml

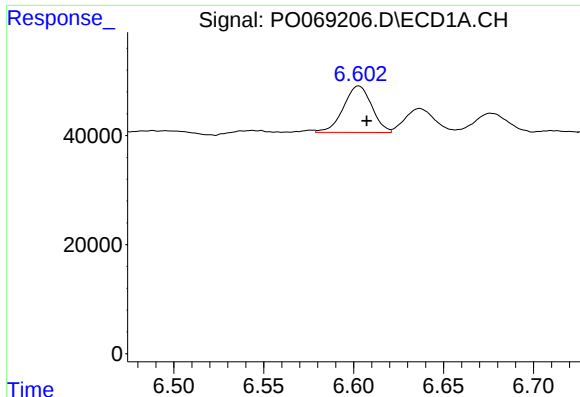


#26 AR-1254-1

R.T.: 6.602 min
Delta R.T.: -0.005 min
Response: 93304
Conc: 61.59 ng/ml m

Instrument :
ECD_O
ClientSampleId :
31064


Manual Integrations
APPROVED

Ankita
6/26/2020 8:53:08 AM

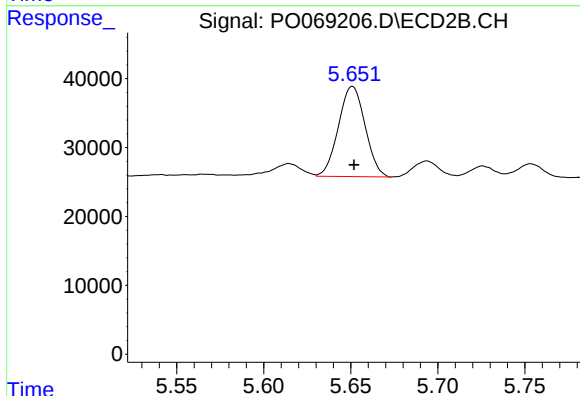


#26 AR-1254-1

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 139507
Conc: 59.34 ng/ml

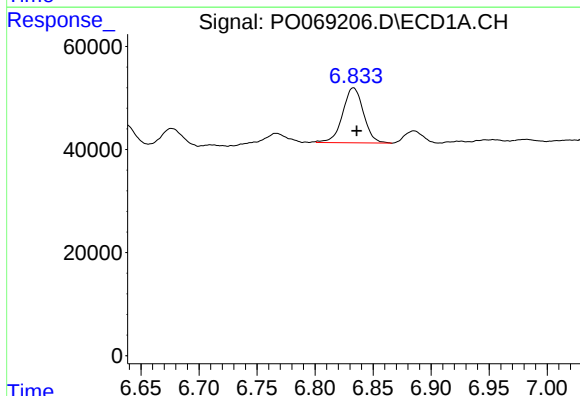


#27 AR-1254-2

R.T.: 6.833 min
Delta R.T.: -0.003 min
Response: 133587
Conc: 55.70 ng/ml

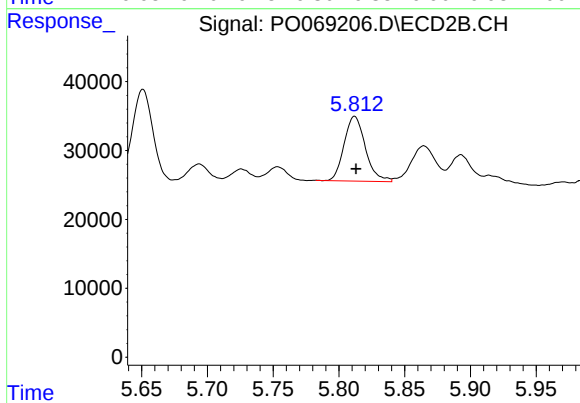

#27 AR-1254-2

R.T.: 5.812 min
Delta R.T.: -0.001 min
Response: 105998
Conc: 50.26 ng/ml

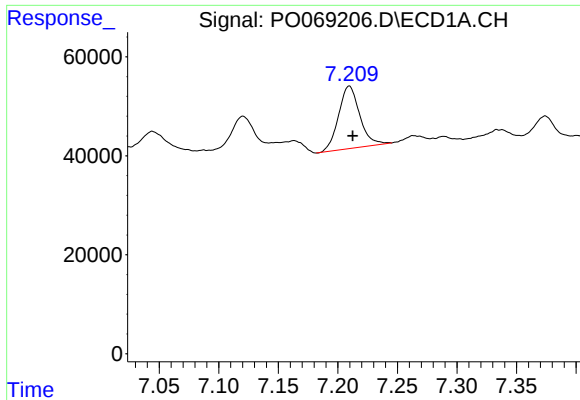


#28 AR-1254-3

R.T.: 7.210 min
Delta R.T.: -0.003 min
Response: 155610
Conc: 58.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
31064


Manual Integrations
APPROVED

Ankita
6/26/2020 8:53:08 AM

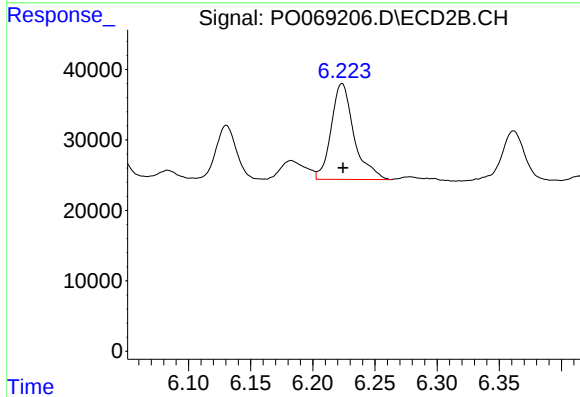


#28 AR-1254-3

R.T.: 6.224 min
Delta R.T.: 0.000 min
Response: 174451
Conc: 50.59 ng/ml

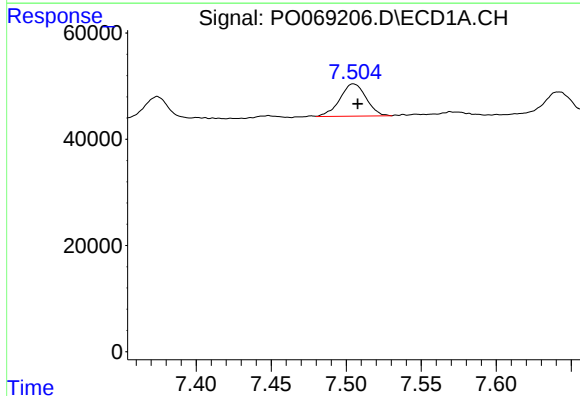


#29 AR-1254-4

R.T.: 7.504 min
Delta R.T.: -0.004 min
Response: 74121
Conc: 34.76 ng/ml m

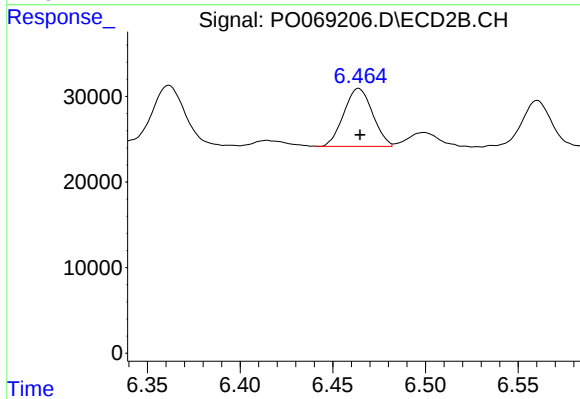

#29 AR-1254-4

R.T.: 6.464 min
Delta R.T.: -0.001 min
Response: 73355
Conc: 31.46 ng/ml m

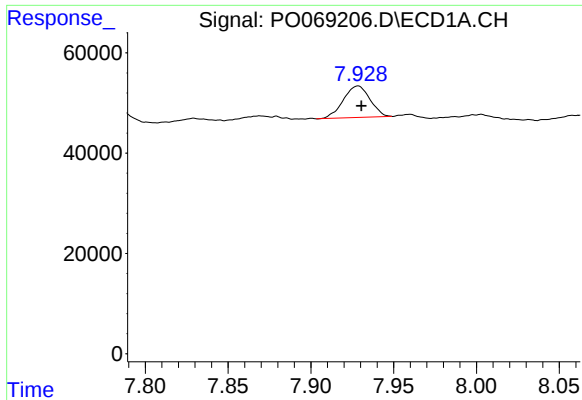


#30 AR-1254-5

R.T.: 7.928 min
Delta R.T.: -0.002 min
Response: 70354
Conc: 31.39 ng/ml m

Instrument :
ECD_O
ClientSampleId :
31064

Manual Integrations
APPROVED

Ankita
6/26/2020 8:53:08 AM

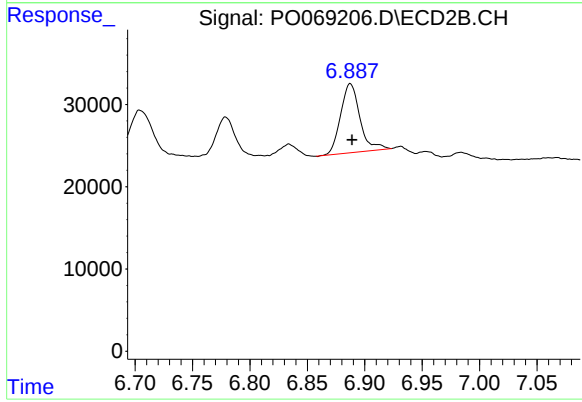

#30 AR-1254-5

R.T.: 6.887 min
Delta R.T.: -0.001 min
Response: 98452
Conc: 30.41 ng/ml