

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062521\
 Data File : P0079172.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2021 22:00
 Operator : DD\AJ
 Sample : PB137333BS
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:31:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.323	3.601	1641702	620394	20.801	20.874
2)	SA Decachlor...	9.922	8.776	1216285	576508	19.475	19.347
Target Compounds							
8)	L2 AR-1221-1	4.571	0.000	12281	0	14.772	N.D. #
9)	L2 AR-1221-2	4.666	0.000	20438	0	33.554	N.D. #
28)	L6 AR-1254-3	7.131	0.000	24512	0	5.504	N.D. #
35)	L7 AR-1260-5	8.445	0.000	21929	0	3.424	N.D. #
37)	L8 AR-1262-2	8.445	0.000	21929	0	3.293	N.D. #
39)	L8 AR-1262-4	8.786	0.000	24151	0	6.488	N.D. #
42)	L9 AR-1268-2	8.786f	0.000	24151	0	3.230	N.D. #
43)	L9 AR-1268-3	8.968f	0.000	1291	0	0.202	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062521\
Data File : P0079172.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2021 22:00
Operator : DD\AJ
Sample : PB137333BS
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:31:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

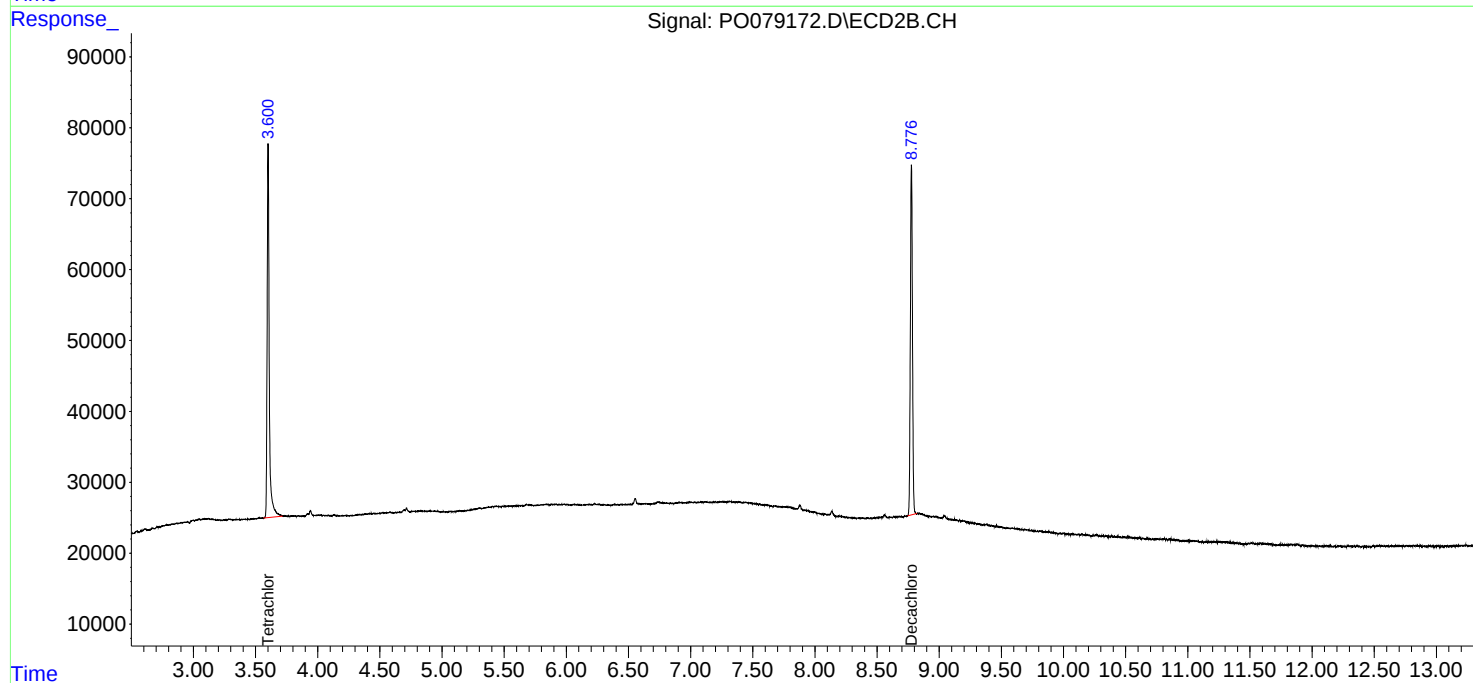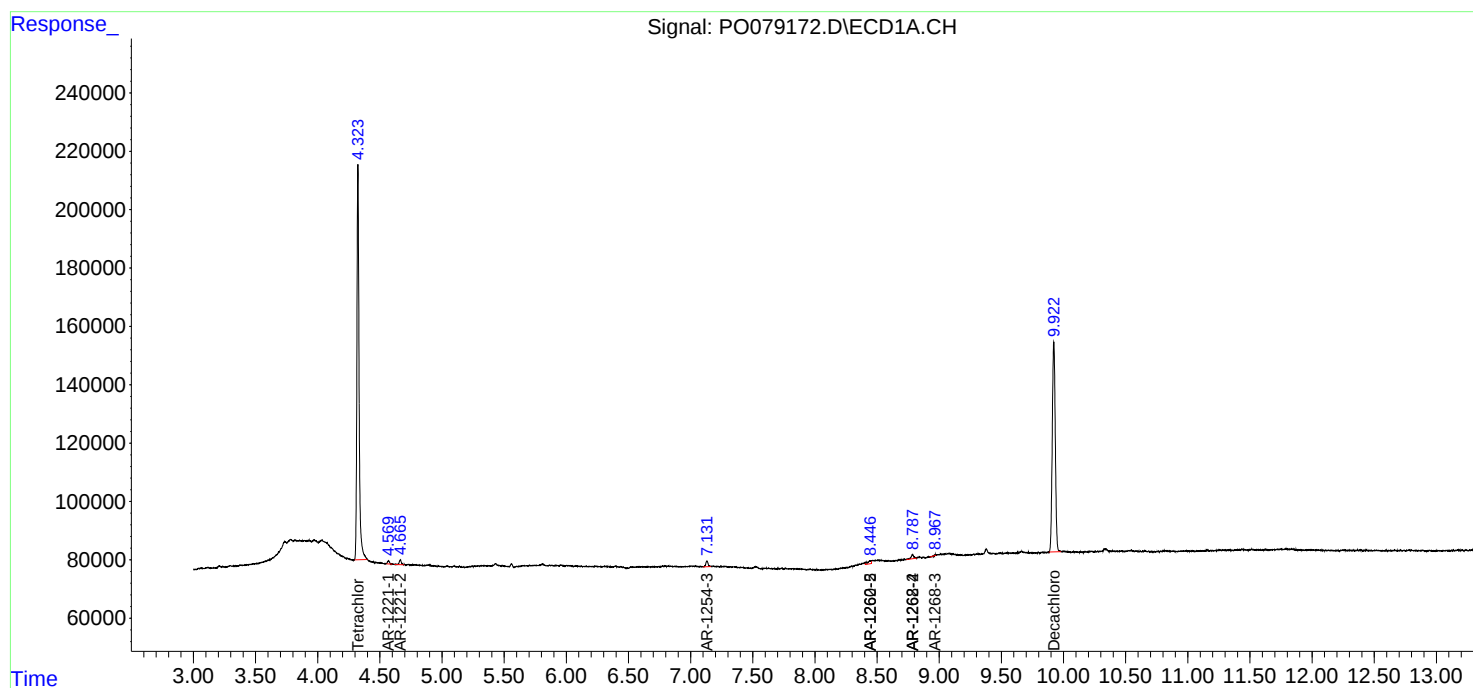


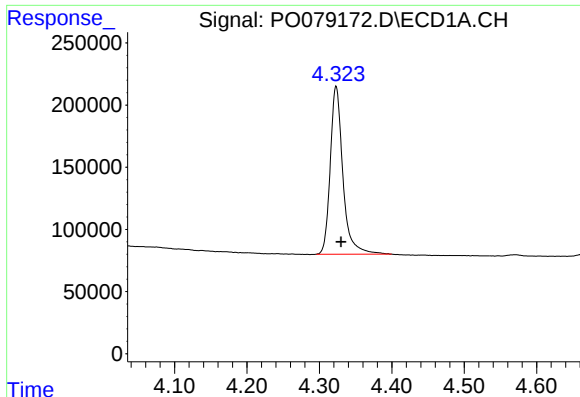

#1 Tetrachloro-m-xylene


R.T.: 4.323 min
Delta R.T.: -0.007 min
Response: 1641702
Conc: 20.80 ng/ml

Instrument :
ECD_O
ClientSampleId :

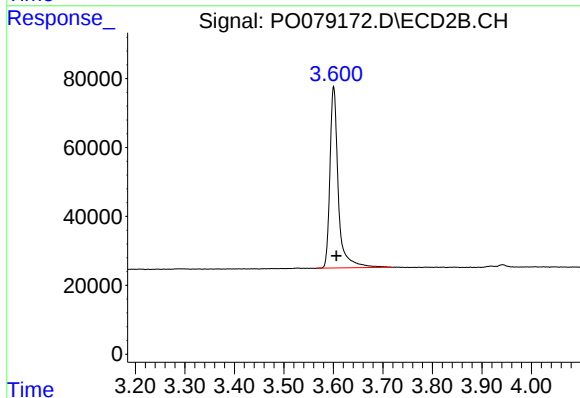


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.006 min
Response: 620394
Conc: 20.87 ng/ml

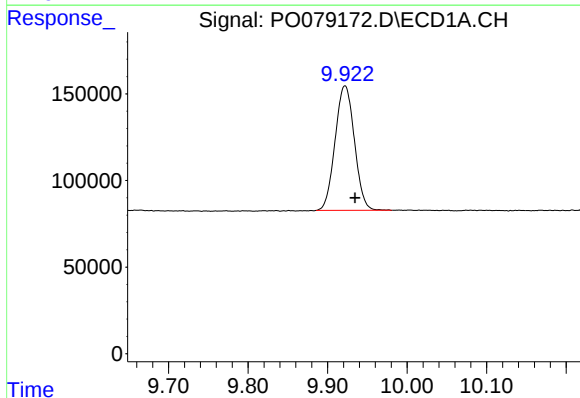


#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: -0.013 min
Response: 1216285
Conc: 19.47 ng/ml

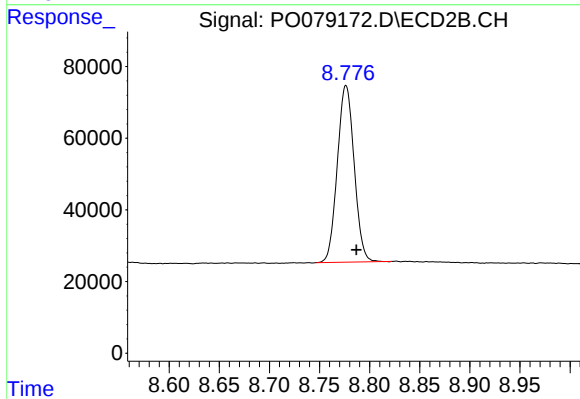

#2 Decachlorobiphenyl


R.T.: 8.776 min
Delta R.T.: -0.010 min
Response: 576508
Conc: 19.35 ng/ml

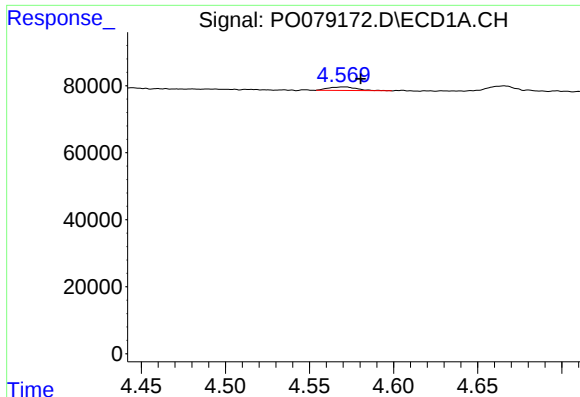

#8 AR-1221-1


R.T.: 4.571 min
Delta R.T.: -0.010 min
Response: 12281
Conc: 14.77 ng/ml

Instrument :
ECD_O
ClientSampleId :

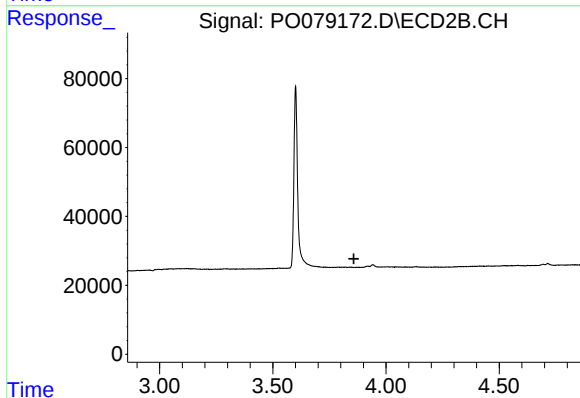


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 3.858 min
Response: 0
Conc: N.D.

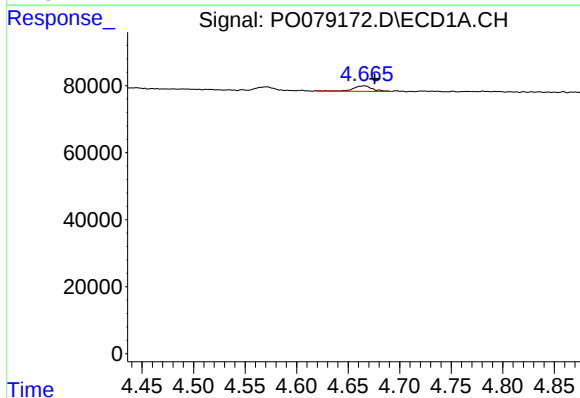


#9 AR-1221-2

R.T.: 4.666 min
Delta R.T.: -0.010 min
Response: 20438
Conc: 33.55 ng/ml

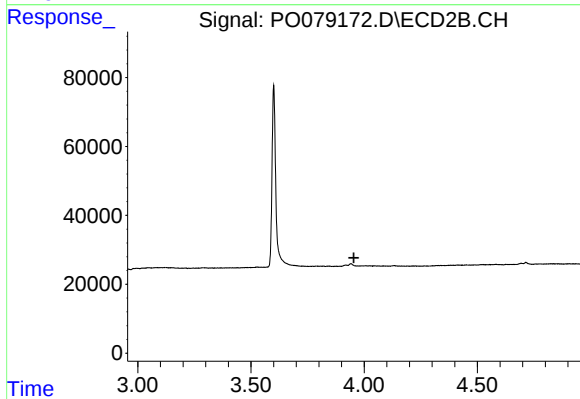

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 3.955 min
Response: 0
Conc: N.D.

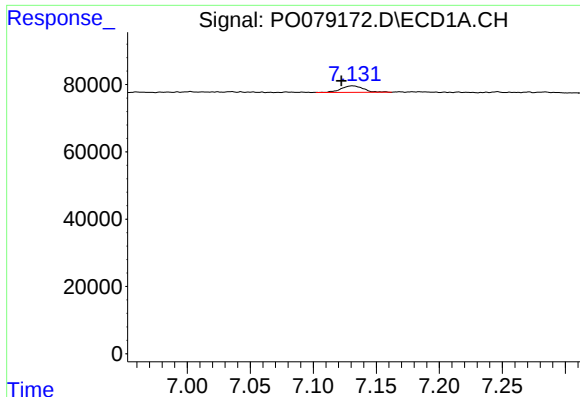

#28 AR-1254-3


R.T.: 7.131 min
Delta R.T.: 0.009 min
Response: 24512
Conc: 5.50 ng/ml

Instrument :
ECD_O
ClientSampleId :

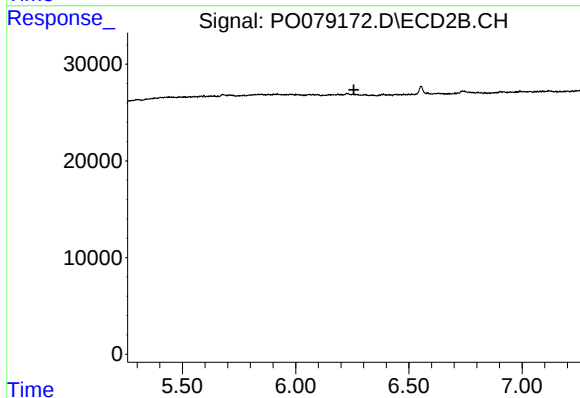


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.257 min
Response: 0
Conc: N.D.

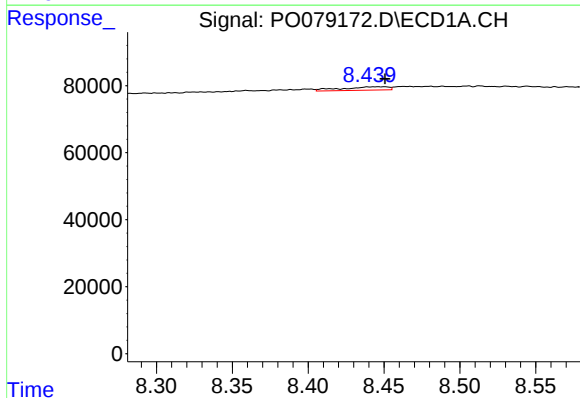


#35 AR-1260-5

R.T.: 8.445 min
Delta R.T.: -0.005 min
Response: 21929
Conc: 3.42 ng/ml

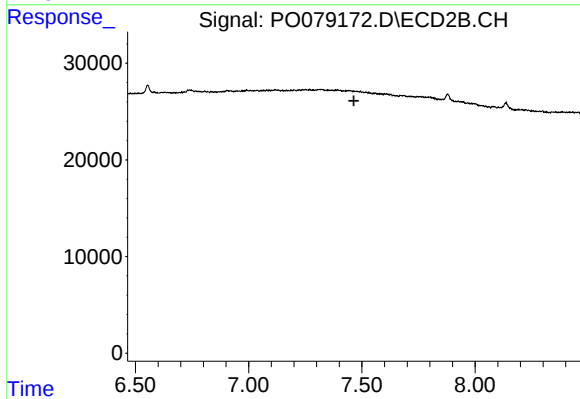

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.465 min
Response: 0
Conc: N.D.

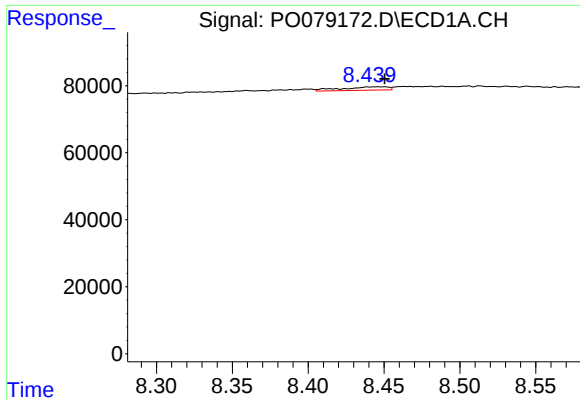

#37 AR-1262-2


R.T.: 8.445 min
Delta R.T.: -0.005 min
Response: 21929
Conc: 3.29 ng/ml

Instrument :
ECD_O
ClientSampleId :

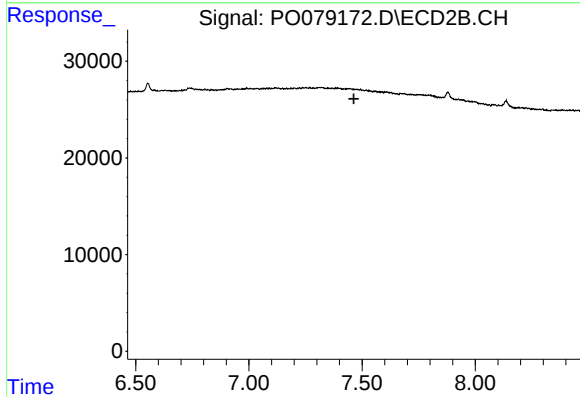


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.464 min
Response: 0
Conc: N.D.

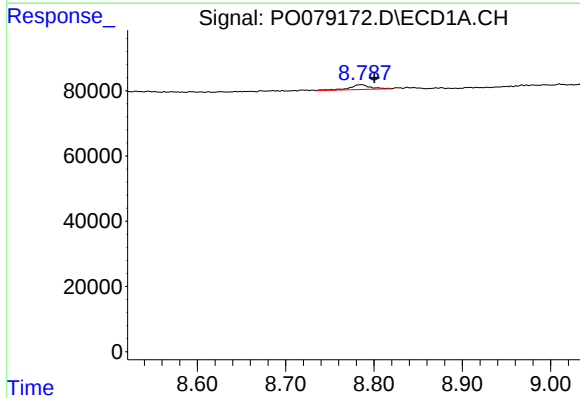


#39 AR-1262-4

R.T.: 8.786 min
Delta R.T.: -0.015 min
Response: 24151
Conc: 6.49 ng/ml

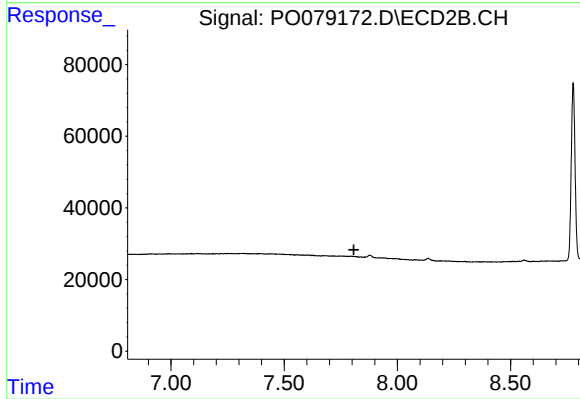

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 7.808 min
Response: 0
Conc: N.D.

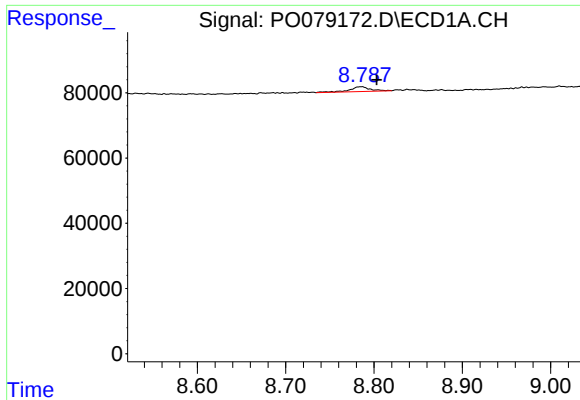

#42 AR-1268-2


R.T.: 8.786 min
Delta R.T.: -0.017 min
Response: 24151
Conc: 3.23 ng/ml

Instrument :
ECD_O
ClientSampleId :

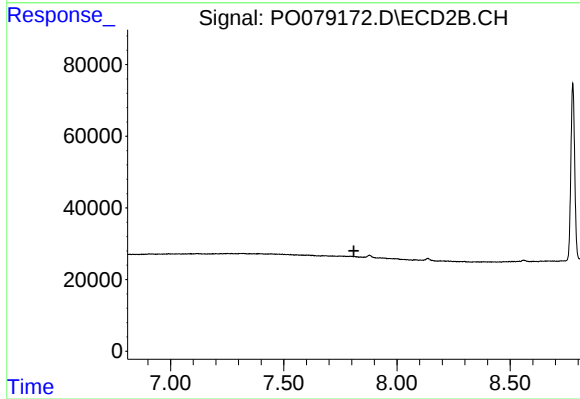


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.810 min
Response: 0
Conc: N.D.

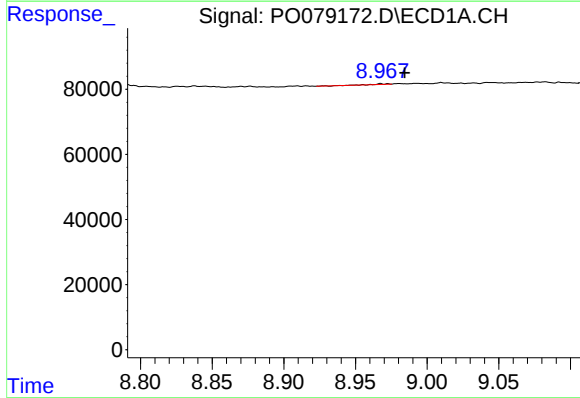

#43 AR-1268-3

R.T.: 8.968 min
Delta R.T.: -0.017 min
Response: 1291
Conc: 0.20 ng/ml

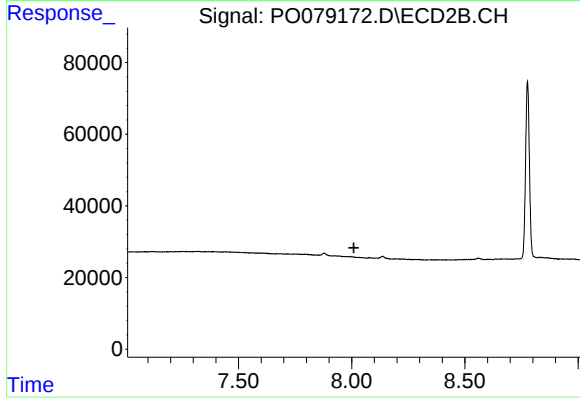

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.010 min
Response: 0
Conc: N.D.