

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062521\
 Data File : P0079156.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2021 16:30
 Operator : DD\AJ
 Sample : M2826-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SS-1(SLUDGE)

Manual Integrations
 APPROVED

mohammad
 6/28/2021 9:34:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:23:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.327	3.611	1641987	514746	20.805m	17.319m
2) SA Decachlor...	9.932	8.786	1155695	568113	18.505	19.065m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062521\
Data File : P0079156.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2021 16:30
Operator : DD\AJ
Sample : M2826-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SS-1(SLUDGE)


Manual Integrations
APPROVED

mohammad
6/28/2021 9:34:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:23:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

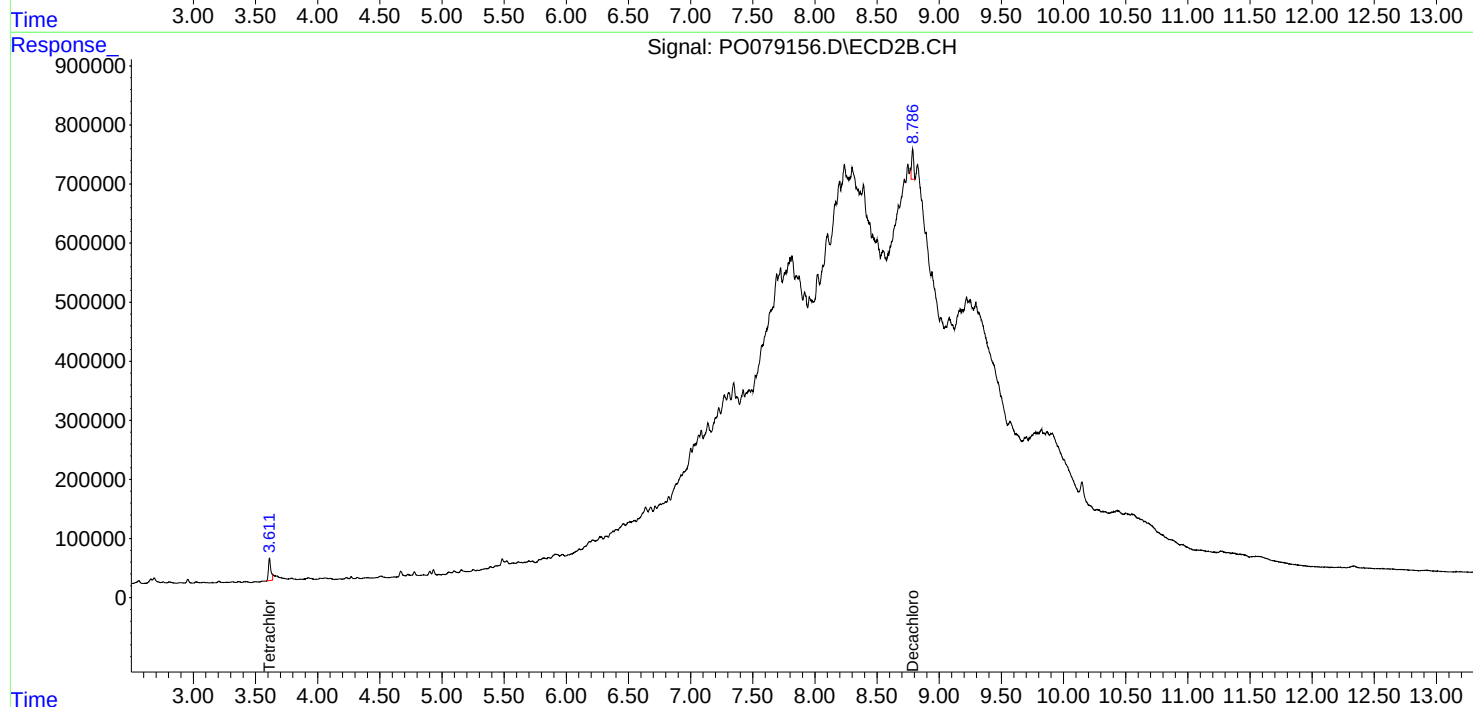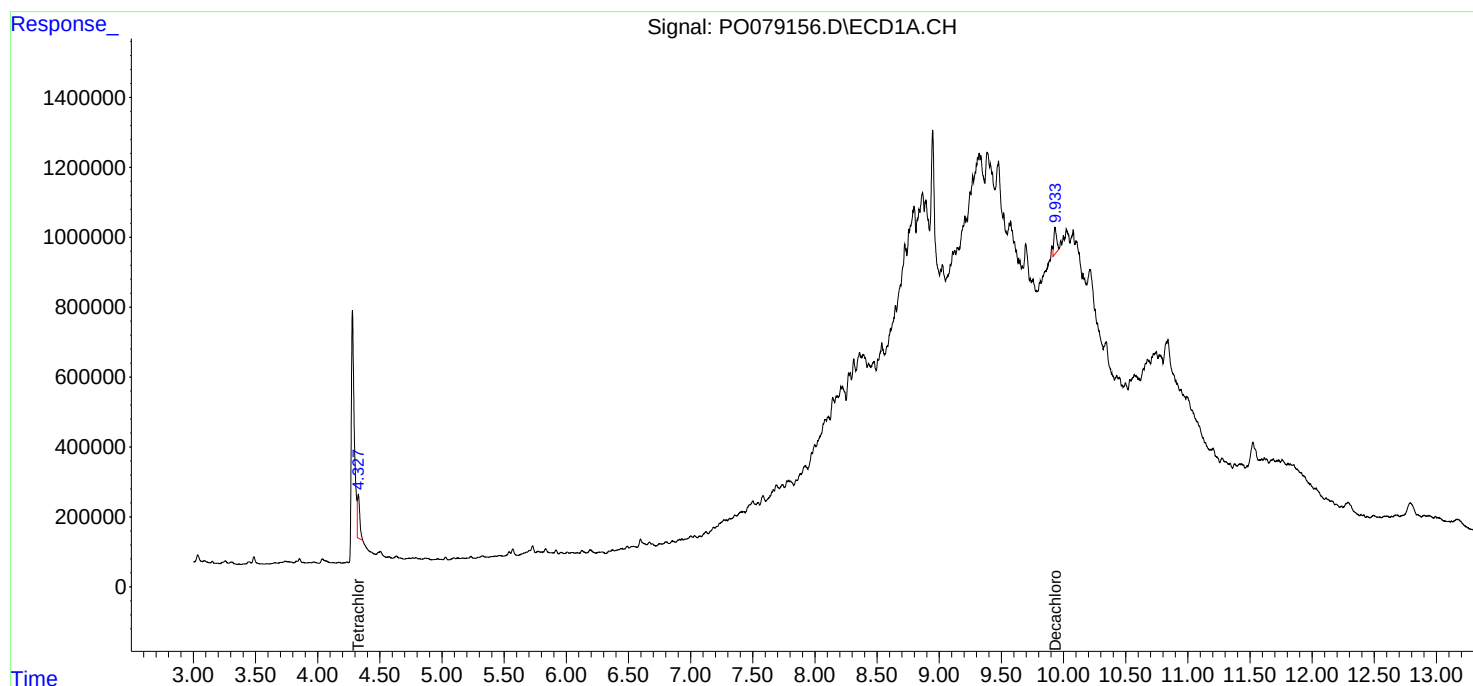

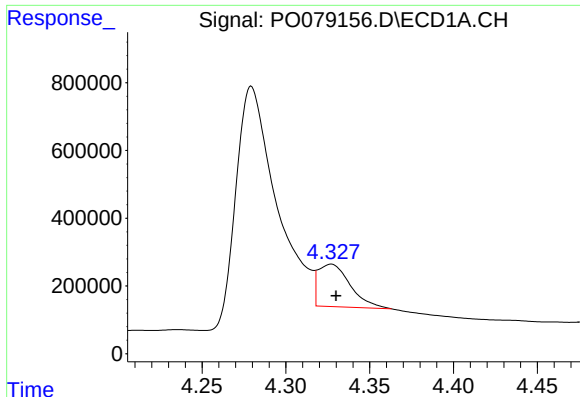


#1 Tetrachloro-m-xylene

R.T.: 4.327 min
Delta R.T.: -0.003 min
Response: 1641987
Conc: 20.81 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SS-1(SLUDGE)


Manual Integrations
APPROVED

mohammad
6/28/2021 9:34:30 AM

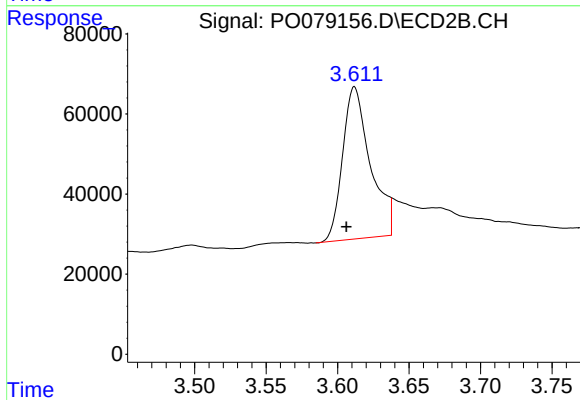


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: 0.005 min
Response: 514746
Conc: 17.32 ng/ml m

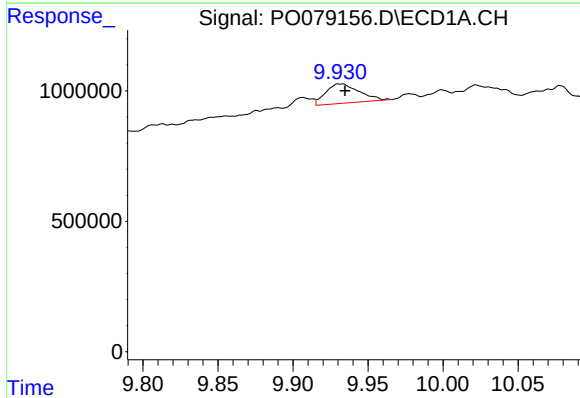

#2 Decachlorobiphenyl

R.T.: 9.932 min
Delta R.T.: -0.003 min
Response: 1155695
Conc: 18.50 ng/ml

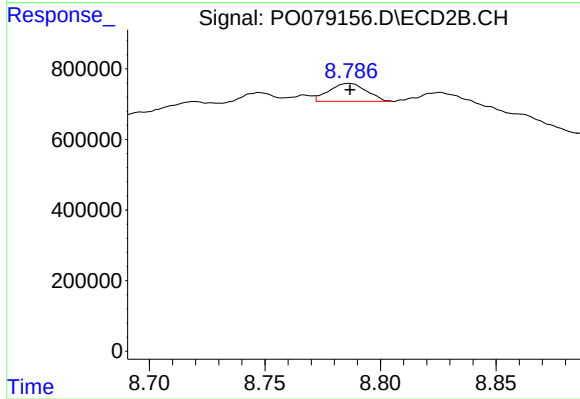

#2 Decachlorobiphenyl

R.T.: 8.786 min
Delta R.T.: 0.000 min
Response: 568113
Conc: 19.07 ng/ml m