

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062521\
 Data File : P0079176.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jun 2021 23:16
 Operator : DD\AJ
 Sample : M2831-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MW-03-GW

Manual Integrations
 APPROVED

mohammad
 6/28/2021 9:34:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:33:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.322	3.601	1183936	536298	15.001	18.045
2) SA Decachlor...	9.922	8.775	1241122	575776	19.872	19.322

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062521\
Data File : P0079176.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jun 2021 23:16
Operator : DD\AJ
Sample : M2831-06
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MW-03-GW


Manual Integrations
APPROVED

mohammad
6/28/2021 9:34:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:33:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

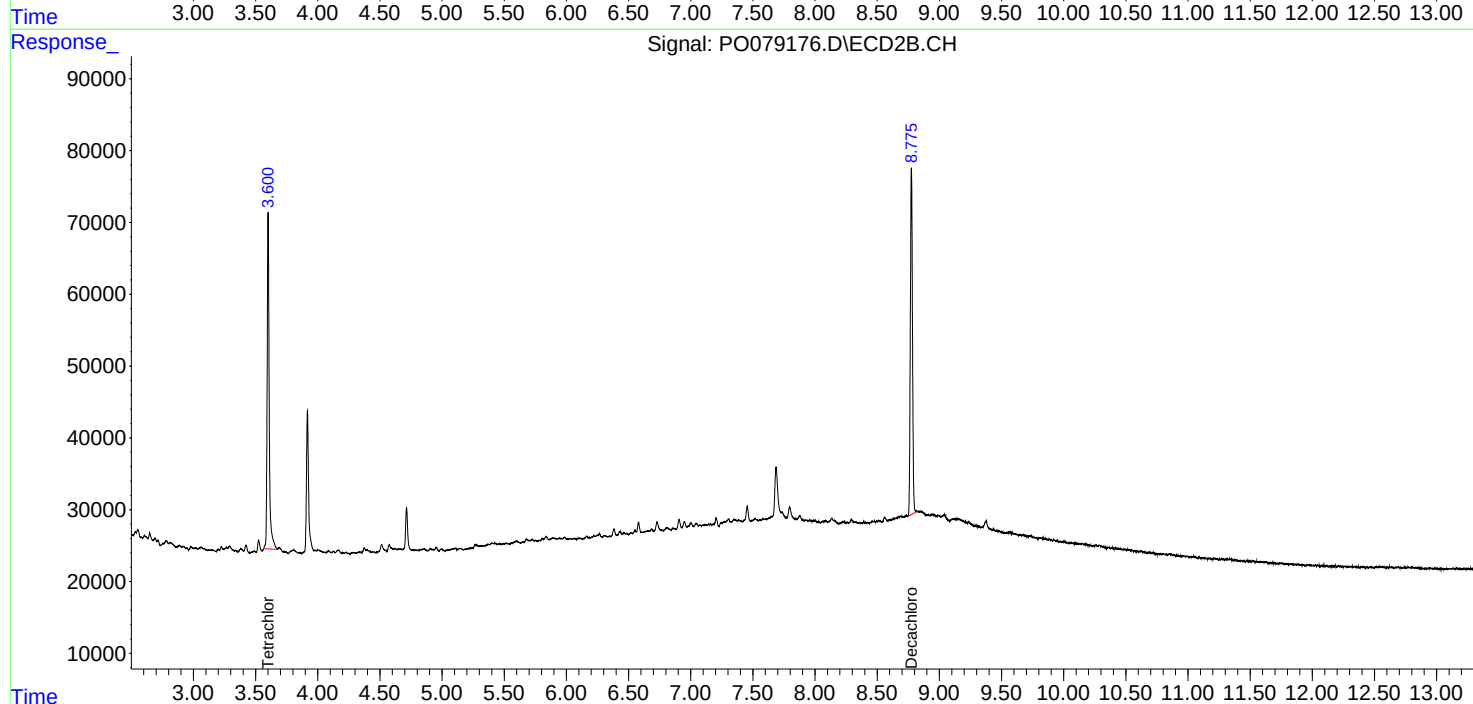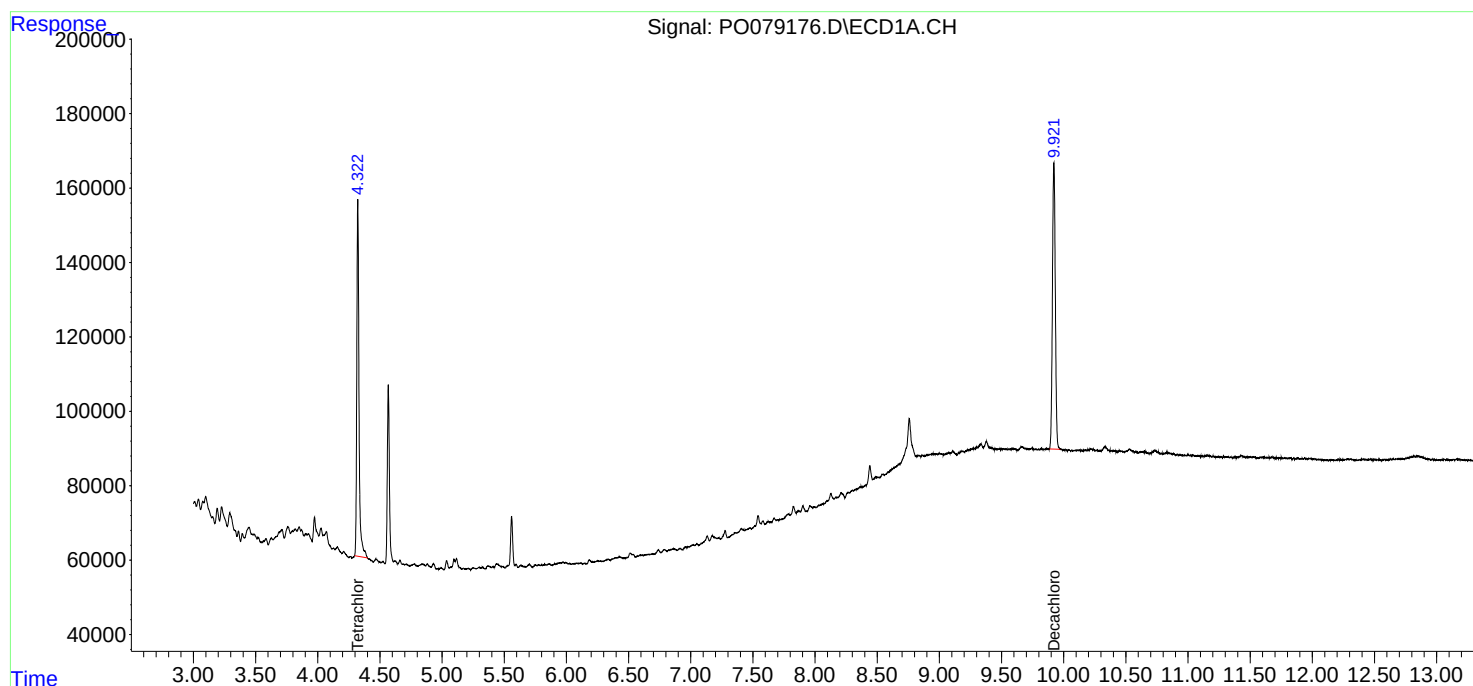

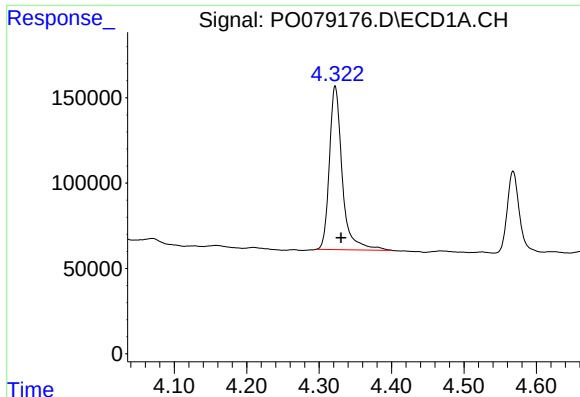

#1 Tetrachloro-m-xylene

R.T.: 4.322 min
Delta R.T.: -0.008 min
Response: 1183936
Conc: 15.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MW-03-GW

Manual Integrations
APPROVED

mohammad
6/28/2021 9:34:46 AM

#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.005 min
Response: 536298
Conc: 18.04 ng/ml

#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: -0.013 min
Response: 1241122
Conc: 19.87 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.775 min
Delta R.T.: -0.011 min
Response: 575776
Conc: 19.32 ng/ml