

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062521\
 Data File : P0079192.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jun 2021 4:54
 Operator : DD\AJ
 Sample : M2847-05
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1966-1969

Manual Integrations
 APPROVED

mohammad
 6/28/2021 9:35:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 02:14:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.332	3.629f	1023017	1058756	12.962m	35.623 #
2) SA Decachlor...	9.923	8.777	874905	398245	14.009	13.365

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062521\
Data File : P0079192.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2021 4:54
Operator : DD\AJ
Sample : M2847-05
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
1966-1969


Manual Integrations
APPROVED

mohammad
6/28/2021 9:35:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 02:14:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

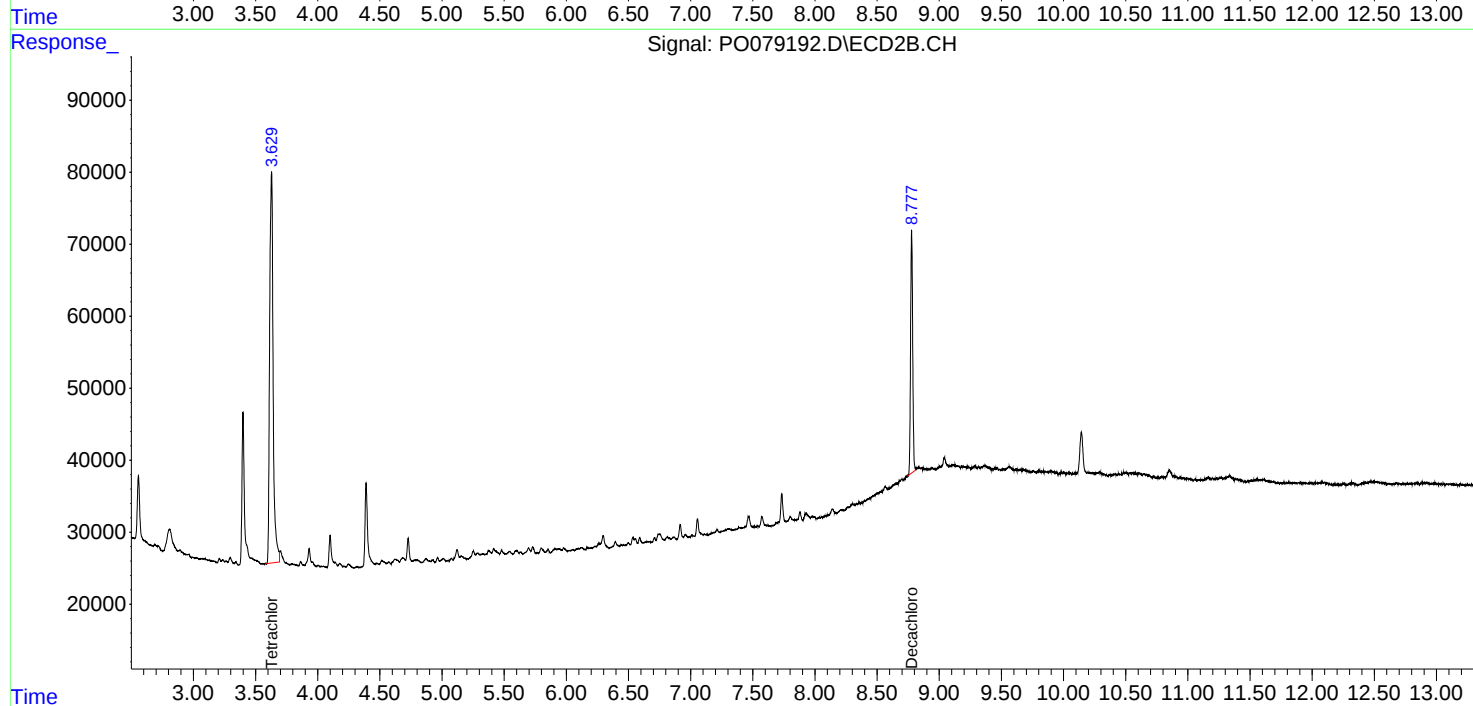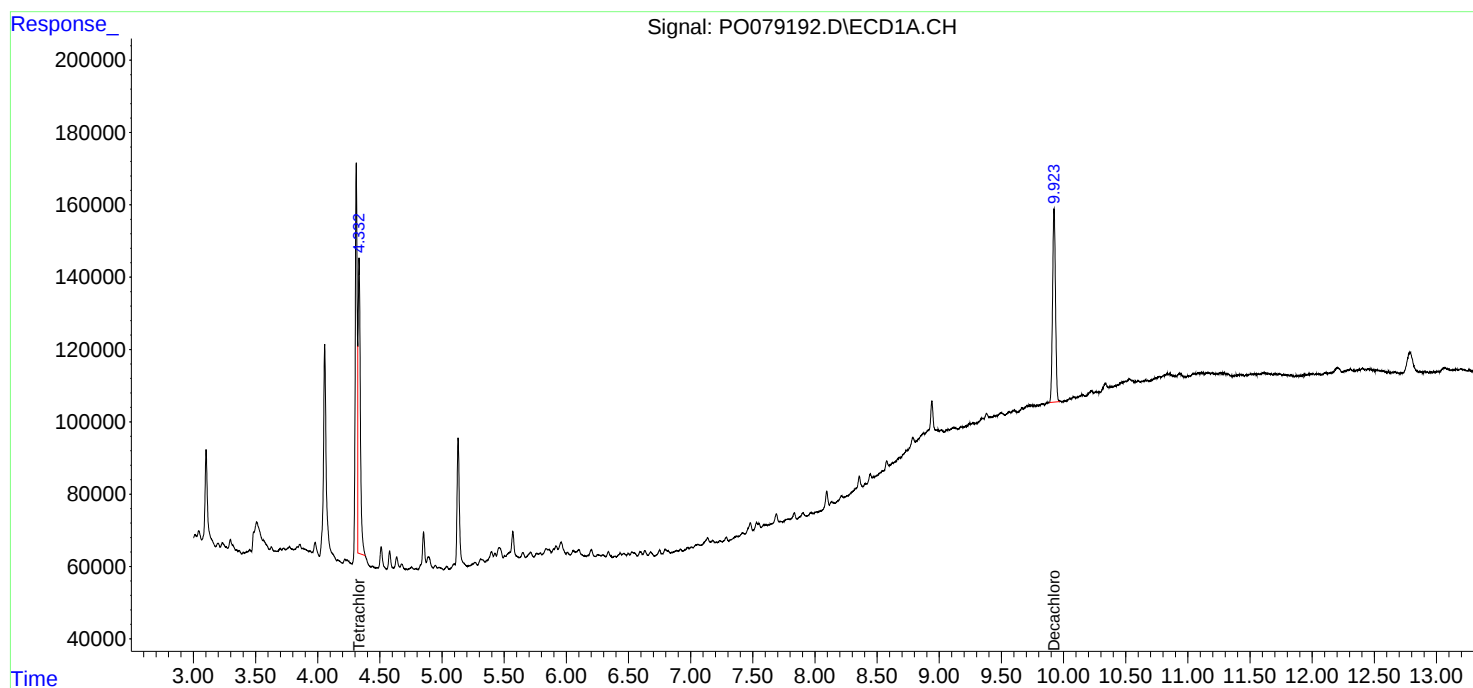

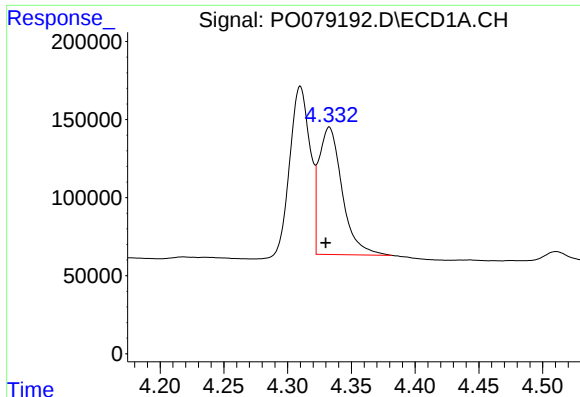


#1 Tetrachloro-m-xylene

R.T.: 4.332 min
Delta R.T.: 0.002 min
Response: 1023017
Conc: 12.96 ng/ml m

Instrument :
ECD_O
ClientSampleId :
1966-1969


Manual Integrations
APPROVED

mohammad
6/28/2021 9:35:24 AM

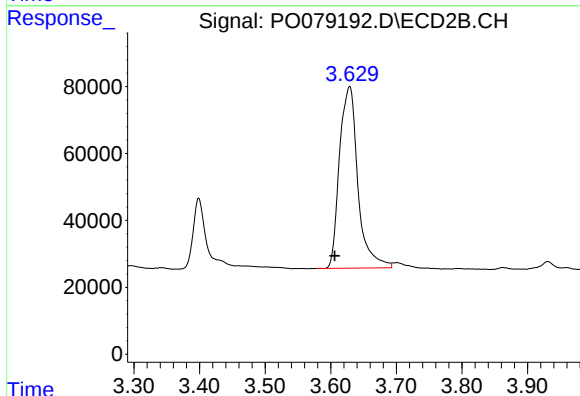


#1 Tetrachloro-m-xylene

R.T.: 3.629 min
Delta R.T.: 0.023 min
Response: 1058756
Conc: 35.62 ng/ml

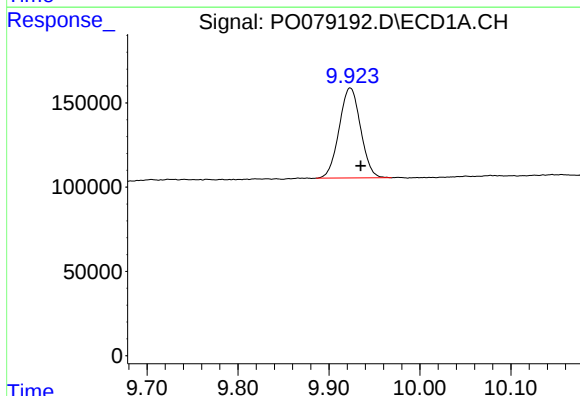

#2 Decachlorobiphenyl

R.T.: 9.923 min
Delta R.T.: -0.011 min
Response: 874905
Conc: 14.01 ng/ml

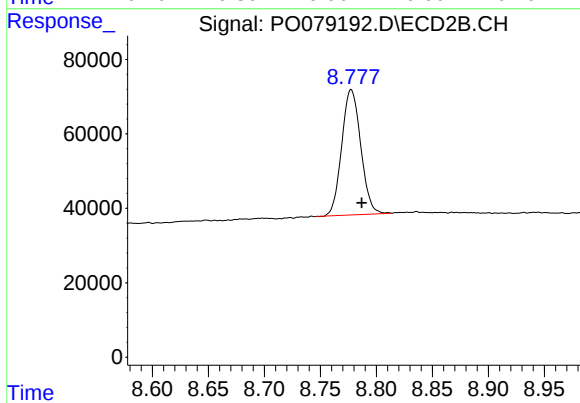

#2 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: -0.009 min
Response: 398245
Conc: 13.36 ng/ml