

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0062618\
Data File : P0046255.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2018 11:13
Operator : SM/UA
Sample : J3241-17RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HR-06-062218-CRE

Manual Integrations
APPROVED

ugo
6/27/2018 4:52:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 11:53:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 26 05:14:56 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.379	3.606	5950826	3220355	10.181	12.974m#
2) SA Decachlor...	10.043	8.572	3452898	1243875	7.489	7.420m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062618\
Data File : P0046255.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2018 11:13
Operator : SM/UA
Sample : J3241-17RE
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
HR-06-062218-CRE


Manual Integrations
APPROVED

ugo
6/27/2018 4:52:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 11:53:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 26 05:14:56 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

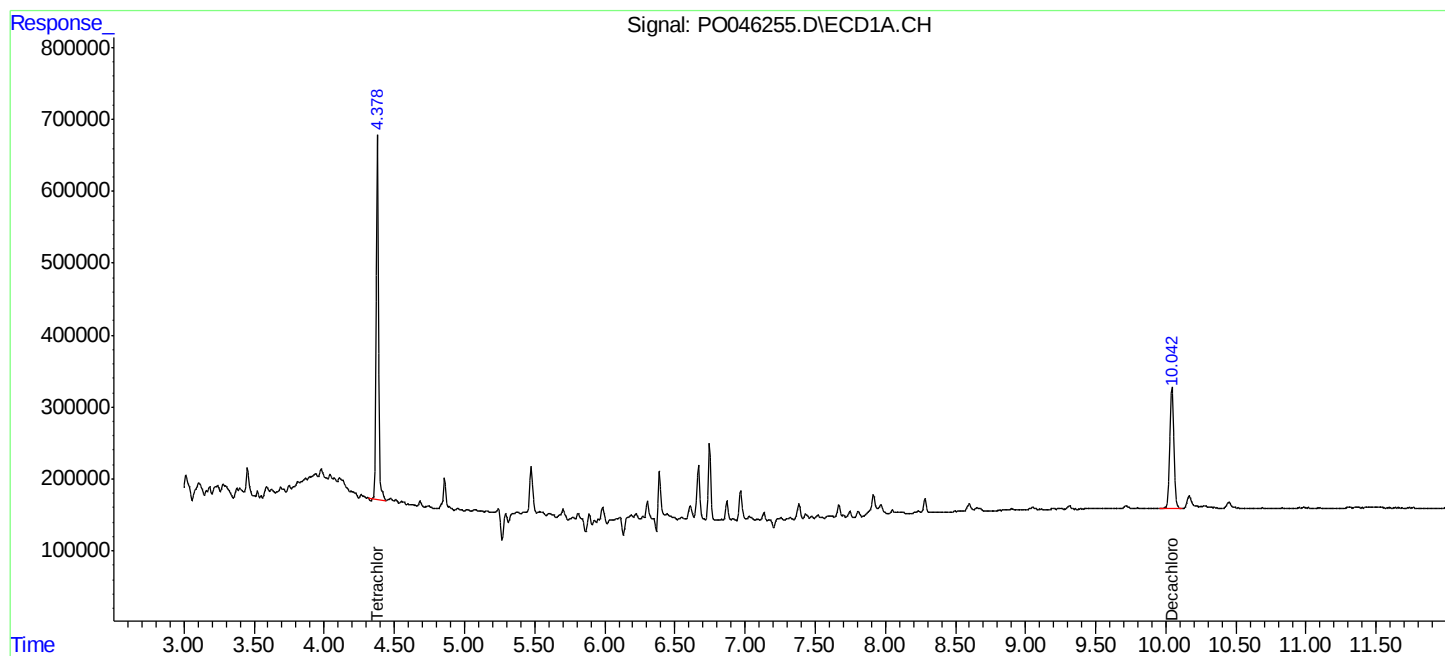

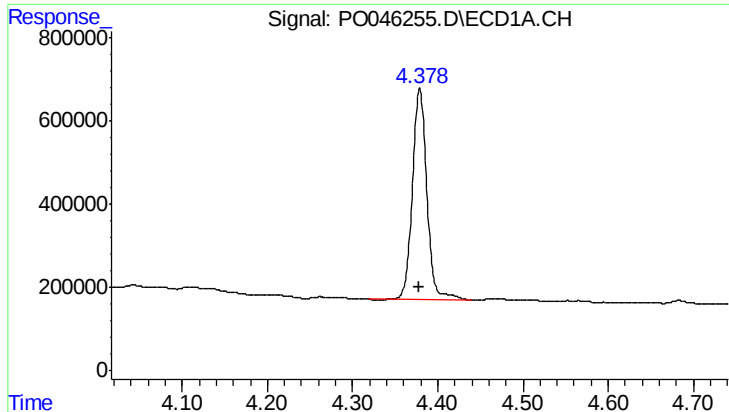


#1 Tetrachloro-m-xylene

R.T.: 4.379 min
Delta R.T.: 0.000 min
Response: 5950826
Conc: 10.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
HR-06-062218-CRE


Manual Integrations
APPROVED

ugo
6/27/2018 4:52:58 PM

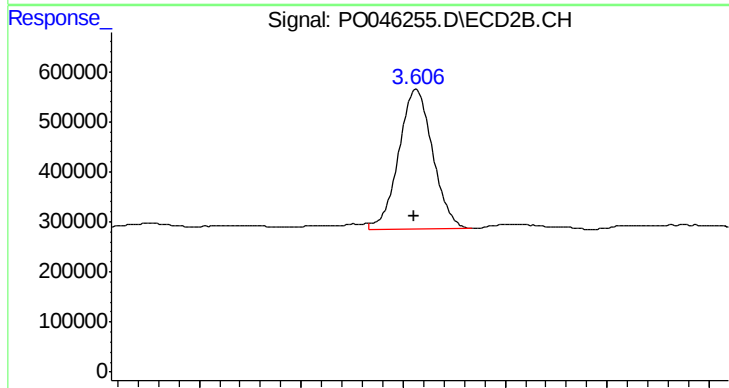


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.001 min
Response: 3220355
Conc: 12.97 ng/ml m

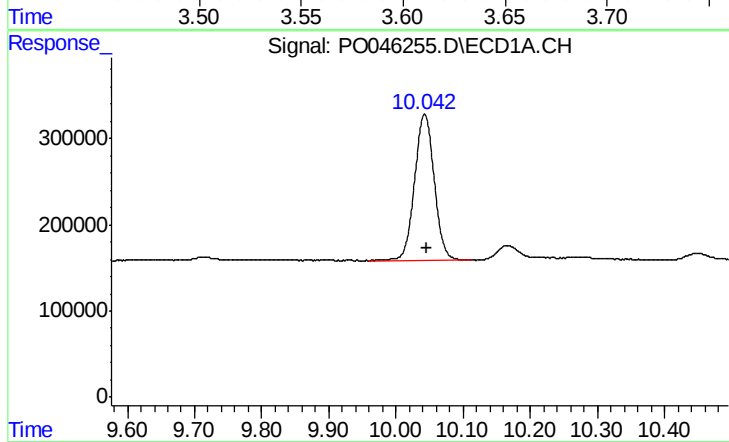

#2 Decachlorobiphenyl

R.T.: 10.043 min
Delta R.T.: -0.003 min
Response: 3452898
Conc: 7.49 ng/ml

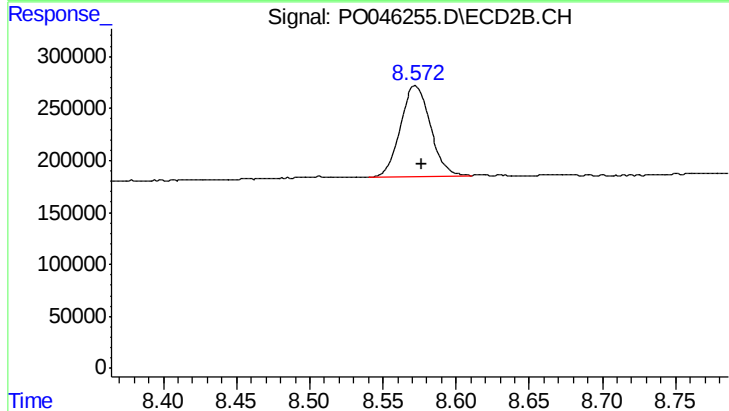

#2 Decachlorobiphenyl

R.T.: 8.572 min
Delta R.T.: -0.005 min
Response: 1243875
Conc: 7.42 ng/ml m