

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0062618\
 Data File : P0046257.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jun 2018 11:56
 Operator : SM/UA
 Sample : J3672-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ETGI-348-CONCRETE

Manual Integrations
 APPROVED

ugo
 6/27/2018 4:53:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 12:39:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 26 05:14:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.380	3.606	9492339	4478991	16.241	18.045m
2) SA Decachlor...	10.046	8.572	5929166	2332937	12.860	13.917m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062618\
Data File : P0046257.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2018 11:56
Operator : SM/UA
Sample : J3672-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ETGI-348-CONCRETE


Manual Integrations
APPROVED

ugo
6/27/2018 4:53:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 12:39:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 26 05:14:56 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

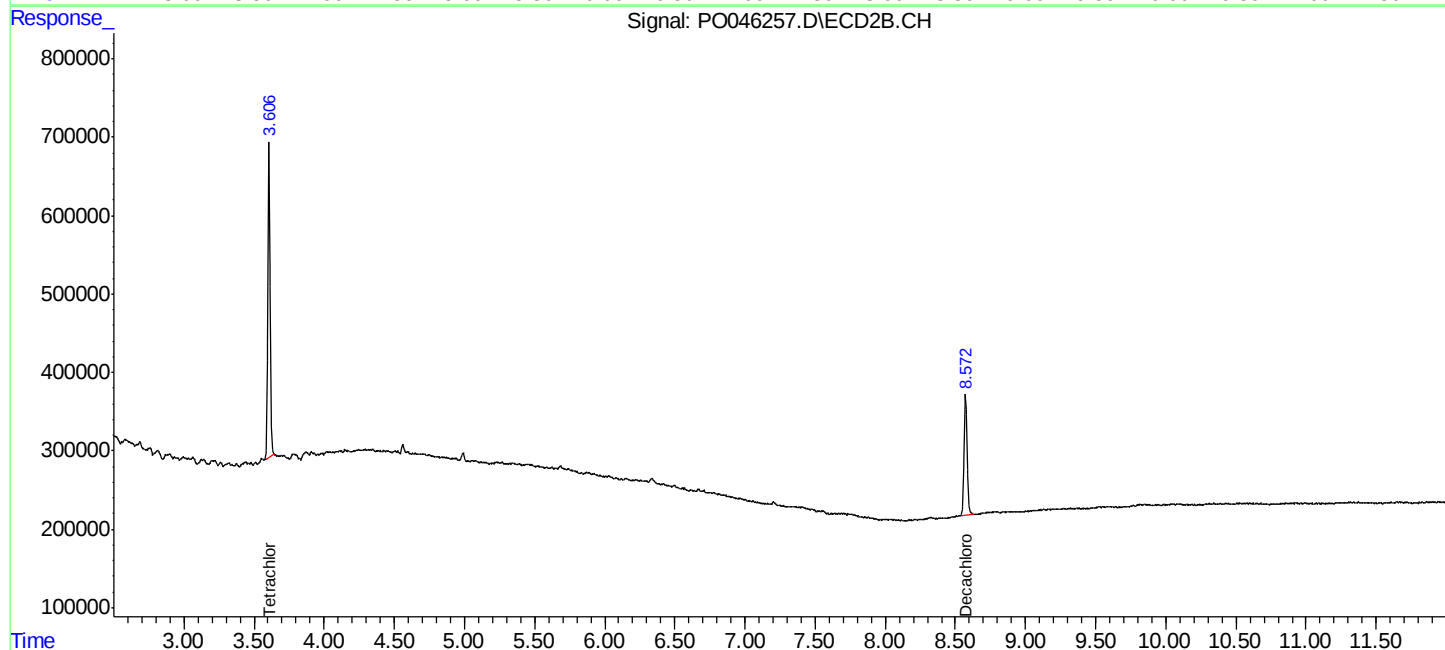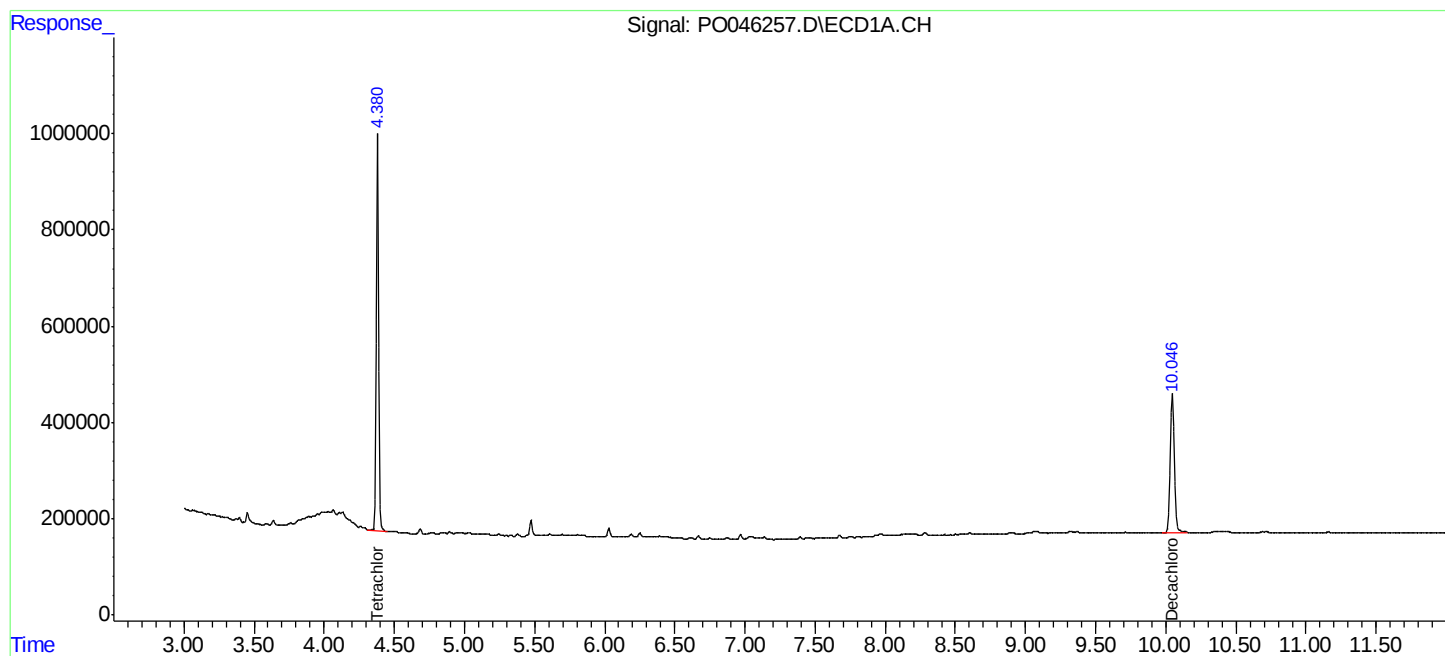

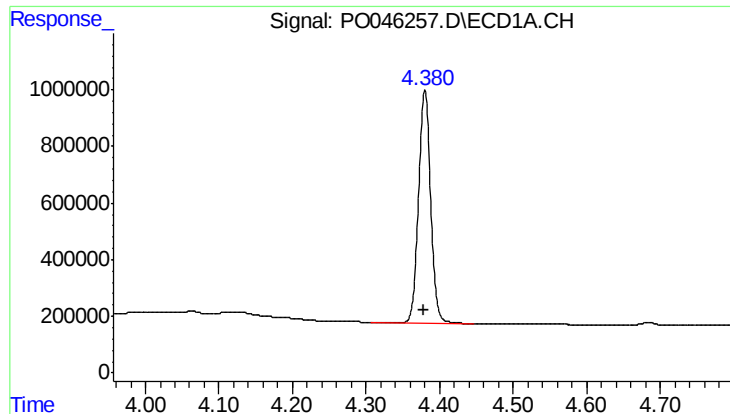


#1 Tetrachloro-m-xylene

R.T.: 4.380 min
Delta R.T.: 0.002 min
Response: 9492339
Conc: 16.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-348-CONCRETE


Manual Integrations
APPROVED

ugo
6/27/2018 4:53:05 PM

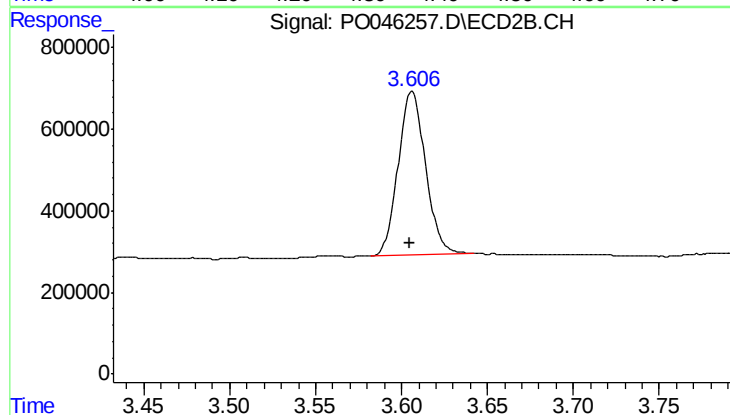


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 4478991
Conc: 18.05 ng/ml m

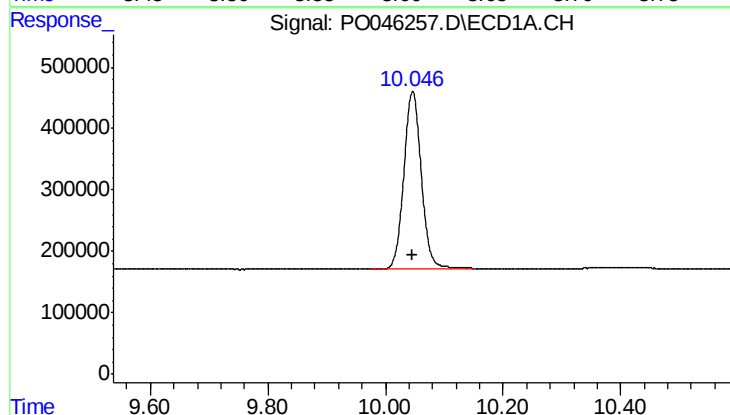

#2 Decachlorobiphenyl

R.T.: 10.046 min
Delta R.T.: 0.000 min
Response: 5929166
Conc: 12.86 ng/ml

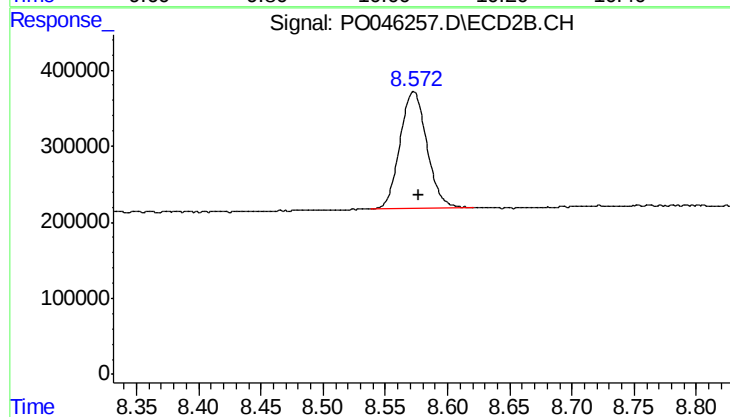

#2 Decachlorobiphenyl

R.T.: 8.572 min
Delta R.T.: -0.004 min
Response: 2332937
Conc: 13.92 ng/ml m