

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062618\
 Data File : P0046279.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jun 2018 19:22
 Operator : SM/UA
 Sample : PB110592BS
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB110592BS

Manual Integrations
 APPROVED

ugo
 6/27/2018 4:53:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 02:19:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 26 05:14:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.379	3.607	14016101	5865595	23.980m	23.632m
2) SA Decachlor...	10.045	8.573	7900296	3617515	17.135	21.580 #

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0062618\
Data File : P0046279.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2018 19:22
Operator : SM/UA
Sample : PB110592BS
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB110592BS


Manual Integrations
APPROVED

ugo
6/27/2018 4:53:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 02:19:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 26 05:14:56 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

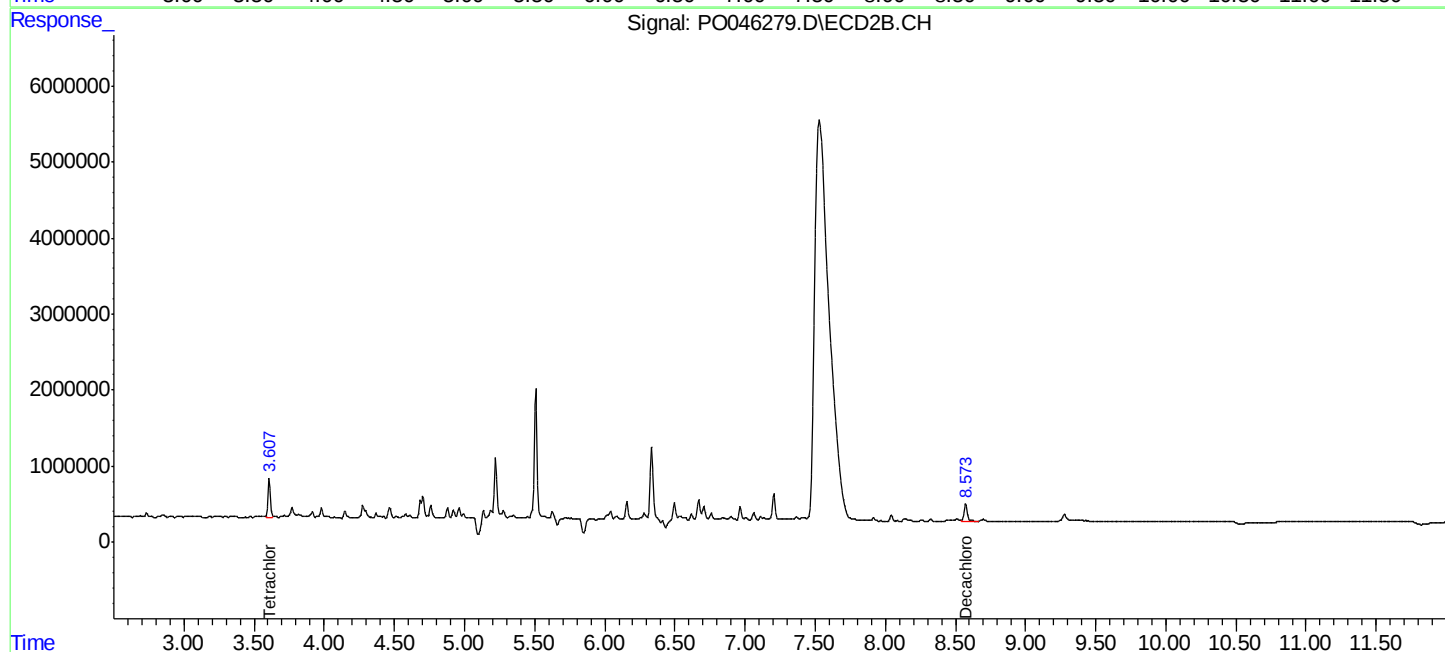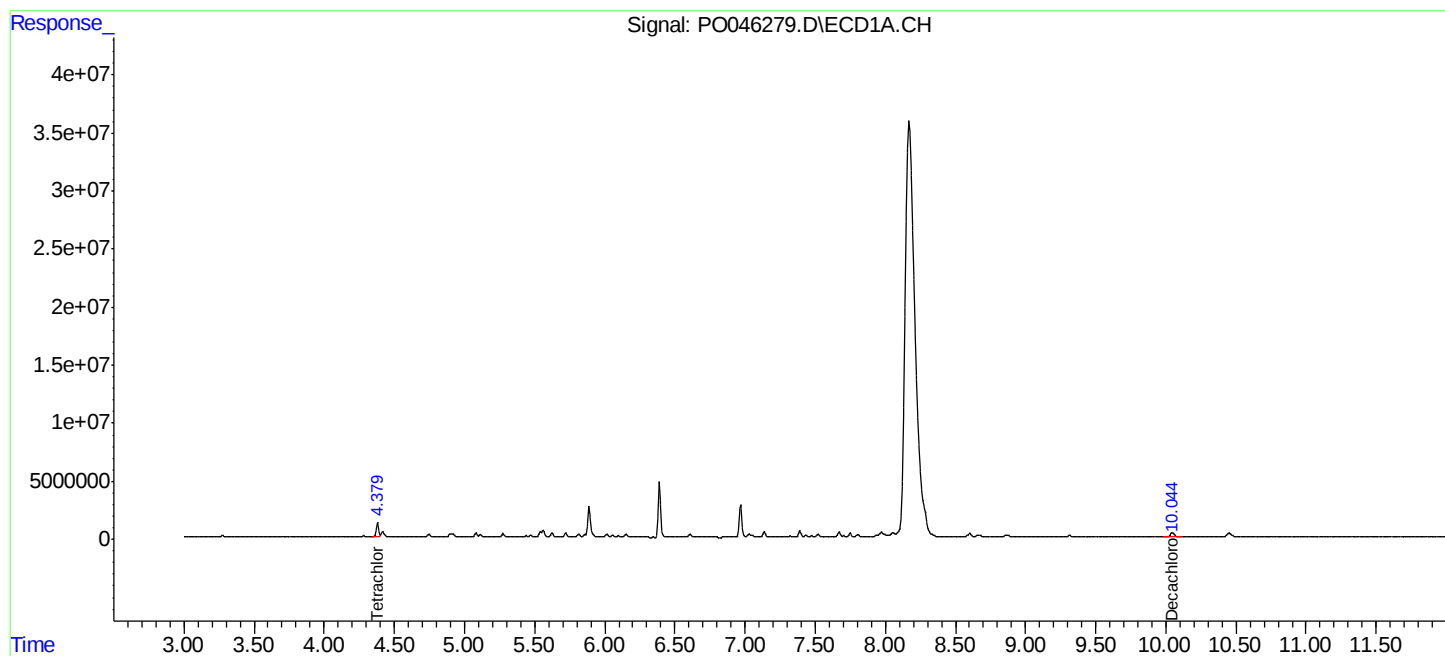

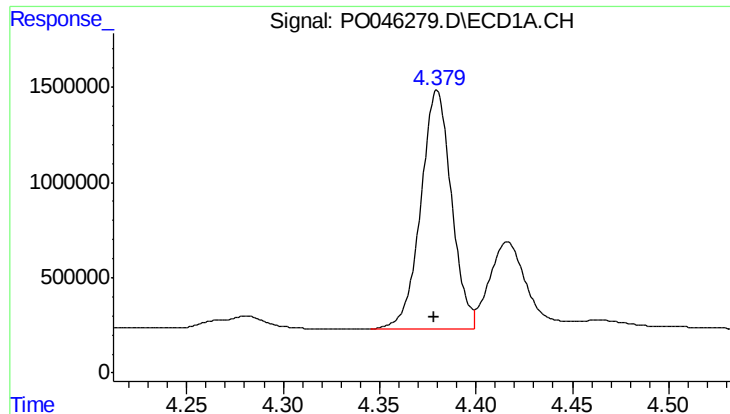


#1 Tetrachloro-m-xylene

R.T.: 4.379 min
Delta R.T.: 0.001 min
Response: 14016101
Conc: 23.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB110592BS


Manual Integrations
APPROVED

ugo
6/27/2018 4:53:52 PM

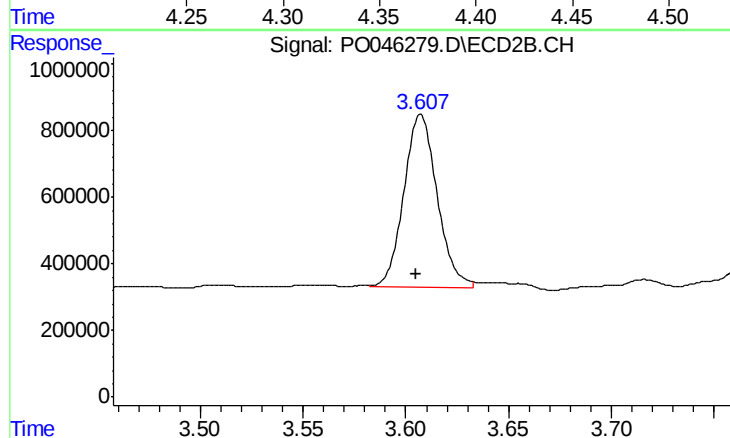


#1 Tetrachloro-m-xylene

R.T.: 3.607 min
Delta R.T.: 0.002 min
Response: 5865595
Conc: 23.63 ng/ml m

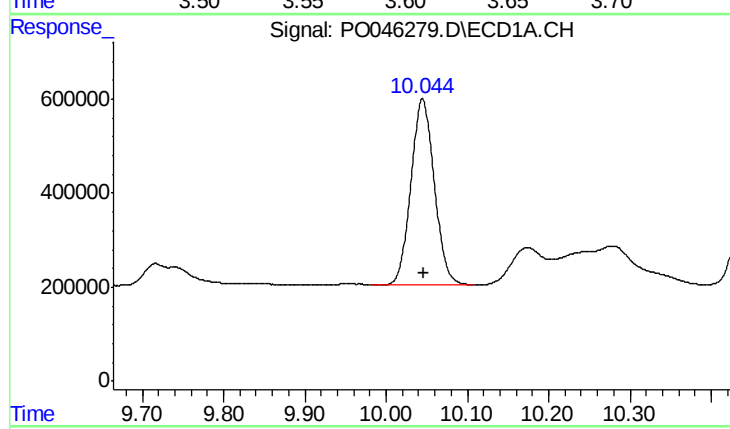

#2 Decachlorobiphenyl

R.T.: 10.045 min
Delta R.T.: -0.001 min
Response: 7900296
Conc: 17.14 ng/ml

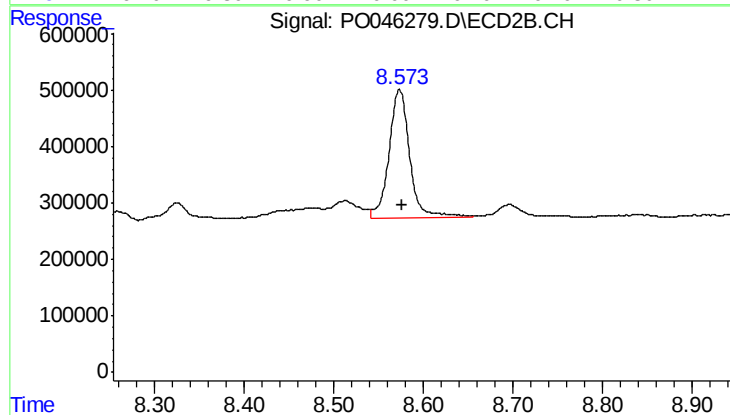

#2 Decachlorobiphenyl

R.T.: 8.573 min
Delta R.T.: -0.004 min
Response: 3617515
Conc: 21.58 ng/ml