

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062619\
 Data File : P0057480.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jun 2019 10:18
 Operator : SM/SJ
 Sample : K3164-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BAT-B09

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 11:44:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.232	3.554	932431	861432	23.737	24.498
2) SA Decachlor...	9.778	8.474	1112977	755466	19.792	20.196
Target Compounds						
3) L1 AR-1016-1	5.322	0.000	28455	0	16.099	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062619\
Data File : P0057480.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2019 10:18
Operator : SM/SJ
Sample : K3164-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BAT-B09

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 11:44:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

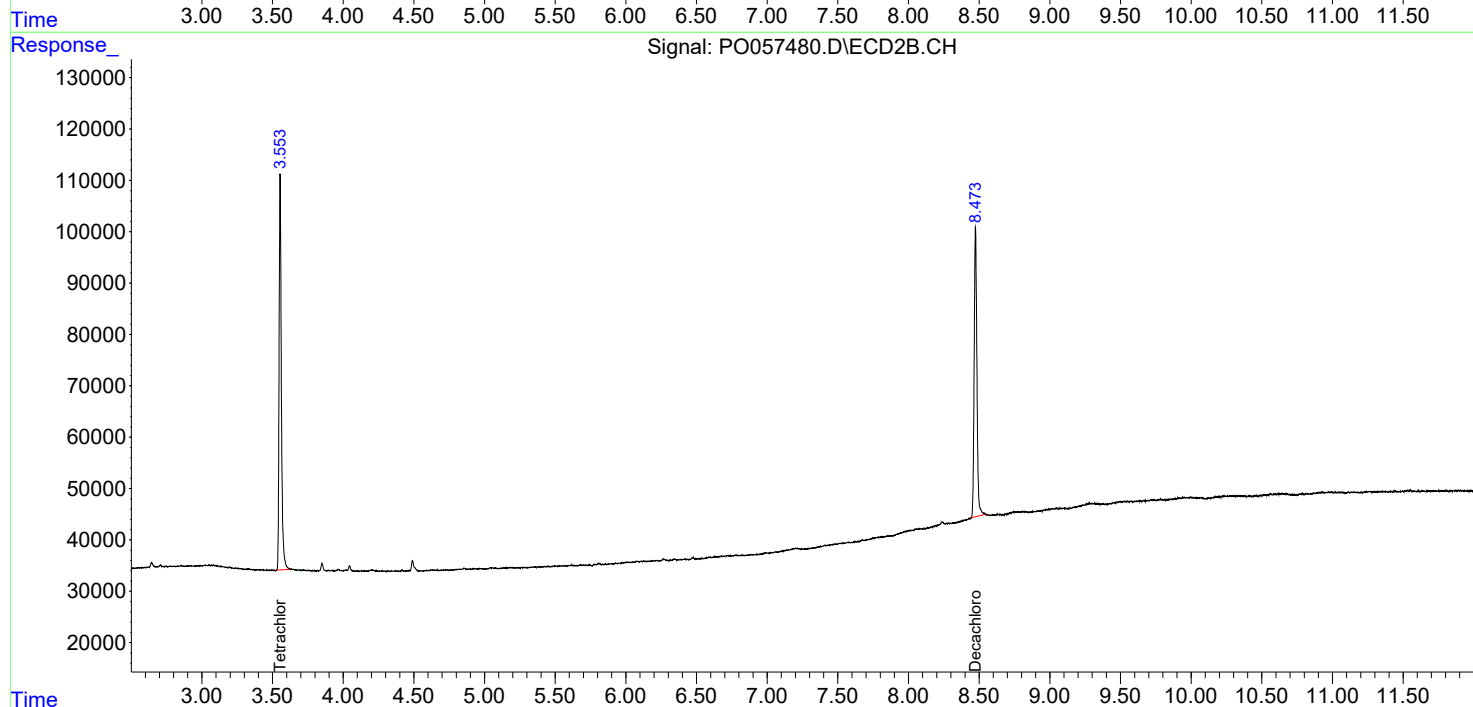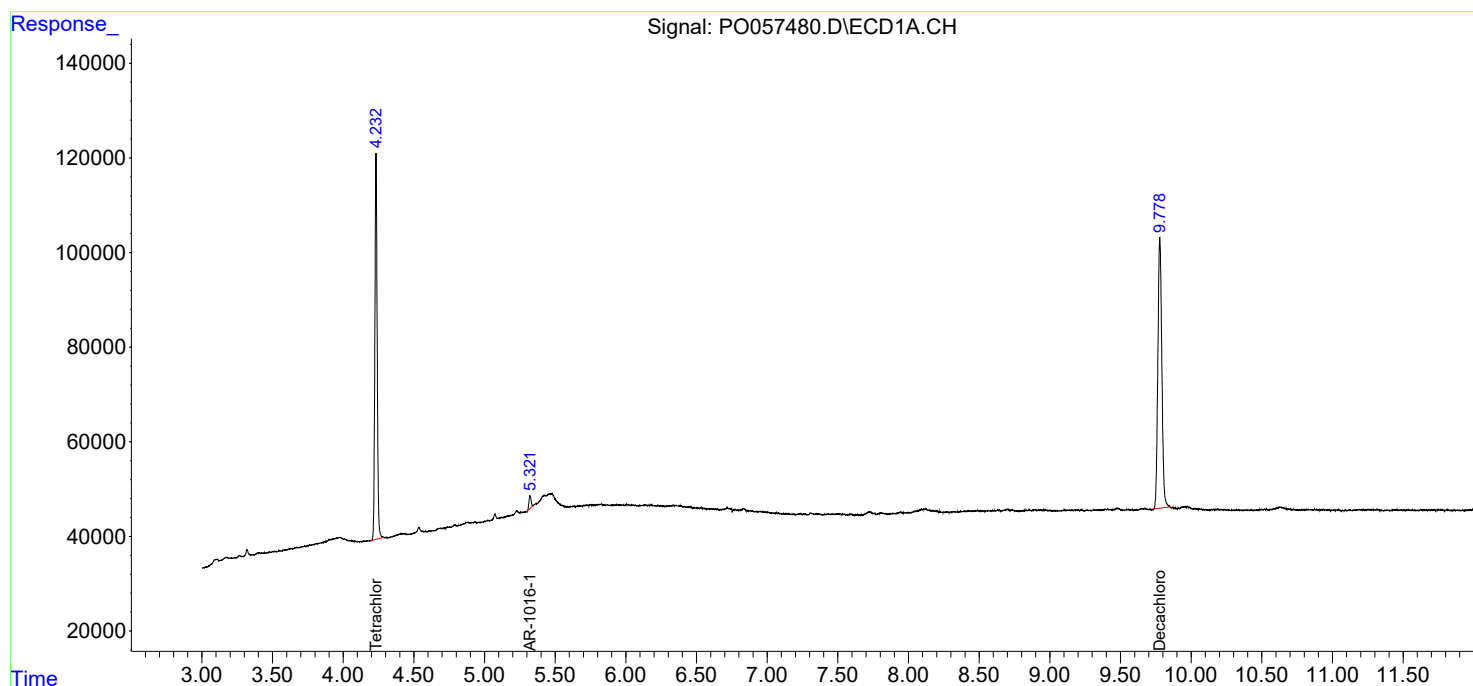


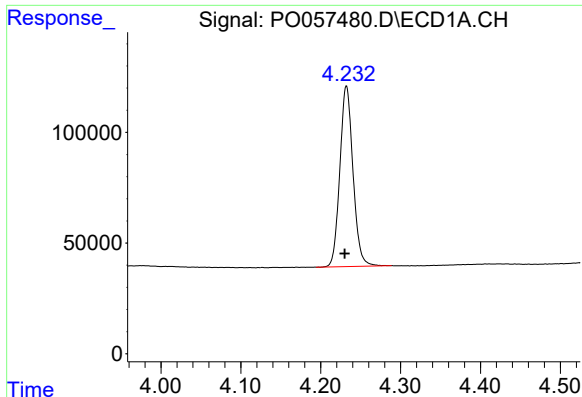

#1 Tetrachloro-m-xylene


R.T.: 4.232 min
Delta R.T.: 0.002 min
Response: 932431
Conc: 23.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
BAT-B09

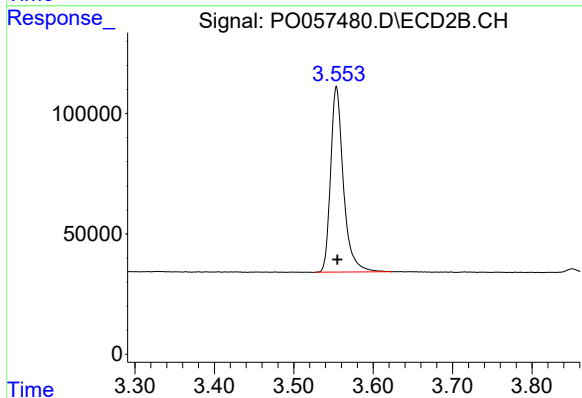


#1 Tetrachloro-m-xylene

R.T.: 3.554 min
Delta R.T.: -0.001 min
Response: 861432
Conc: 24.50 ng/ml

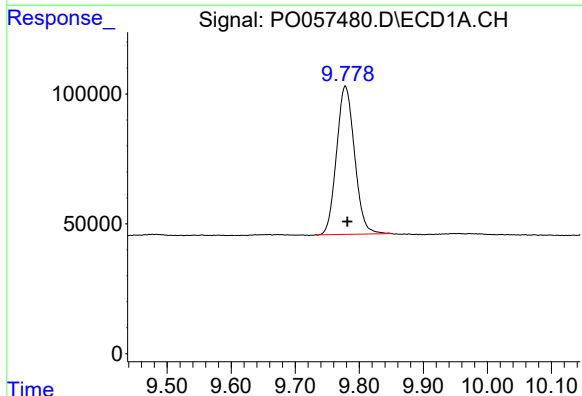


#2 Decachlorobiphenyl

R.T.: 9.778 min
Delta R.T.: -0.003 min
Response: 1112977
Conc: 19.79 ng/ml

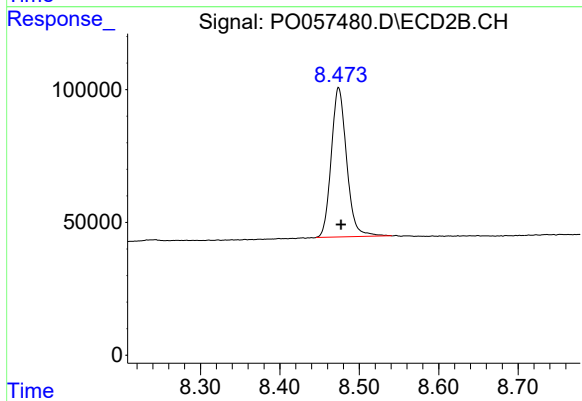

#2 Decachlorobiphenyl


R.T.: 8.474 min
Delta R.T.: -0.003 min
Response: 755466
Conc: 20.20 ng/ml

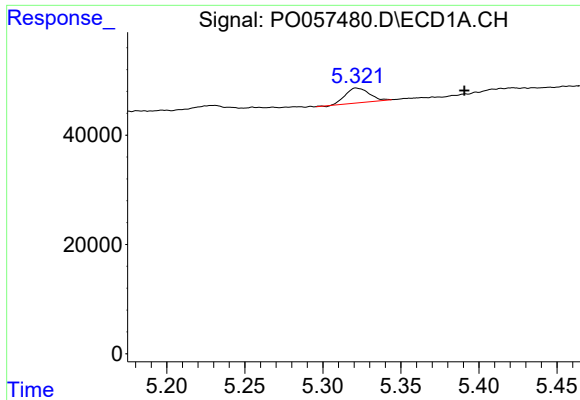

#3 AR-1016-1

R.T.: 5.322 min
Delta R.T.: -0.069 min
Response: 28455
Conc: 16.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
BAT-B09

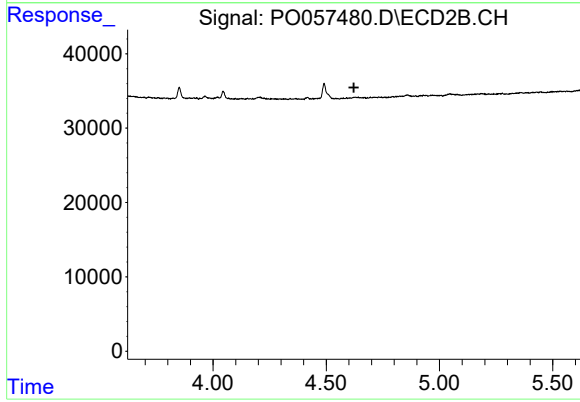

#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.622 min
Response: 0
Conc: N.D.