

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062619\
Data File : P0057499.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2019 18:31
Operator : SM/SJ
Sample : K3510-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TR-04-062419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 04:55:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	3.554	1038920	897050	26.448	25.511
2)	SA Decachlor...	9.779	8.474	1095098	733055	19.474	19.597

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062619\
Data File : PO057499.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2019 18:31
Operator : SM/SJ
Sample : K3510-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TR-04-062419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 04:55:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

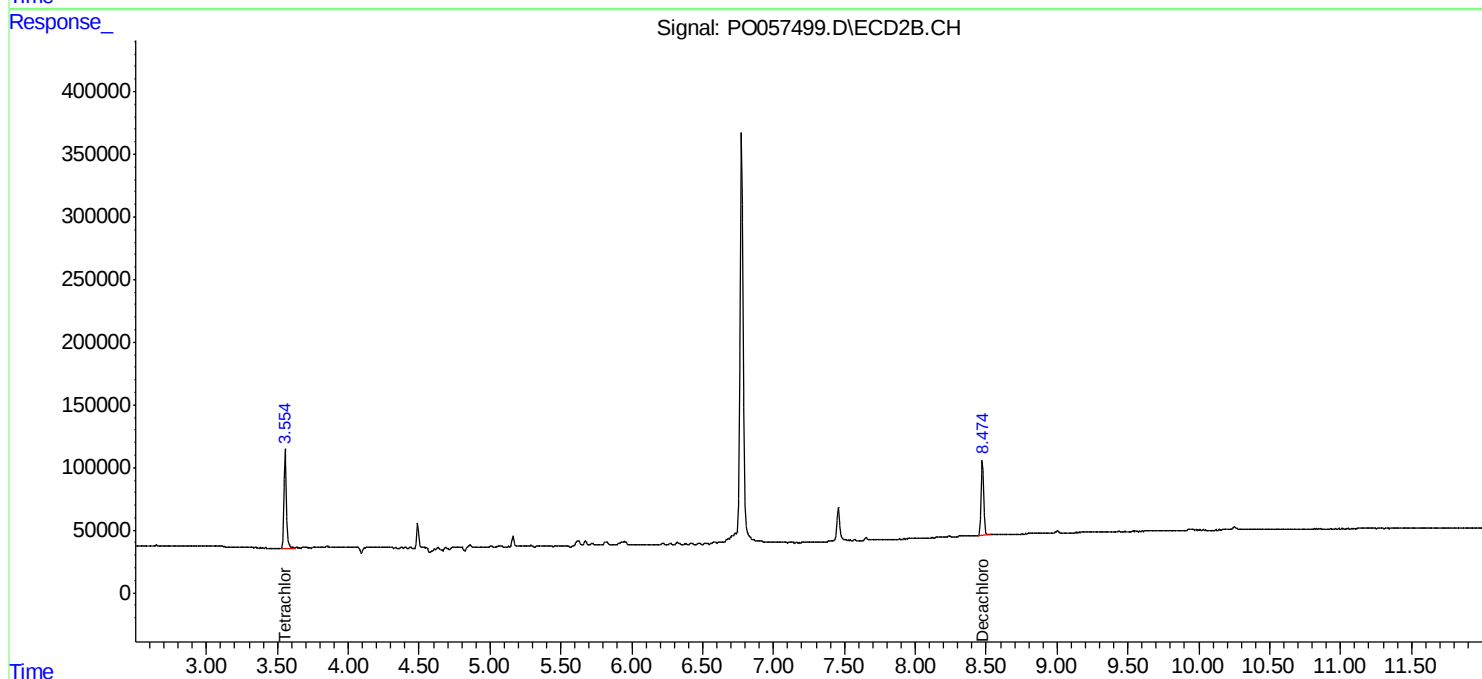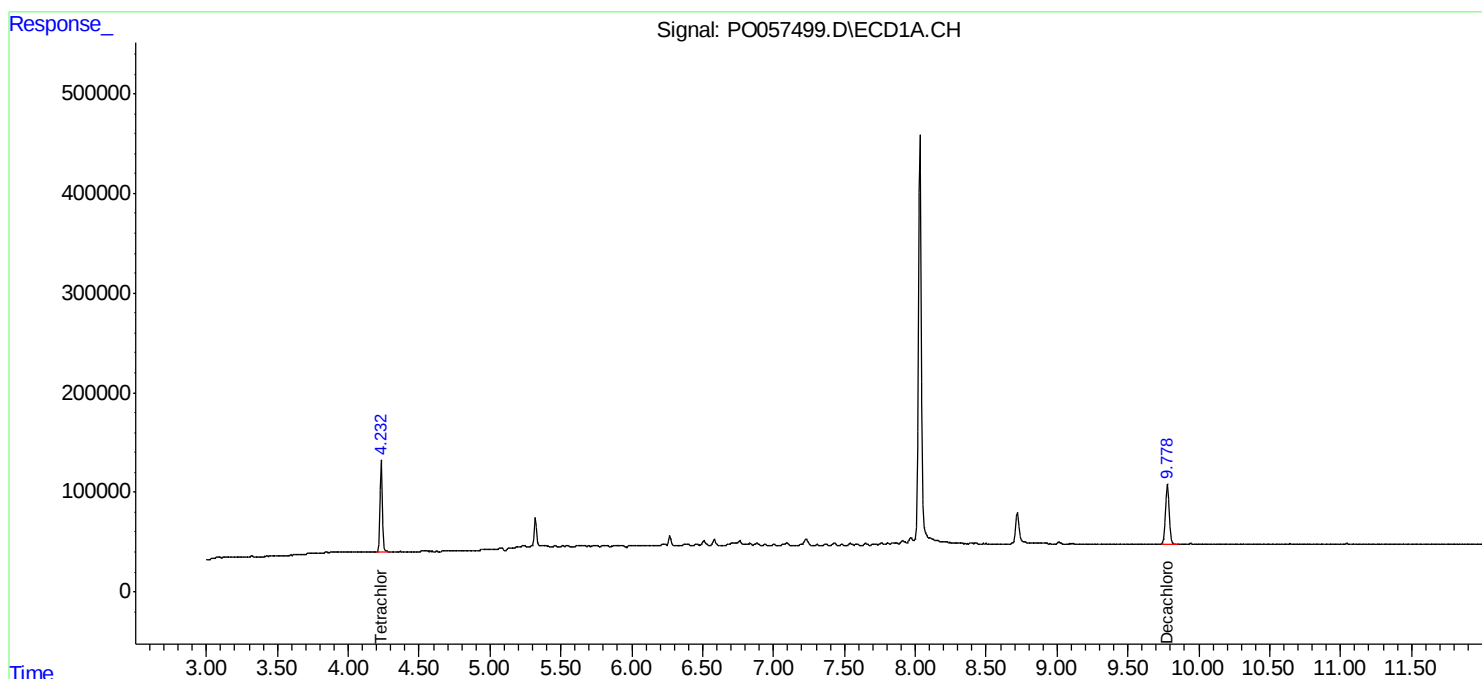


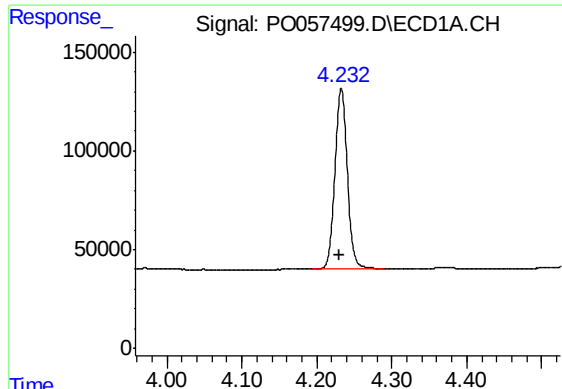

#1 Tetrachloro-m-xylene


R.T.: 4.233 min
Delta R.T.: 0.003 min
Response: 1038920
Conc: 26.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
TR-04-062419

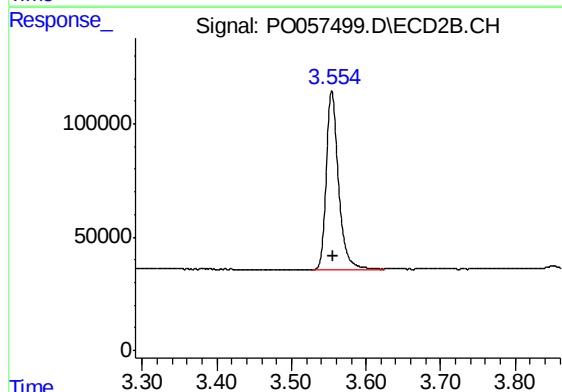


#1 Tetrachloro-m-xylene

R.T.: 3.554 min
Delta R.T.: 0.000 min
Response: 897050
Conc: 25.51 ng/ml

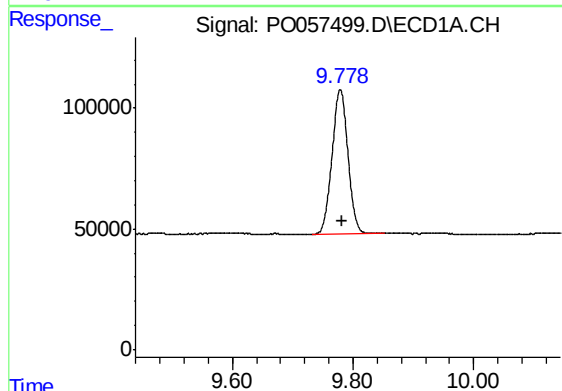

#2 Decachlorobiphenyl

R.T.: 9.779 min
Delta R.T.: -0.002 min
Response: 1095098
Conc: 19.47 ng/ml

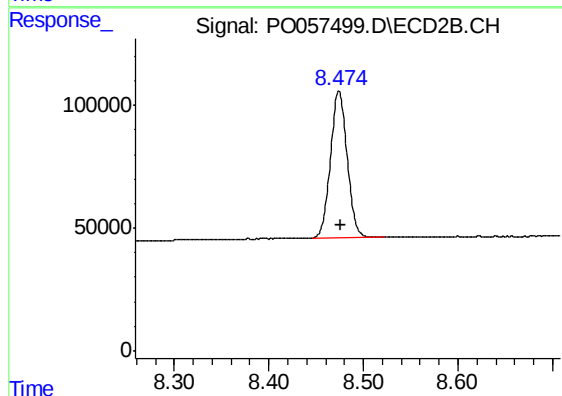

#2 Decachlorobiphenyl

R.T.: 8.474 min
Delta R.T.: -0.003 min
Response: 733055
Conc: 19.60 ng/ml