

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062619\
 Data File : P0057503.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jun 2019 19:42
 Operator : SM/SJ
 Sample : K3512-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SAMPLE-8

Manual Integrations
 APPROVED

Ankita
 6/27/2019 12:19:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 04:56:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.224	3.554	1062722	934948	27.054	26.589
2) SA Decachlor...	9.767	8.471	1112744	747527	19.788m	19.984

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062619\
Data File : P0057503.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2019 19:42
Operator : SM/SJ
Sample : K3512-06
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SAMPLE-8


Manual Integrations
APPROVED

Ankita
6/27/2019 12:19:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 04:56:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

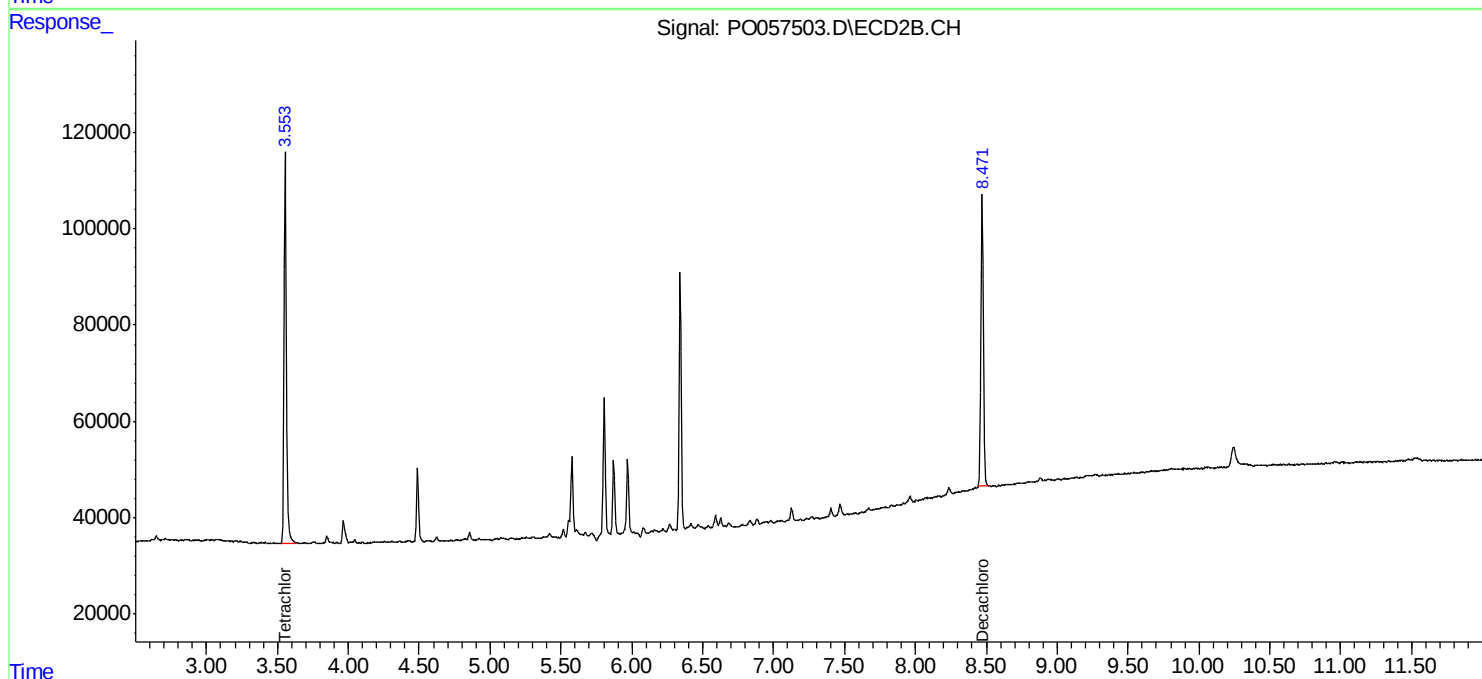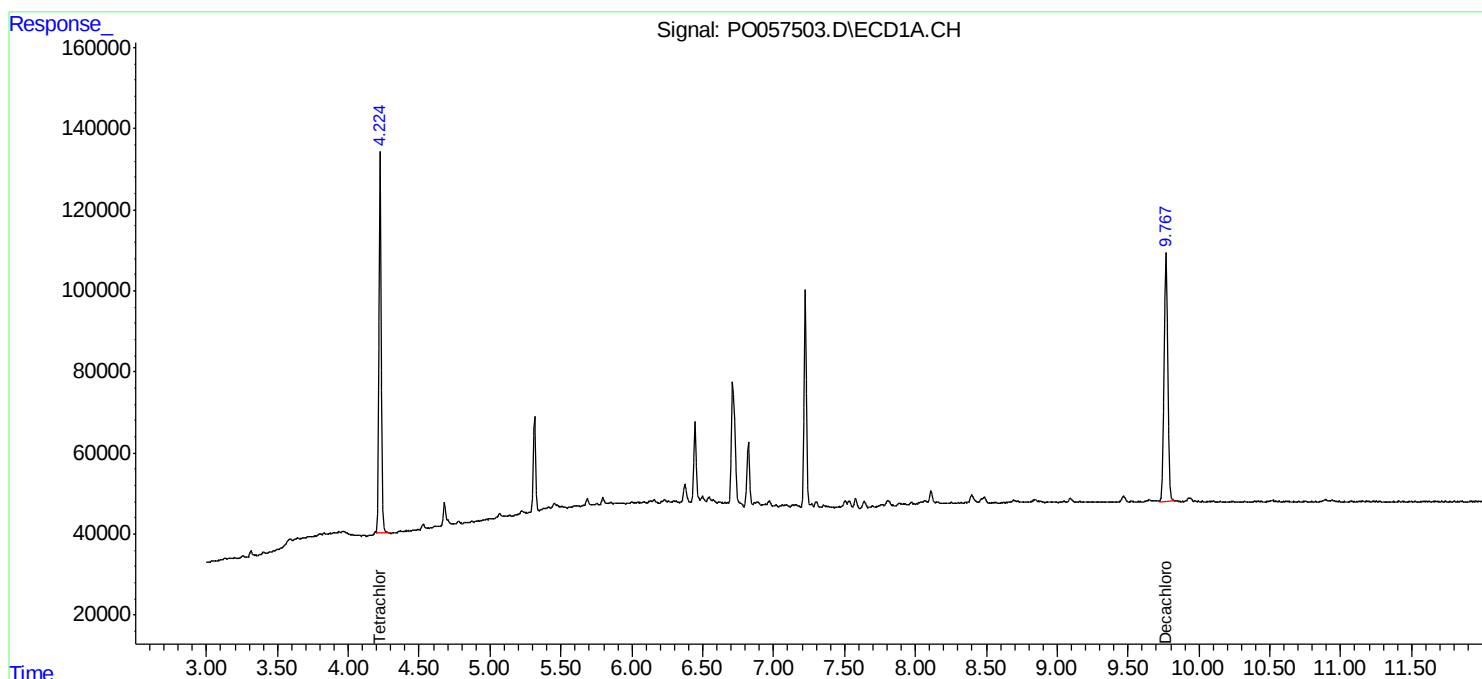

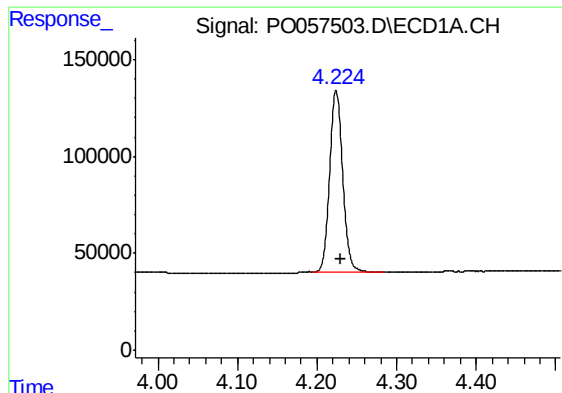


#1 Tetrachloro-m-xylene

R.T.: 4.224 min
Delta R.T.: -0.006 min
Response: 1062722
Conc: 27.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
SAMPLE-8


Manual Integrations
APPROVED

Ankita
6/27/2019 12:19:50 PM

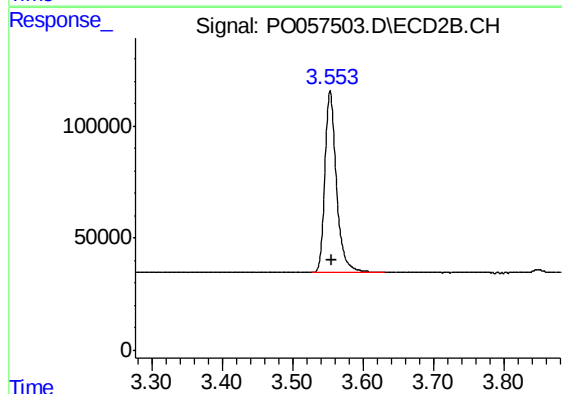


#1 Tetrachloro-m-xylene

R.T.: 3.554 min
Delta R.T.: -0.002 min
Response: 934948
Conc: 26.59 ng/ml

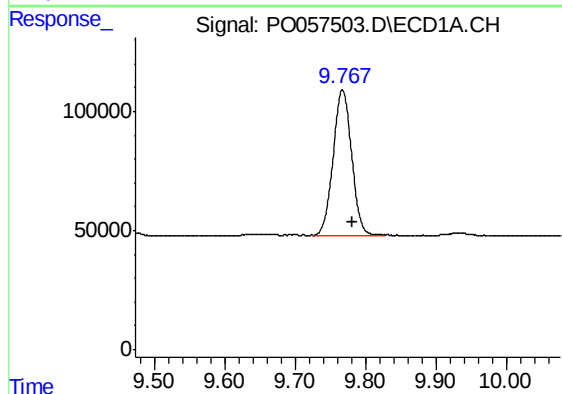

#2 Decachlorobiphenyl

R.T.: 9.767 min
Delta R.T.: -0.015 min
Response: 1112744
Conc: 19.79 ng/ml m

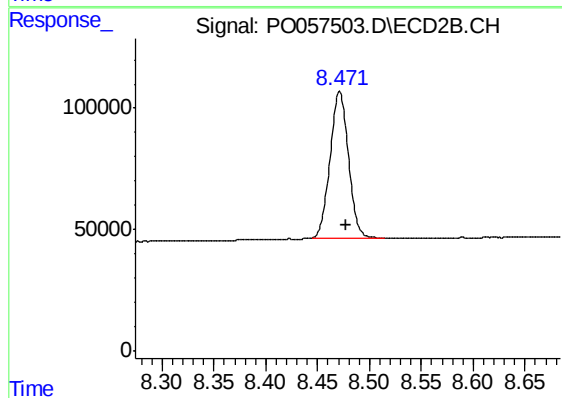

#2 Decachlorobiphenyl

R.T.: 8.471 min
Delta R.T.: -0.006 min
Response: 747527
Conc: 19.98 ng/ml