

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062619\
 Data File : P0057510.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jun 2019 21:41
 Operator : SM/SJ
 Sample : K3528-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-07-COMP

Manual Integrations
 APPROVED

Ankita
 6/27/2019 12:19:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 04:59:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.223	3.553	861517	747980	21.932	21.272
2)	SA Decachlor...	9.766	8.468	833349	565032	14.820m	15.105m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062619\
Data File : P0057510.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jun 2019 21:41
Operator : SM/SJ
Sample : K3528-04
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-07-COMP


Manual Integrations
APPROVED

Ankita
6/27/2019 12:19:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 04:59:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

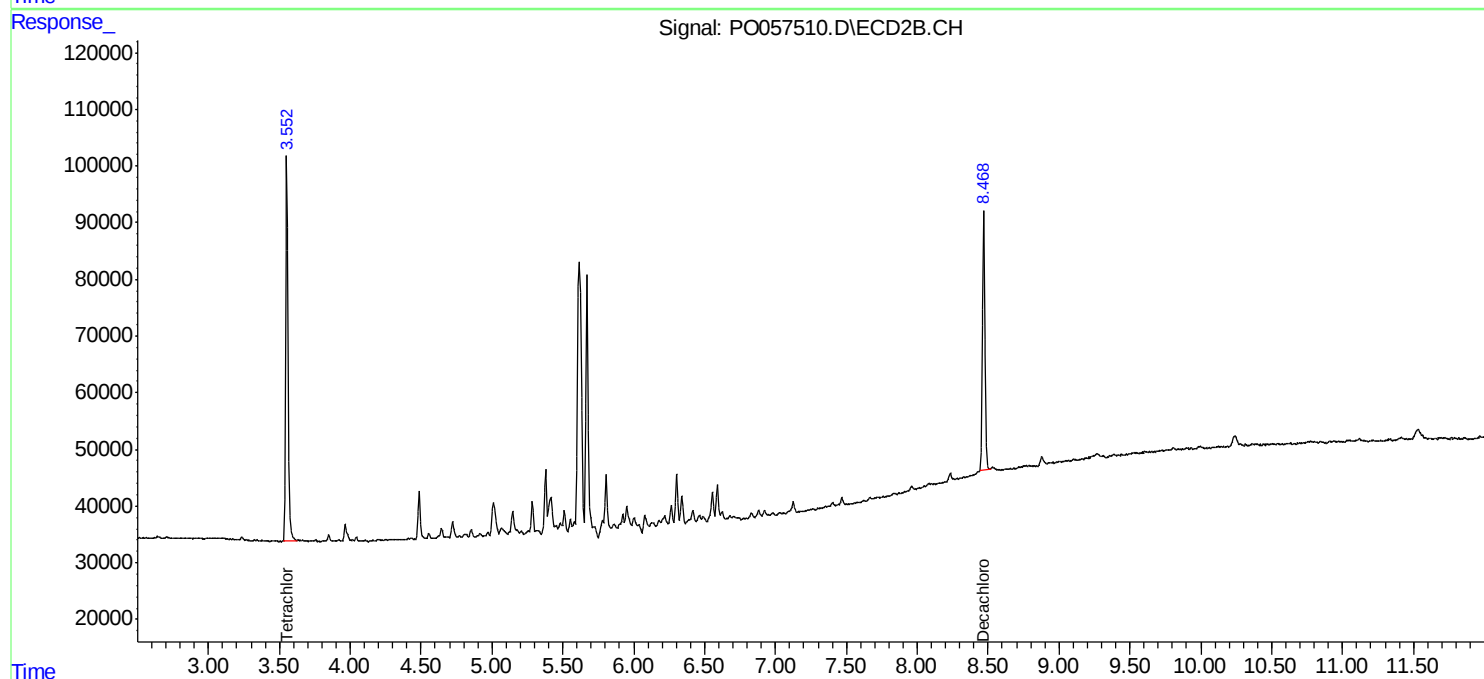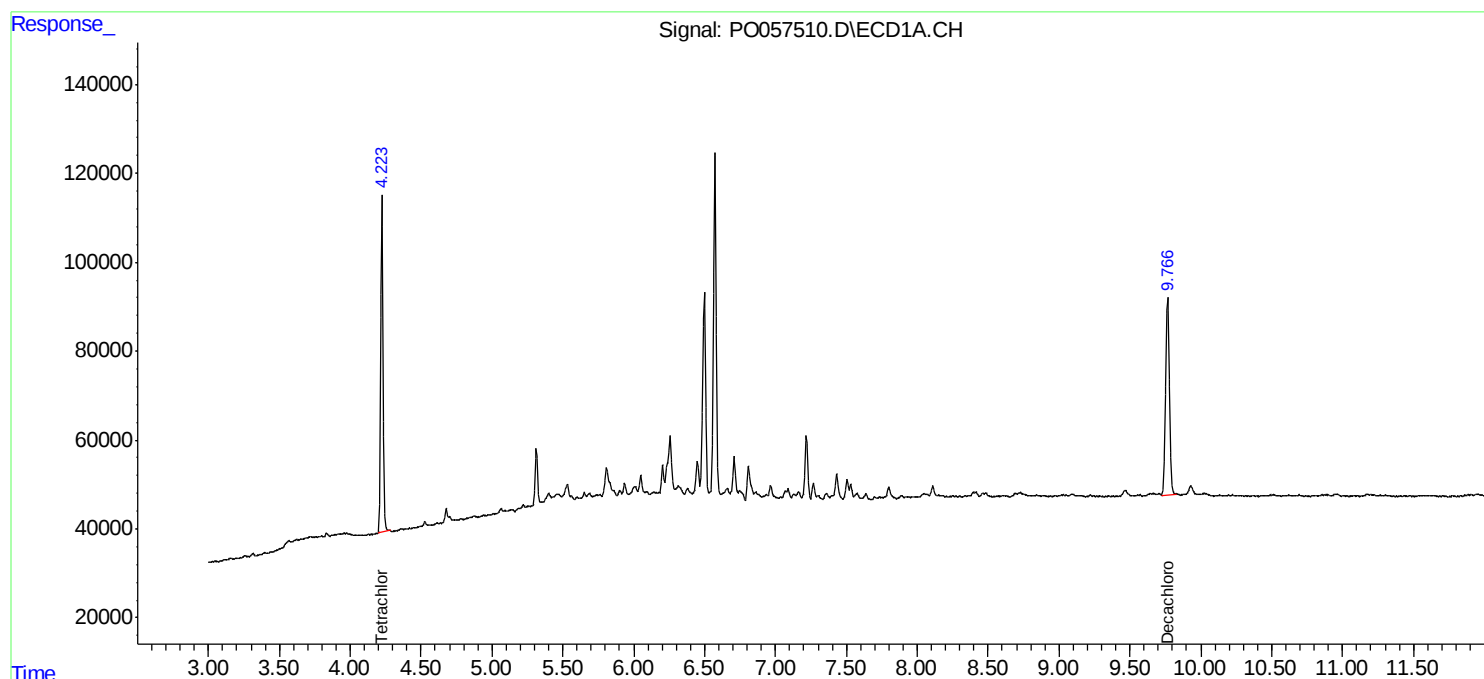

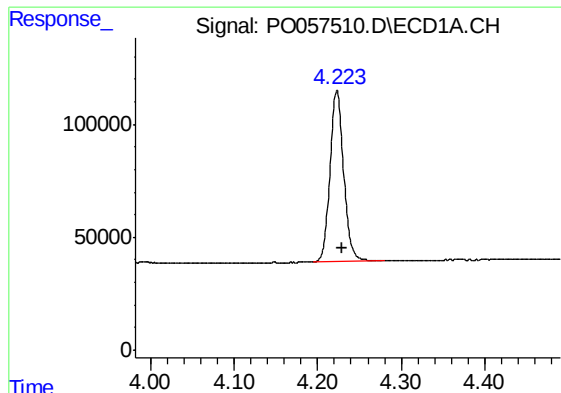


#1 Tetrachloro-m-xylene

R.T.: 4.223 min
Delta R.T.: -0.007 min
Response: 861517
Conc: 21.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-07-COMP


Manual Integrations
APPROVED

Ankita
6/27/2019 12:19:59 PM

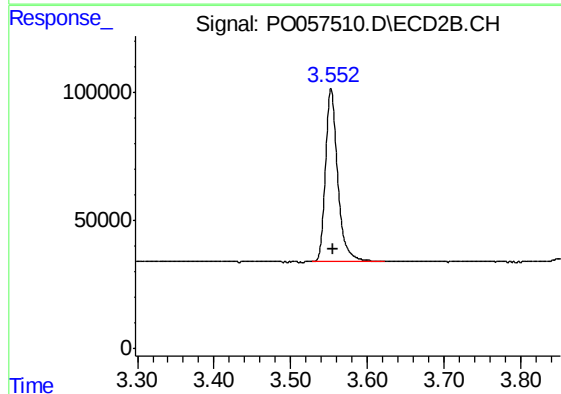


#1 Tetrachloro-m-xylene

R.T.: 3.553 min
Delta R.T.: -0.003 min
Response: 747980
Conc: 21.27 ng/ml

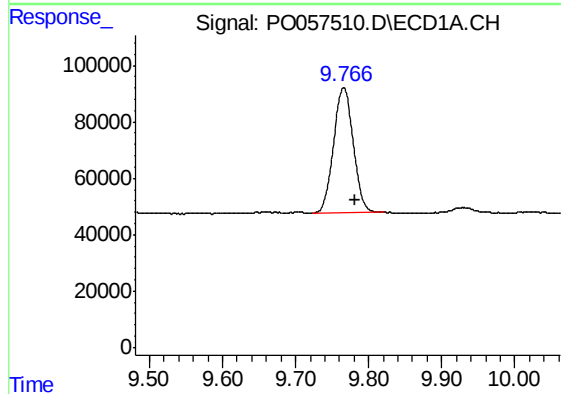

#2 Decachlorobiphenyl

R.T.: 9.766 min
Delta R.T.: -0.016 min
Response: 833349
Conc: 14.82 ng/ml m

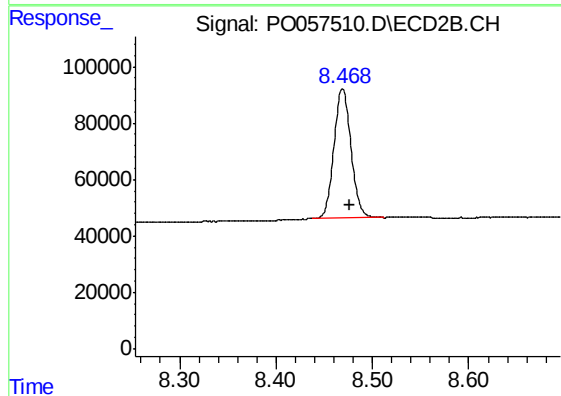

#2 Decachlorobiphenyl

R.T.: 8.468 min
Delta R.T.: -0.008 min
Response: 565032
Conc: 15.11 ng/ml m