

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062619\
 Data File : P0057519.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jun 2019 3:25
 Operator : SM/SJ
 Sample : K3530-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-02-044-B

Manual Integrations
 APPROVED

Ankita
 6/27/2019 12:20:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 05:02:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.225	3.553	1011314	849004	25.745m	24.145
2)	SA Decachlor...	9.768	8.471	998424	650677	17.755m	17.395
Target Compounds							
31)	L7 AR-1260-1	6.968	6.079	256885	208326	92.692	97.335
32)	L7 AR-1260-2	7.224	6.266	930644	282037	252.440	102.797 #
33)	L7 AR-1260-3	7.580	6.417	237471	241457	78.163	98.897 #
34)	L7 AR-1260-4	7.805	6.883	233690	159564	77.056	76.638
35)	L7 AR-1260-5	8.111	7.126	415238	347473	66.400	68.506

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062619\
Data File : PO057519.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jun 2019 3:25
Operator : SM/SJ
Sample : K3530-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
FK-GF-02-044-B


Manual Integrations
APPROVED

Ankita
6/27/2019 12:20:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 05:02:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

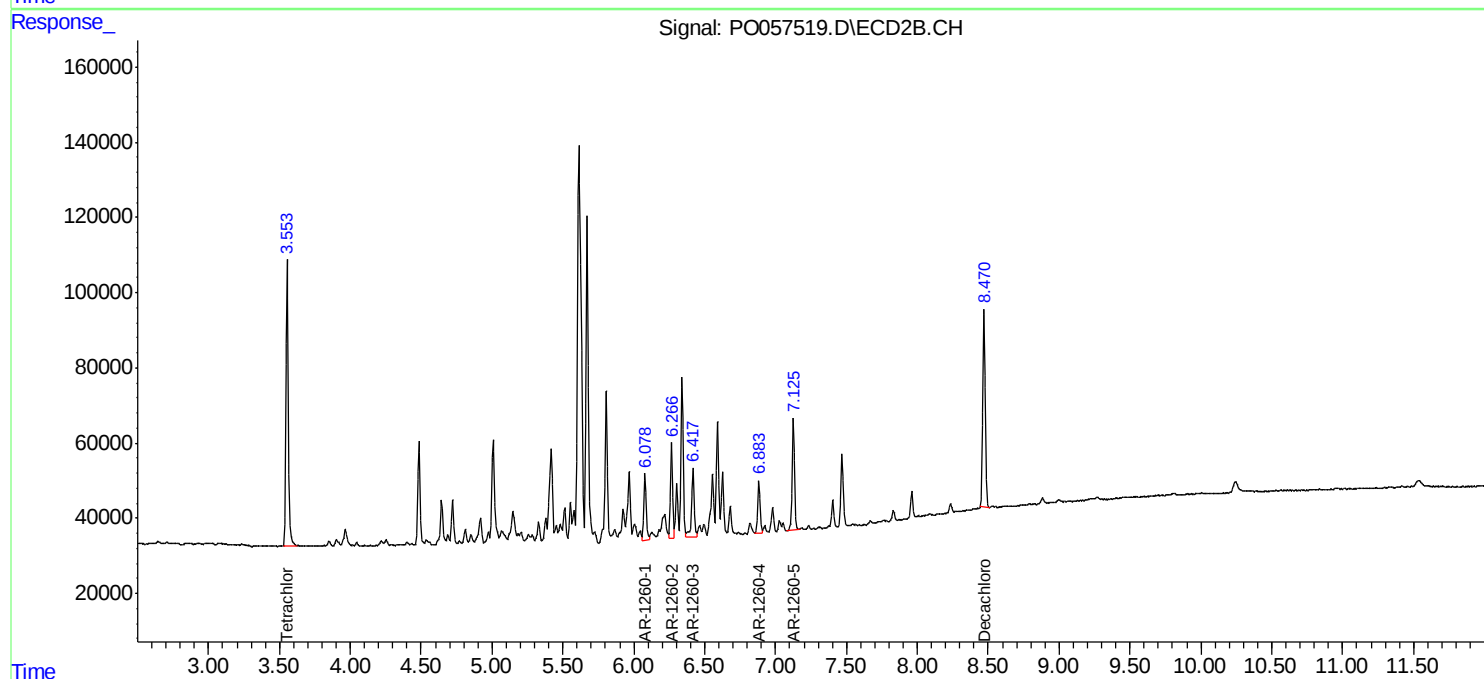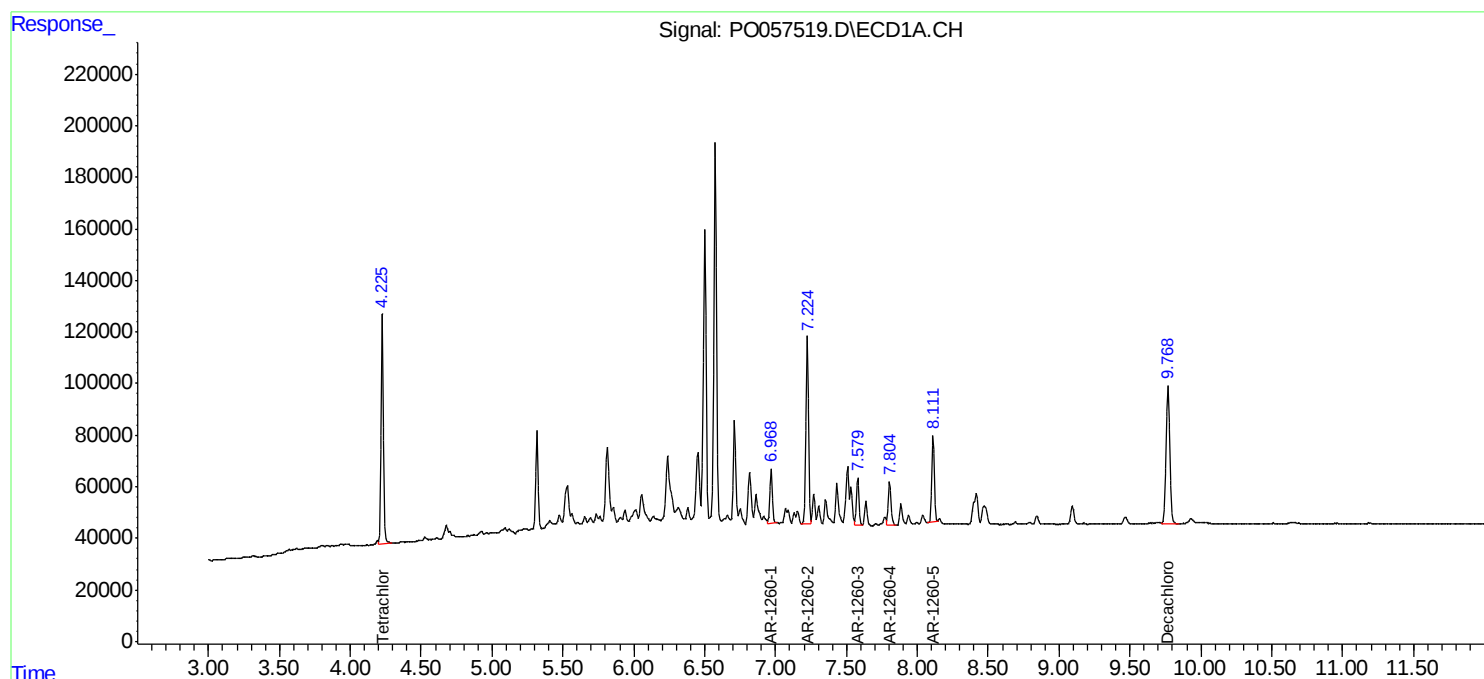

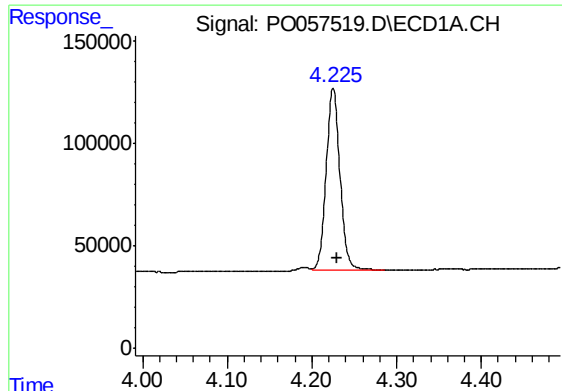


#1 Tetrachloro-m-xylene

R.T.: 4.225 min
Delta R.T.: -0.005 min
Response: 1011314
Conc: 25.75 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-044-B


Manual Integrations
APPROVED

Ankita
6/27/2019 12:20:46 PM

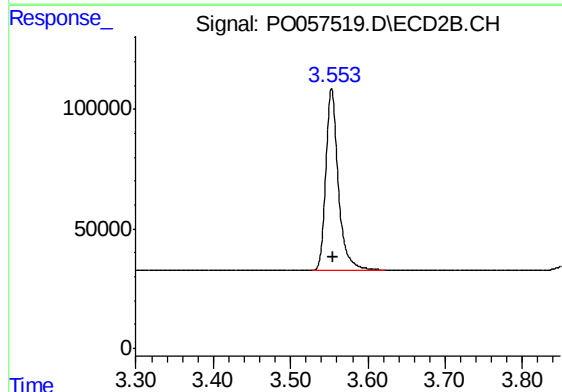


#1 Tetrachloro-m-xylene

R.T.: 3.553 min
Delta R.T.: -0.002 min
Response: 849004
Conc: 24.14 ng/ml

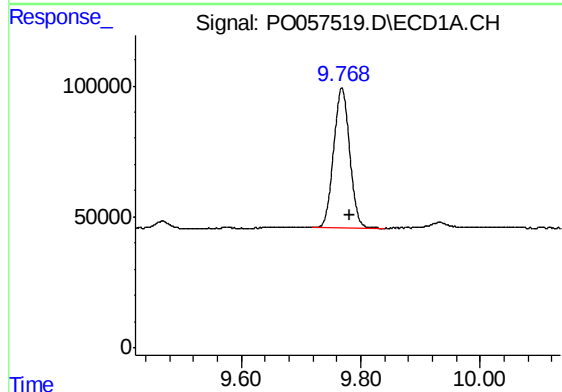


#2 Decachlorobiphenyl

R.T.: 9.768 min
Delta R.T.: -0.014 min
Response: 998424
Conc: 17.76 ng/ml m

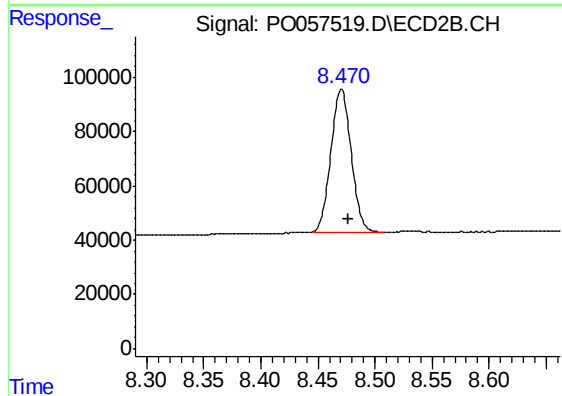

#2 Decachlorobiphenyl

R.T.: 8.471 min
Delta R.T.: -0.006 min
Response: 650677
Conc: 17.39 ng/ml

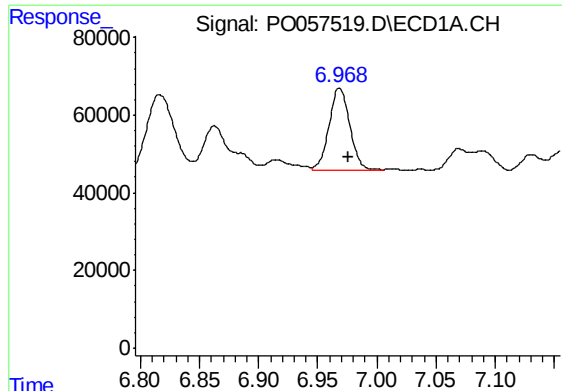


#31 AR-1260-1

R.T.: 6.968 min
Delta R.T.: -0.007 min
Response: 256885
Conc: 92.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-044-B


Manual Integrations
APPROVED

Ankita
6/27/2019 12:20:46 PM

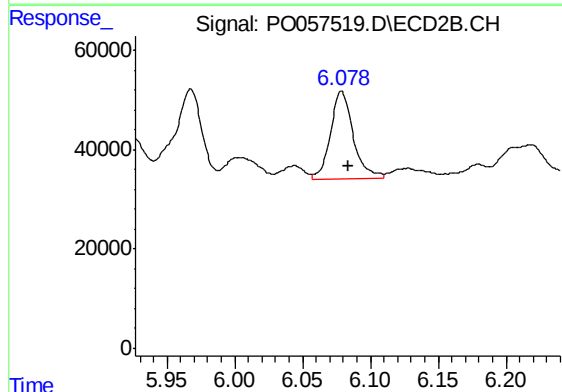


#31 AR-1260-1

R.T.: 6.079 min
Delta R.T.: -0.005 min
Response: 208326
Conc: 97.34 ng/ml

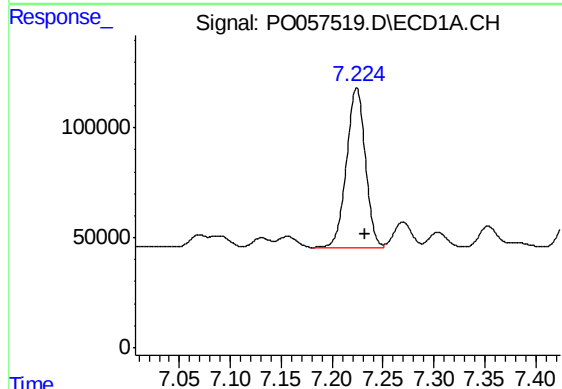


#32 AR-1260-2

R.T.: 7.224 min
Delta R.T.: -0.008 min
Response: 930644
Conc: 252.44 ng/ml

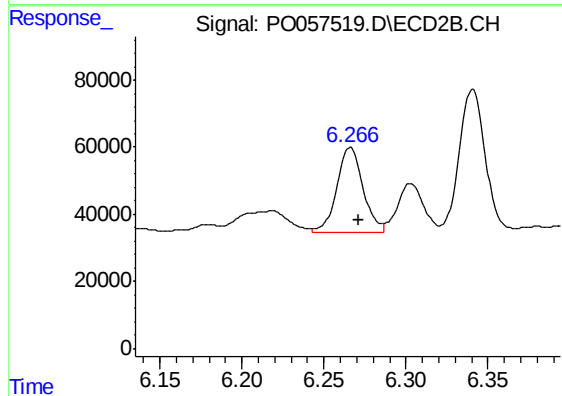

#32 AR-1260-2

R.T.: 6.266 min
Delta R.T.: -0.005 min
Response: 282037
Conc: 102.80 ng/ml

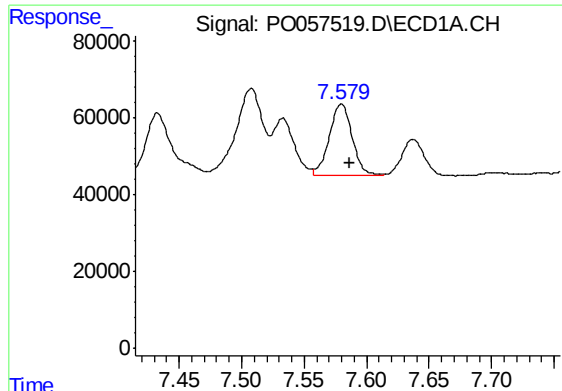


#33 AR-1260-3

R.T.: 7.580 min
Delta R.T.: -0.007 min
Response: 237471
Conc: 78.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-044-B


Manual Integrations
APPROVED

Ankita
6/27/2019 12:20:46 PM

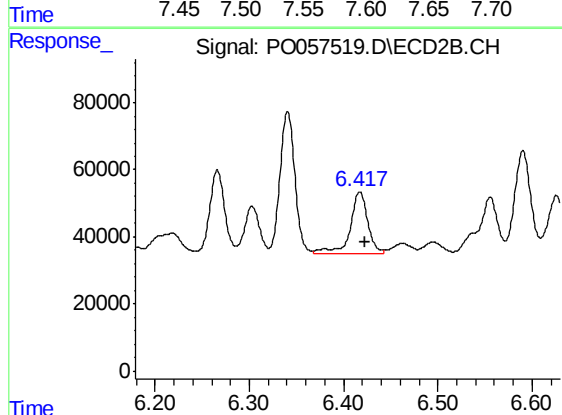


#33 AR-1260-3

R.T.: 6.417 min
Delta R.T.: -0.006 min
Response: 241457
Conc: 98.90 ng/ml

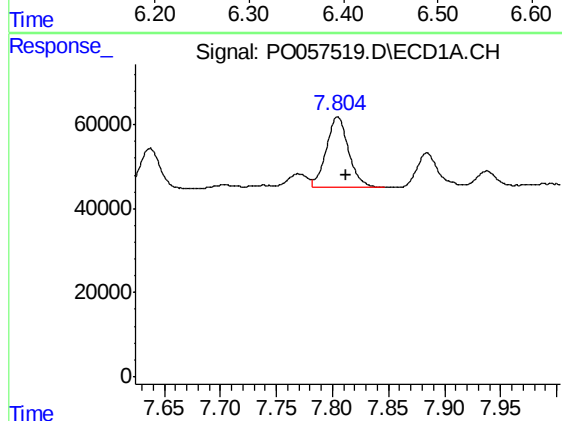


#34 AR-1260-4

R.T.: 7.805 min
Delta R.T.: -0.007 min
Response: 233690
Conc: 77.06 ng/ml

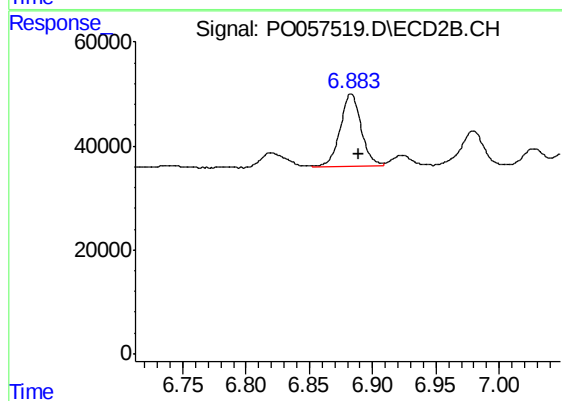

#34 AR-1260-4

R.T.: 6.883 min
Delta R.T.: -0.006 min
Response: 159564
Conc: 76.64 ng/ml

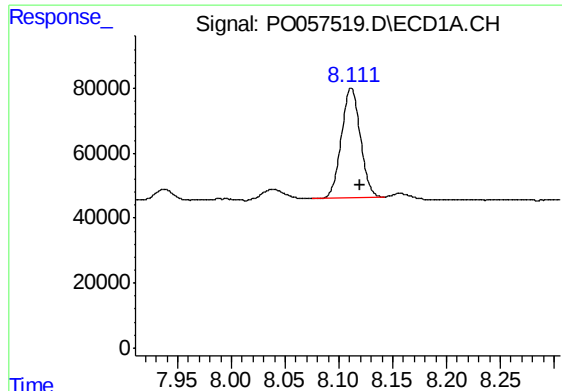


#35 AR-1260-5

R.T.: 8.111 min
Delta R.T.: -0.008 min
Response: 415238
Conc: 66.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-044-B

Manual Integrations
APPROVED

Ankita
6/27/2019 12:20:46 PM

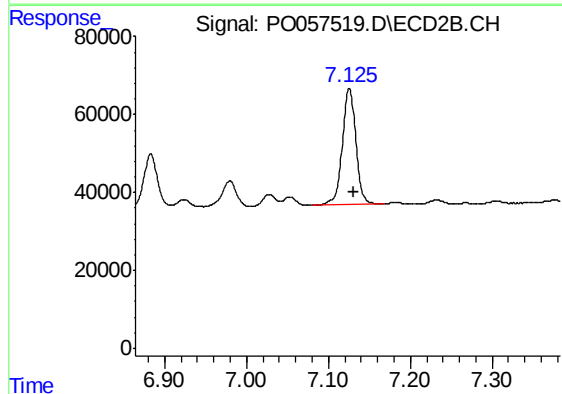

#35 AR-1260-5

R.T.: 7.126 min
Delta R.T.: -0.005 min
Response: 347473
Conc: 68.51 ng/ml