

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062619\
 Data File : P0057521.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jun 2019 3:59
 Operator : SM/SJ
 Sample : K3525-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HD-7-11(0.5-1.0)

Manual Integrations
 APPROVED

Ankita
 6/27/2019 12:20:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 05:02:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.223	3.554	945721	781644	24.075	22.229
2)	SA Decachlor...	9.765	8.470	750243	497001	13.342m	13.286
Target Compounds							
26)	L6 AR-1254-1	6.226	5.407	107585	86994	55.235m	40.905 #
27)	L6 AR-1254-2	6.442	5.553	151357	81307	48.562	43.684
28)	L6 AR-1254-3	6.807	5.950	156625	135546	47.375	45.014m
29)	L6 AR-1254-4	7.090	6.179	118209	78358	43.557	43.531m
30)	L6 AR-1254-5	7.506	6.589	116634	118576	41.716	43.769m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062619\
Data File : PO057521.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jun 2019 3:59
Operator : SM/SJ
Sample : K3525-02
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HD-7-11(0.5-1.0)


Manual Integrations
APPROVED

Ankita
6/27/2019 12:20:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 05:02:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

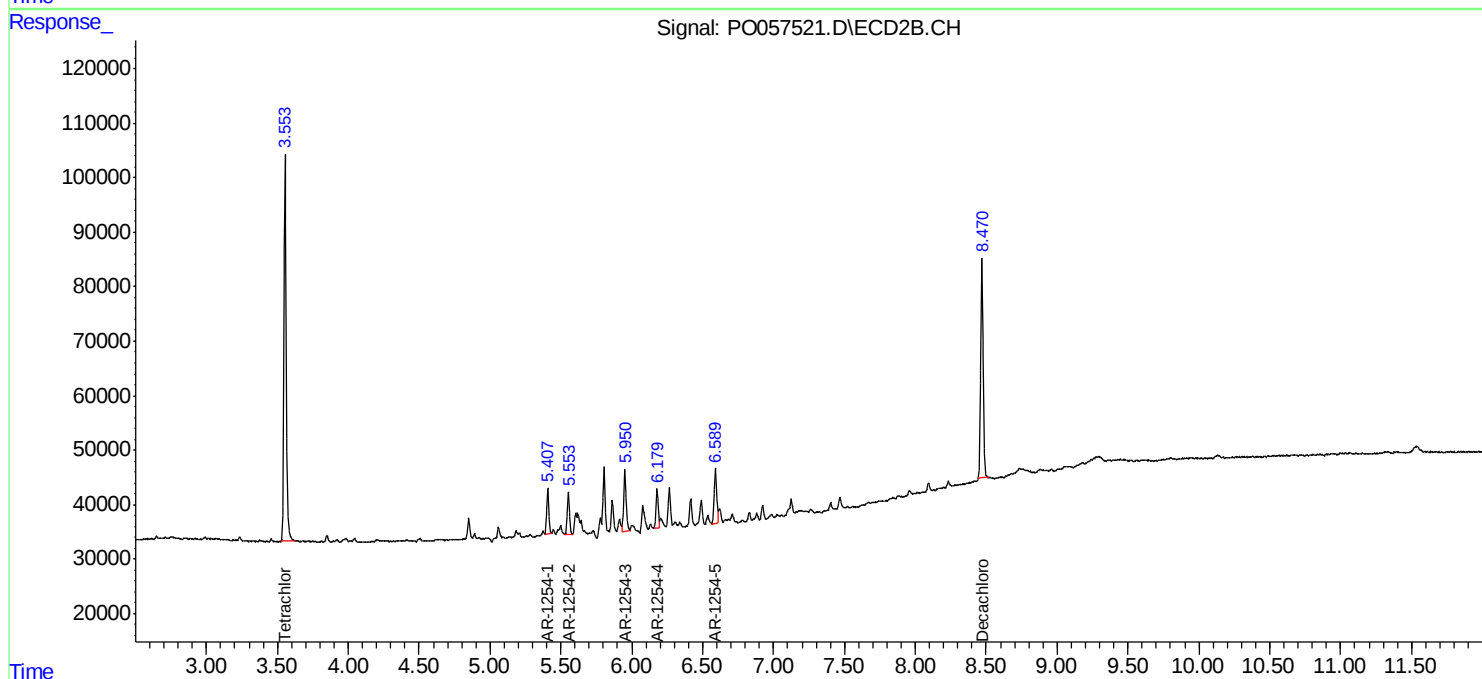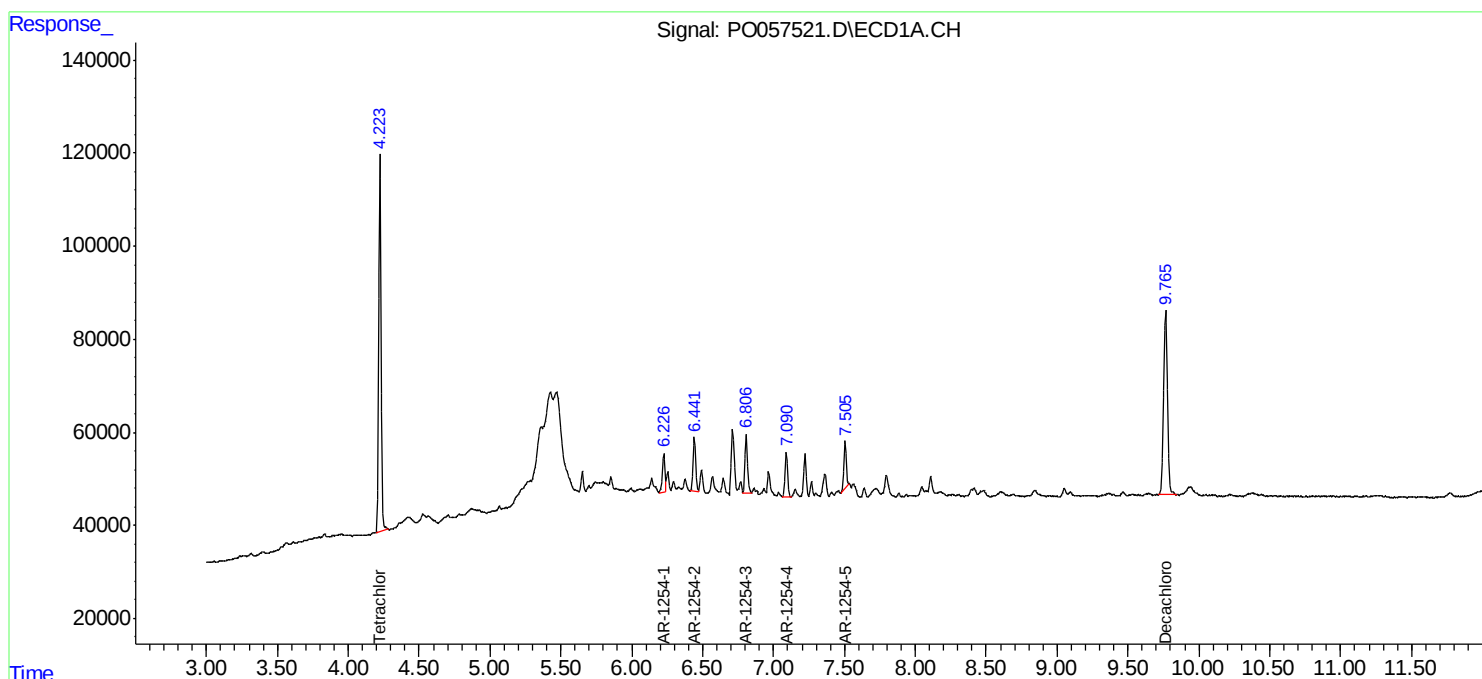

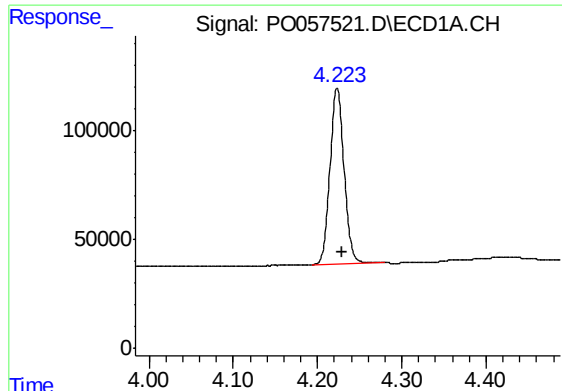


#1 Tetrachloro-m-xylene

R.T.: 4.223 min
Delta R.T.: -0.007 min
Response: 945721
Conc: 24.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-7-11(0.5-1.0)


Manual Integrations
APPROVED

Ankita
6/27/2019 12:20:10 PM

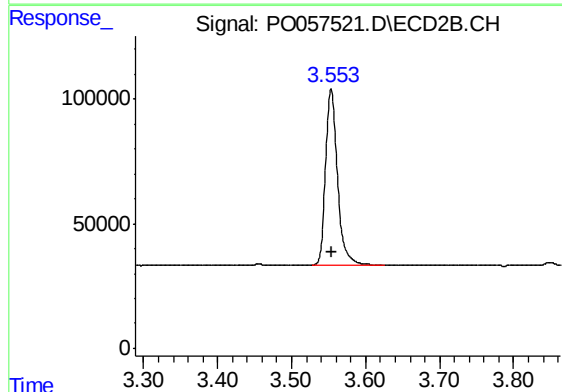


#1 Tetrachloro-m-xylene

R.T.: 3.554 min
Delta R.T.: -0.002 min
Response: 781644
Conc: 22.23 ng/ml

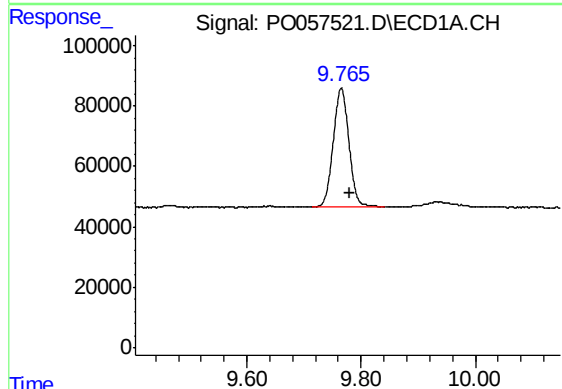


#2 Decachlorobiphenyl

R.T.: 9.765 min
Delta R.T.: -0.017 min
Response: 750243
Conc: 13.34 ng/ml m

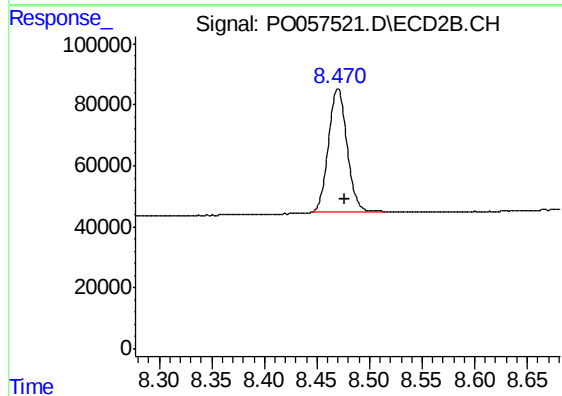

#2 Decachlorobiphenyl

R.T.: 8.470 min
Delta R.T.: -0.007 min
Response: 497001
Conc: 13.29 ng/ml

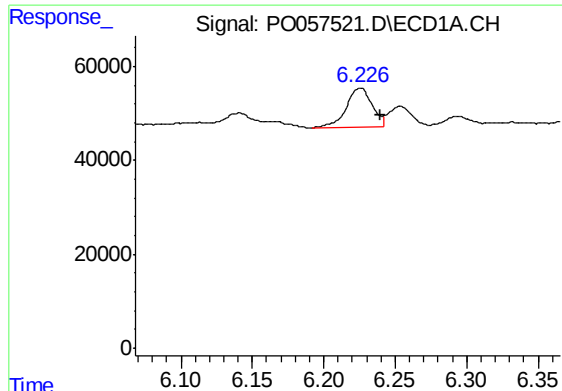


#26 AR-1254-1

R.T.: 6.226 min
Delta R.T.: -0.014 min
Response: 107585
Conc: 55.24 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HD-7-11(0.5-1.0)


Manual Integrations
APPROVED

Ankita
6/27/2019 12:20:10 PM

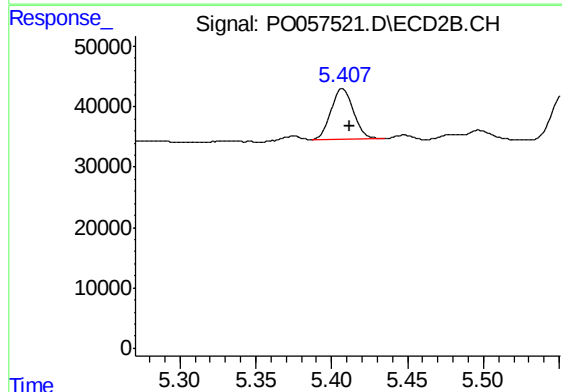


#26 AR-1254-1

R.T.: 5.407 min
Delta R.T.: -0.005 min
Response: 86994
Conc: 40.91 ng/ml

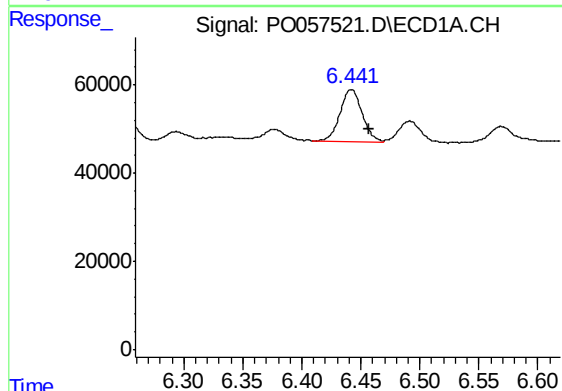


#27 AR-1254-2

R.T.: 6.442 min
Delta R.T.: -0.015 min
Response: 151357
Conc: 48.56 ng/ml

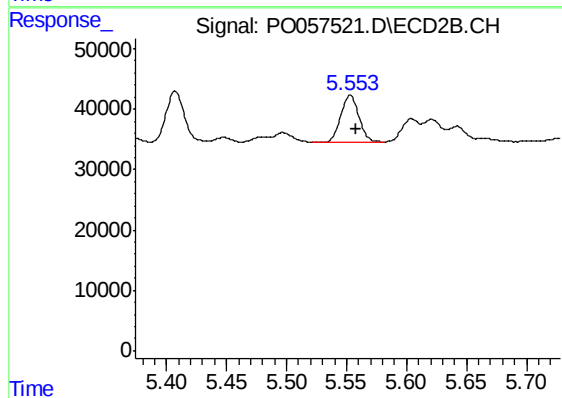

#27 AR-1254-2

R.T.: 5.553 min
Delta R.T.: -0.005 min
Response: 81307
Conc: 43.68 ng/ml

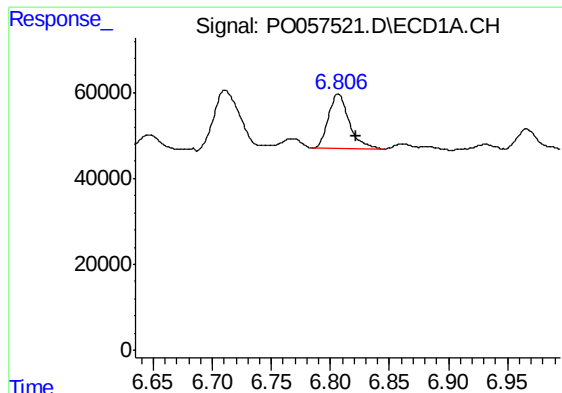


#28 AR-1254-3

R.T.: 6.807 min
Delta R.T.: -0.016 min
Response: 156625
Conc: 47.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-7-11(0.5-1.0)


Manual Integrations
APPROVED

Ankita
6/27/2019 12:20:10 PM

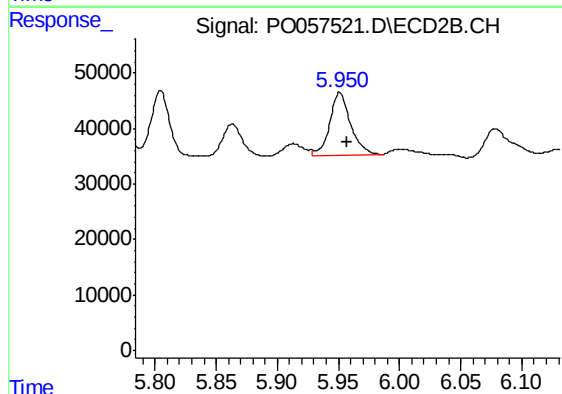


#28 AR-1254-3

R.T.: 5.950 min
Delta R.T.: -0.007 min
Response: 135546
Conc: 45.01 ng/ml m

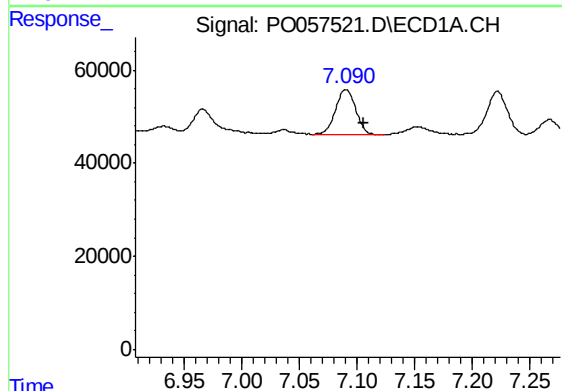


#29 AR-1254-4

R.T.: 7.090 min
Delta R.T.: -0.016 min
Response: 118209
Conc: 43.56 ng/ml

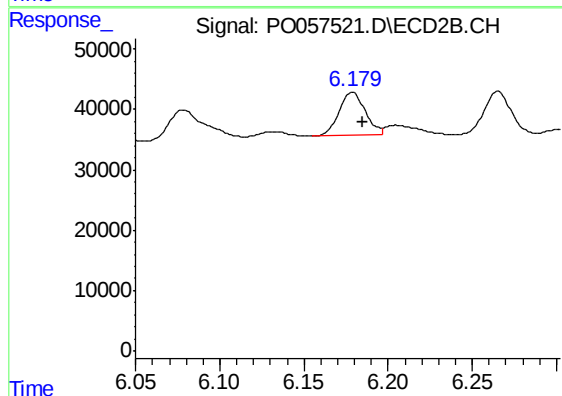

#29 AR-1254-4

R.T.: 6.179 min
Delta R.T.: -0.006 min
Response: 78358
Conc: 43.53 ng/ml m

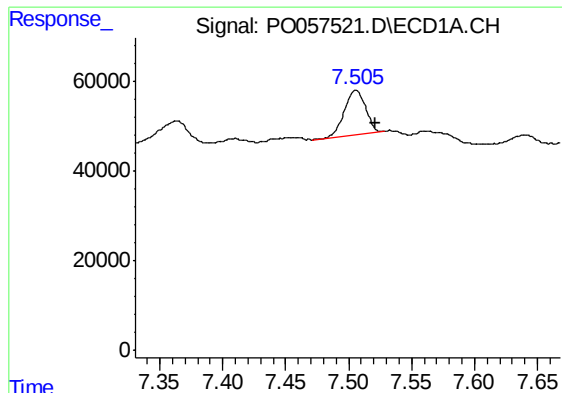


#30 AR-1254-5

R.T.: 7.506 min
Delta R.T.: -0.015 min
Response: 116634
Conc: 41.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-7-11(0.5-1.0)

Manual Integrations
APPROVED

Ankita
6/27/2019 12:20:10 PM

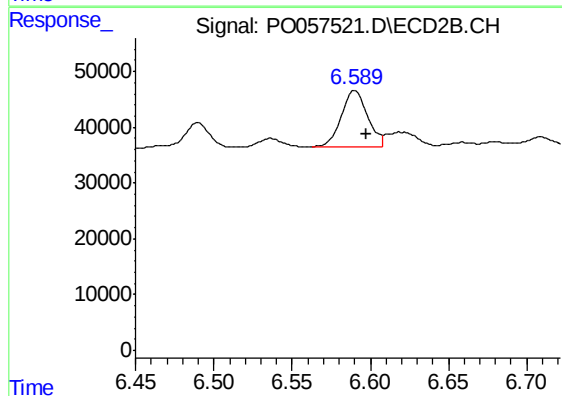

#30 AR-1254-5

R.T.: 6.589 min
Delta R.T.: -0.008 min
Response: 118576
Conc: 43.77 ng/ml m