

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062619\
 Data File : P0057523.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jun 2019 4:33
 Operator : SM/SJ
 Sample : K3525-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HD-8-1(0.5-1.0)

Manual Integrations
 APPROVED

Ankita
 6/27/2019 12:20:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 05:03:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.222	3.553	979016	820108	24.923	23.323
2)	SA Decachlor...	9.763	8.468	1006662	683766	17.902m	18.279m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062619\
Data File : P0057523.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jun 2019 4:33
Operator : SM/SJ
Sample : K3525-04
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HD-8-1(0.5-1.0)


Manual Integrations
APPROVED

Ankita
6/27/2019 12:20:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 05:03:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

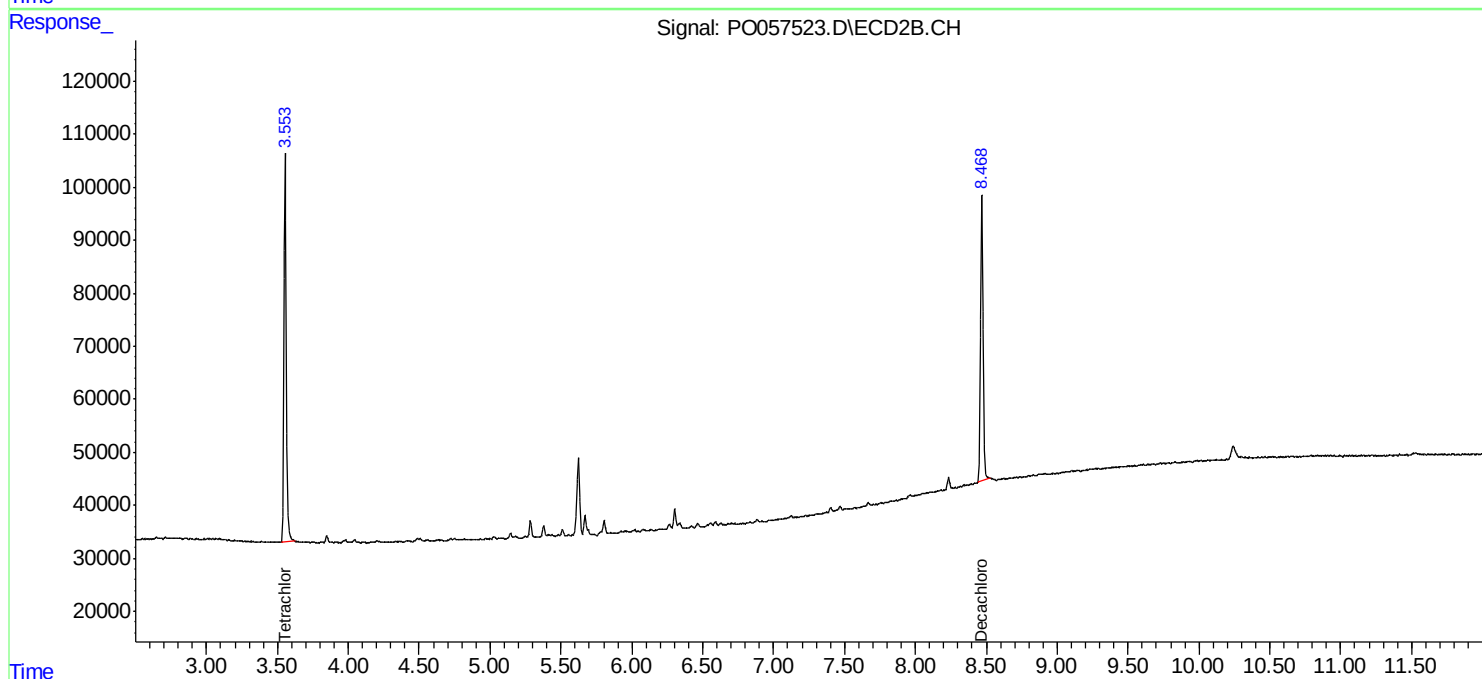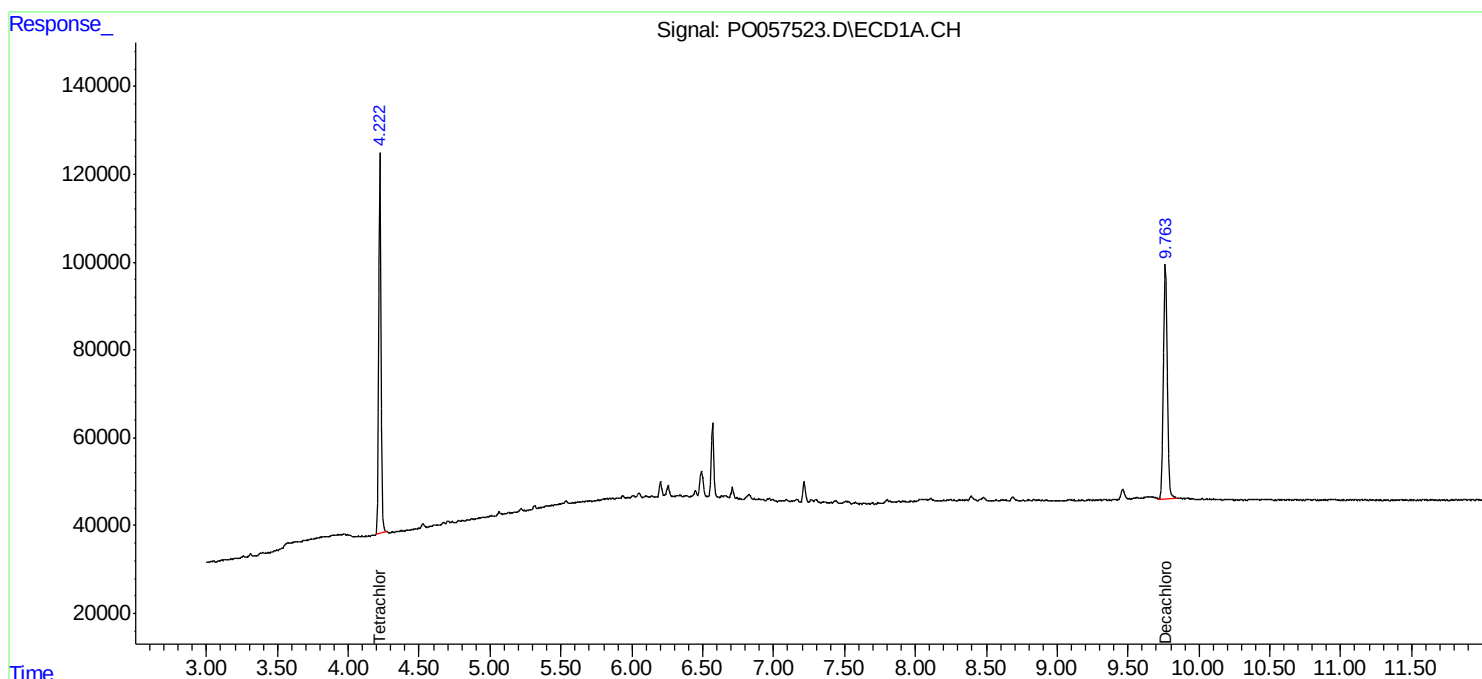

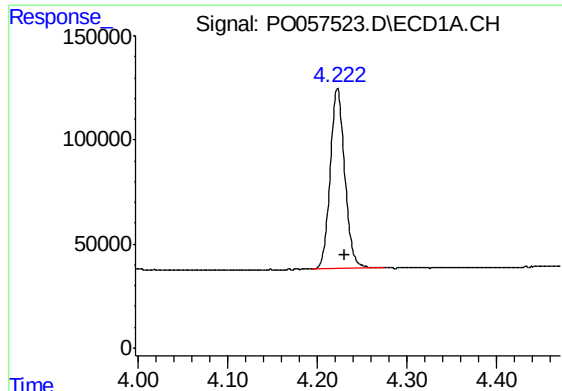


#1 Tetrachloro-m-xylene

R.T.: 4.222 min
Delta R.T.: -0.008 min
Response: 979016
Conc: 24.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-8-1(0.5-1.0)


Manual Integrations
APPROVED

Ankita
6/27/2019 12:20:13 PM

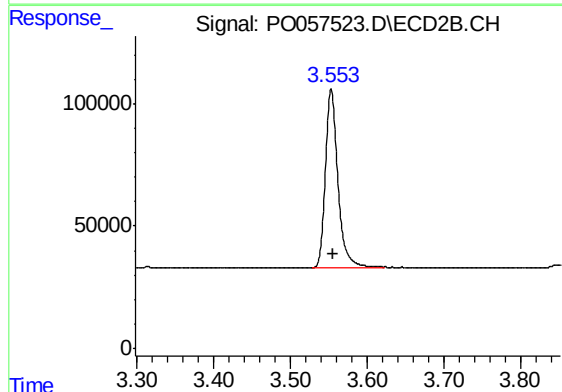


#1 Tetrachloro-m-xylene

R.T.: 3.553 min
Delta R.T.: -0.002 min
Response: 820108
Conc: 23.32 ng/ml

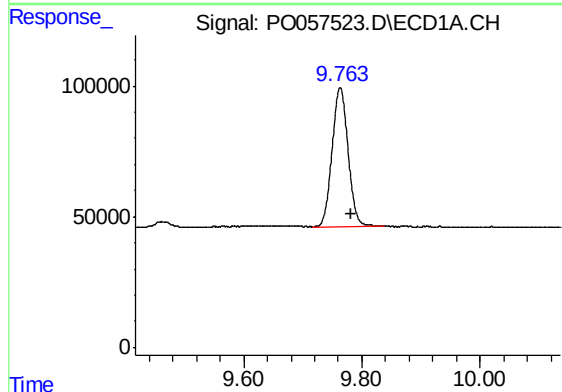

#2 Decachlorobiphenyl

R.T.: 9.763 min
Delta R.T.: -0.018 min
Response: 1006662
Conc: 17.90 ng/ml m

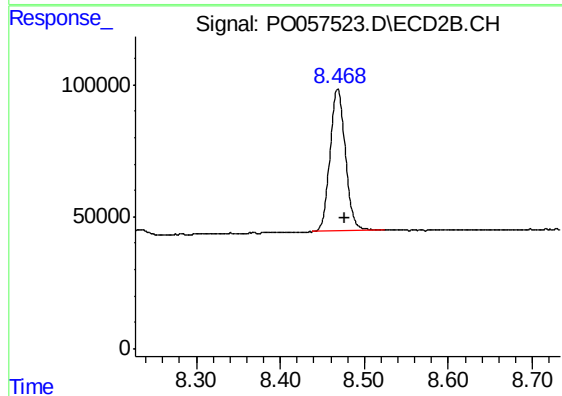

#2 Decachlorobiphenyl

R.T.: 8.468 min
Delta R.T.: -0.009 min
Response: 683766
Conc: 18.28 ng/ml m