

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062623\
 Data File : P0095969.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2023 12:19
 Operator : YP/AJ
 Sample : 03381-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP1-0622

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :Ankita Jodhani 06/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 21:53:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 21 13:08:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.424	3.644	36137530	16538552	12.420	12.186
2) SA Decachlor...	10.248	8.673	44589430	21235368	21.523m	17.318m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062623\
Data File : P0095969.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2023 12:19
Operator : YP/AJ
Sample : 03381-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP1-0622


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/27/2023
Supervised By :Ankita Jodhani 06/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 21:53:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 21 13:08:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

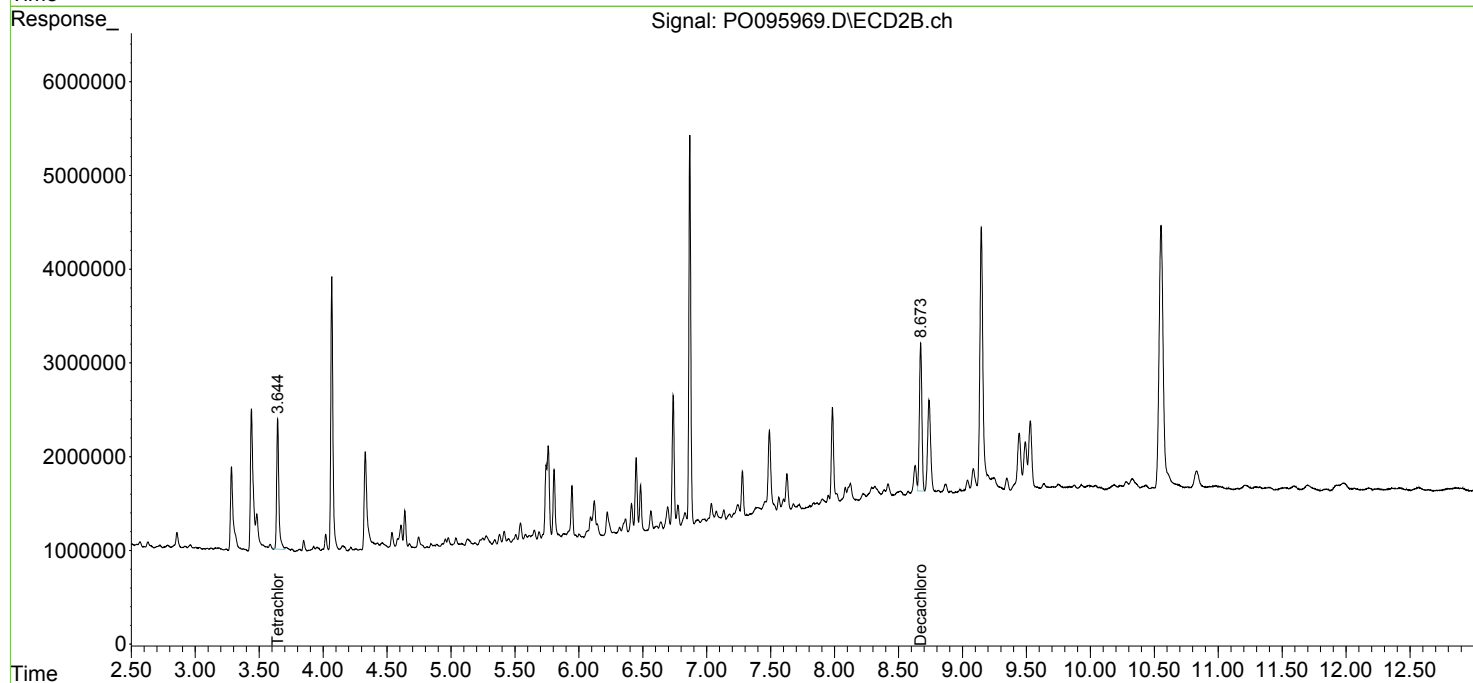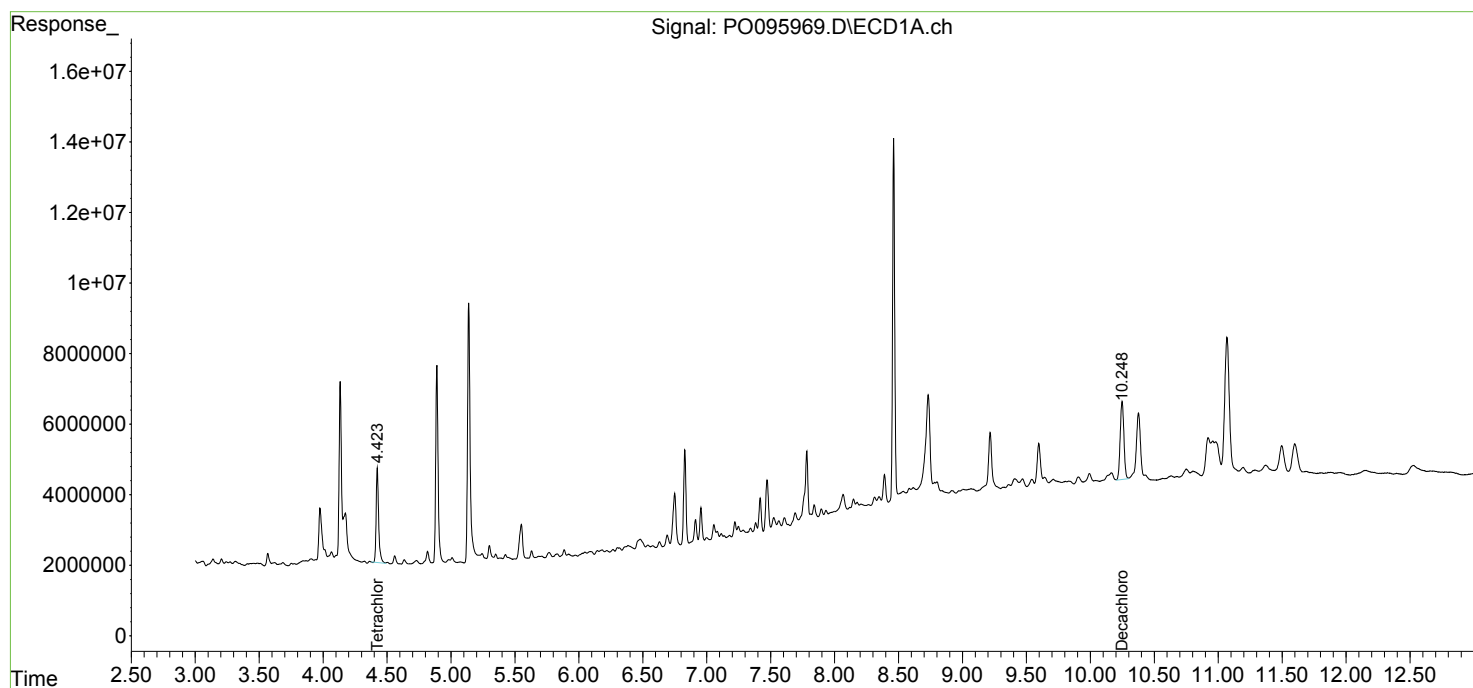

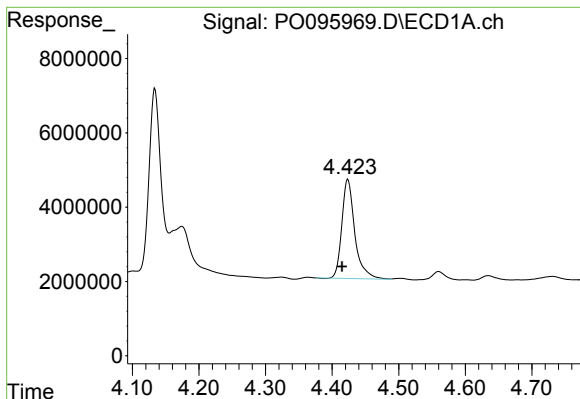


#1 Tetrachloro-m-xylene

R.T.: 4.424 min
Delta R.T.: 0.009 min
Response: 36137530
Conc: 12.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP1-0622


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/27/2023
Supervised By :Ankita Jodhani 06/27/2023

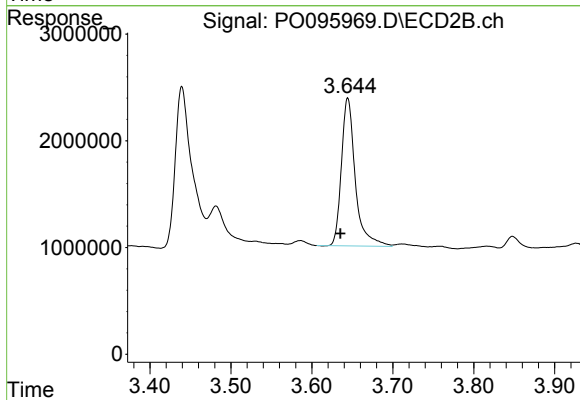


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: 0.009 min
Response: 16538552
Conc: 12.19 ng/ml

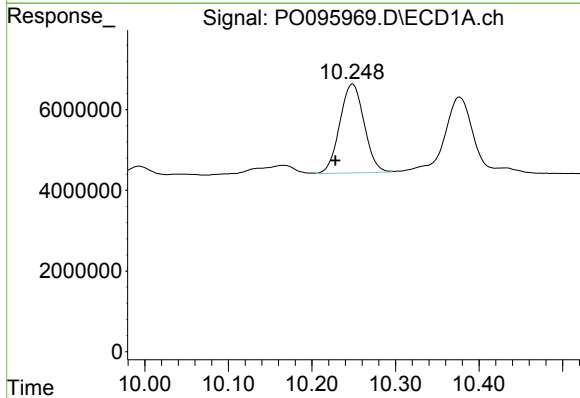

#2 Decachlorobiphenyl

R.T.: 10.248 min
Delta R.T.: 0.020 min
Response: 44589430
Conc: 21.52 ng/ml m

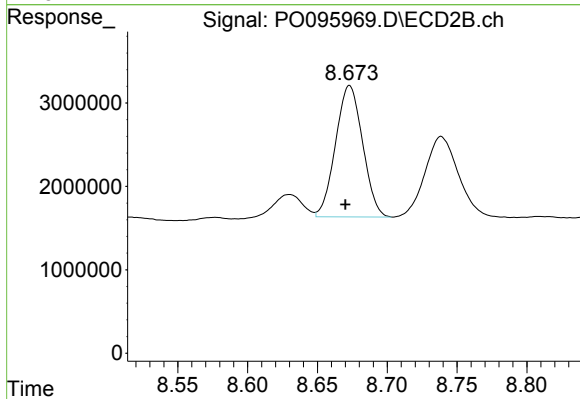

#2 Decachlorobiphenyl

R.T.: 8.673 min
Delta R.T.: 0.002 min
Response: 21235368
Conc: 17.32 ng/ml m