

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062623\
 Data File : P0095970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2023 12:36
 Operator : YP/AJ
 Sample : 03381-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP2-0622

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/27/2023
 Supervised By :Ankita Jodhani 06/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 21:54:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 21 13:08:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.421	3.640	40477979	18375024	13.912	13.539
2) SA Decachlor...	10.250	8.674	48233989	26205194	23.282	21.371m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062623\
Data File : P0095970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2023 12:36
Operator : YP/AJ
Sample : 03381-02
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP2-0622


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/27/2023
Supervised By :Ankita Jodhani 06/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 21:54:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 21 13:08:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

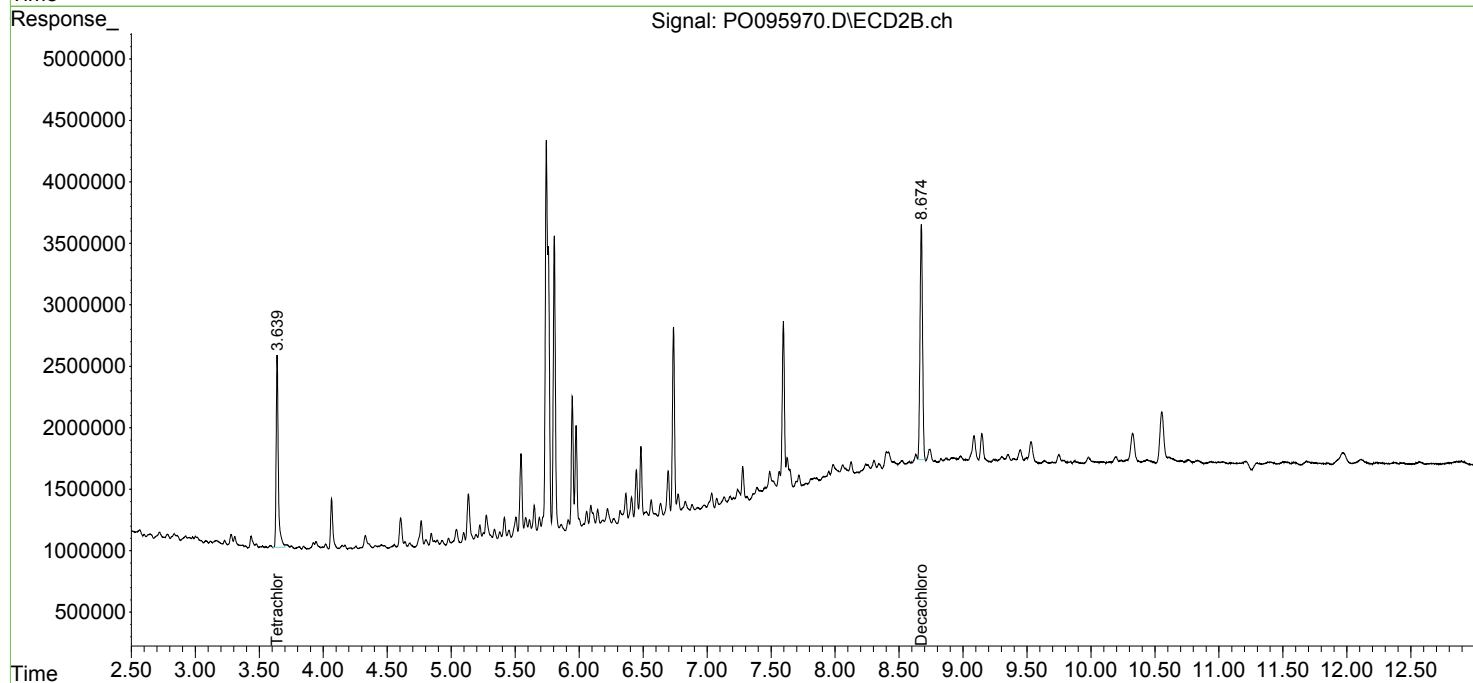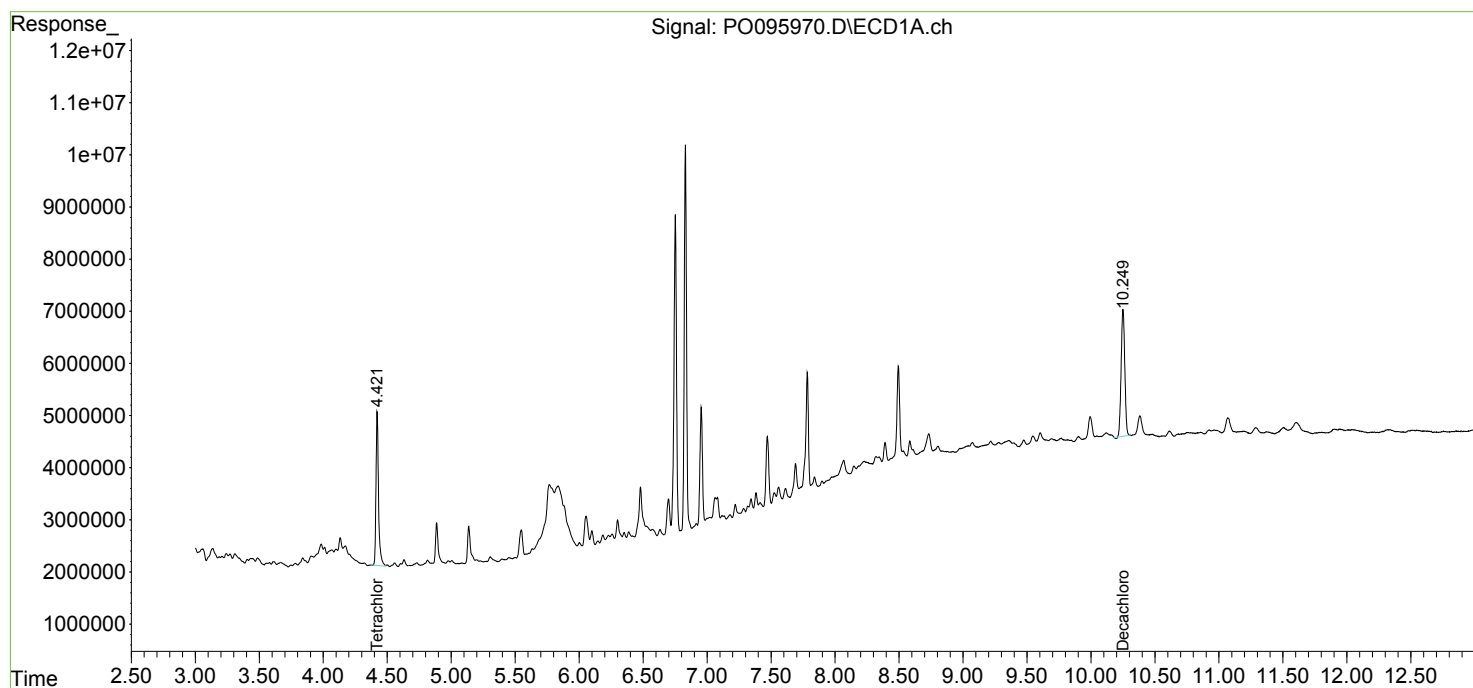

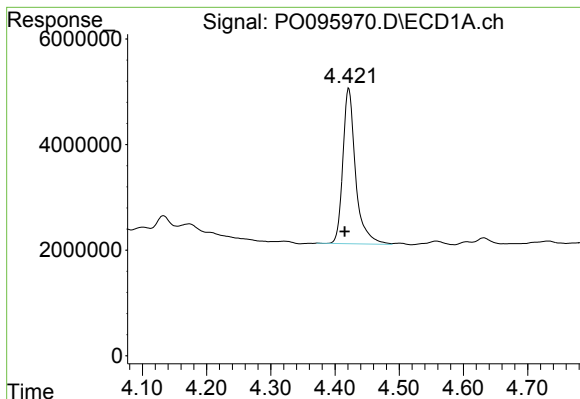

#1 Tetrachloro-m-xylene

R.T.: 4.421 min
Delta R.T.: 0.006 min
Response: 40477979
Conc: 13.91 ng/ml

Instrument :

ECD_O


ClientSampleId :

COMP2-0622

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 06/27/2023
Supervised By :Ankita Jodhani 06/27/2023

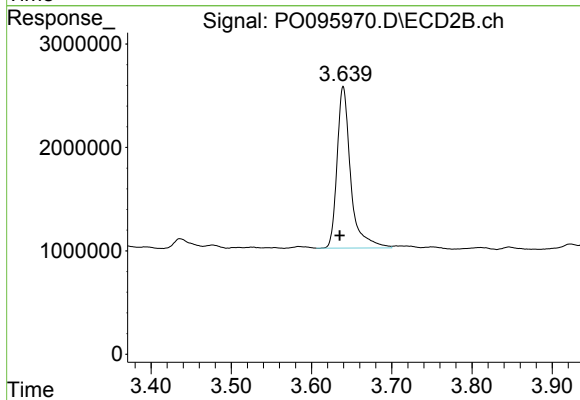


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: 0.004 min
Response: 18375024
Conc: 13.54 ng/ml

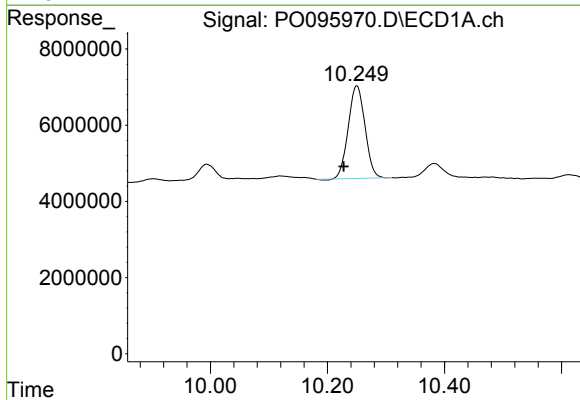

#2 Decachlorobiphenyl

R.T.: 10.250 min
Delta R.T.: 0.022 min
Response: 48233989
Conc: 23.28 ng/ml

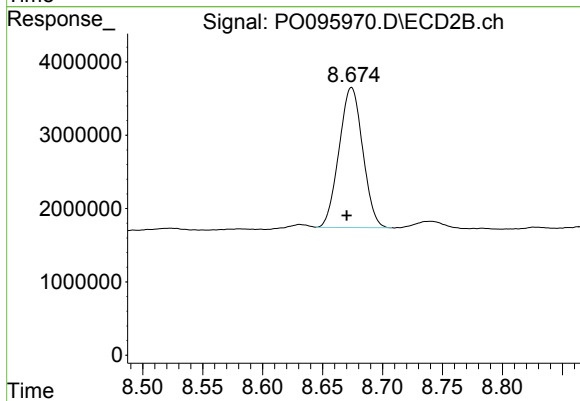

#2 Decachlorobiphenyl

R.T.: 8.674 min
Delta R.T.: 0.004 min
Response: 26205194
Conc: 21.37 ng/ml m