

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062719\
Data File : P0057533.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jun 2019 10:26
Operator : SM/SJ
Sample : K3530-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-044-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:01:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.227	3.551	882737	742441	22.472	21.114
2) SA Decachlor...	9.768	8.468	904085	592931	16.077	15.851

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062719\
Data File : PO057533.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jun 2019 10:26
Operator : SM/SJ
Sample : K3530-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-044-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:01:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

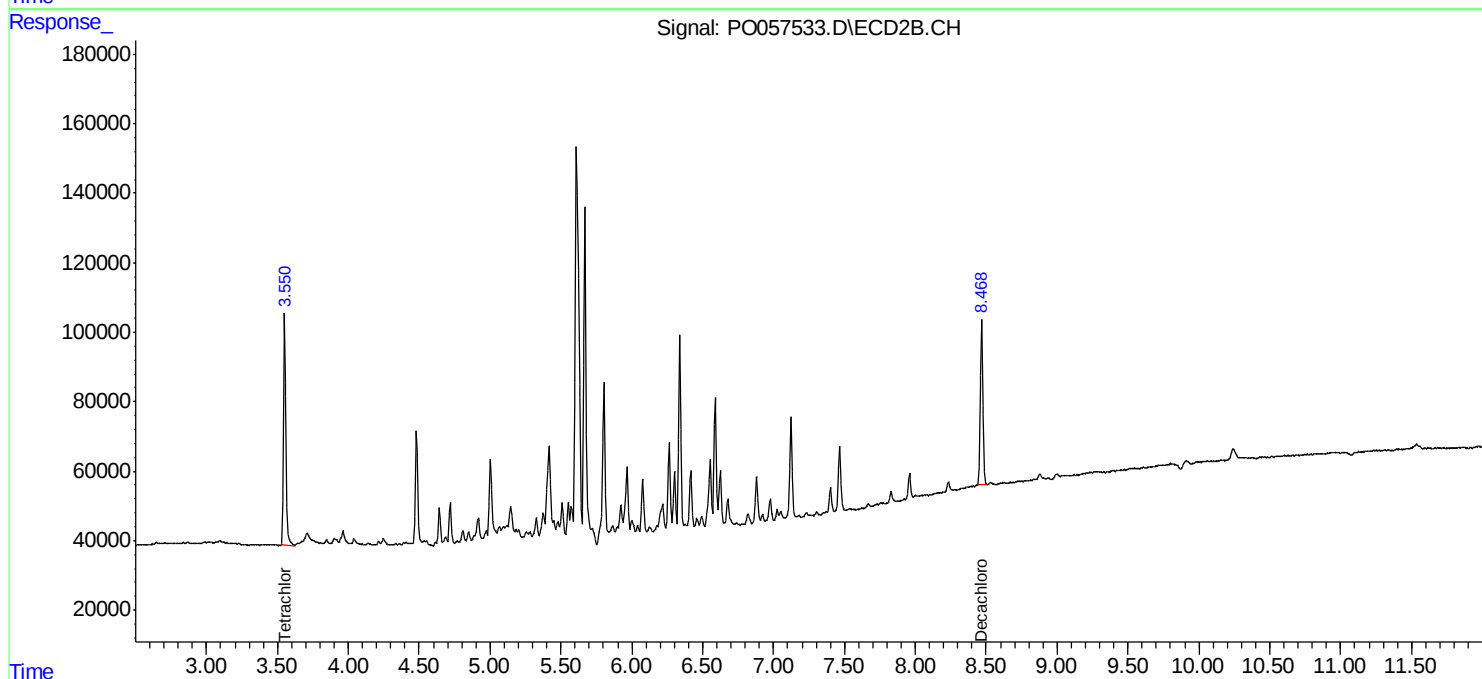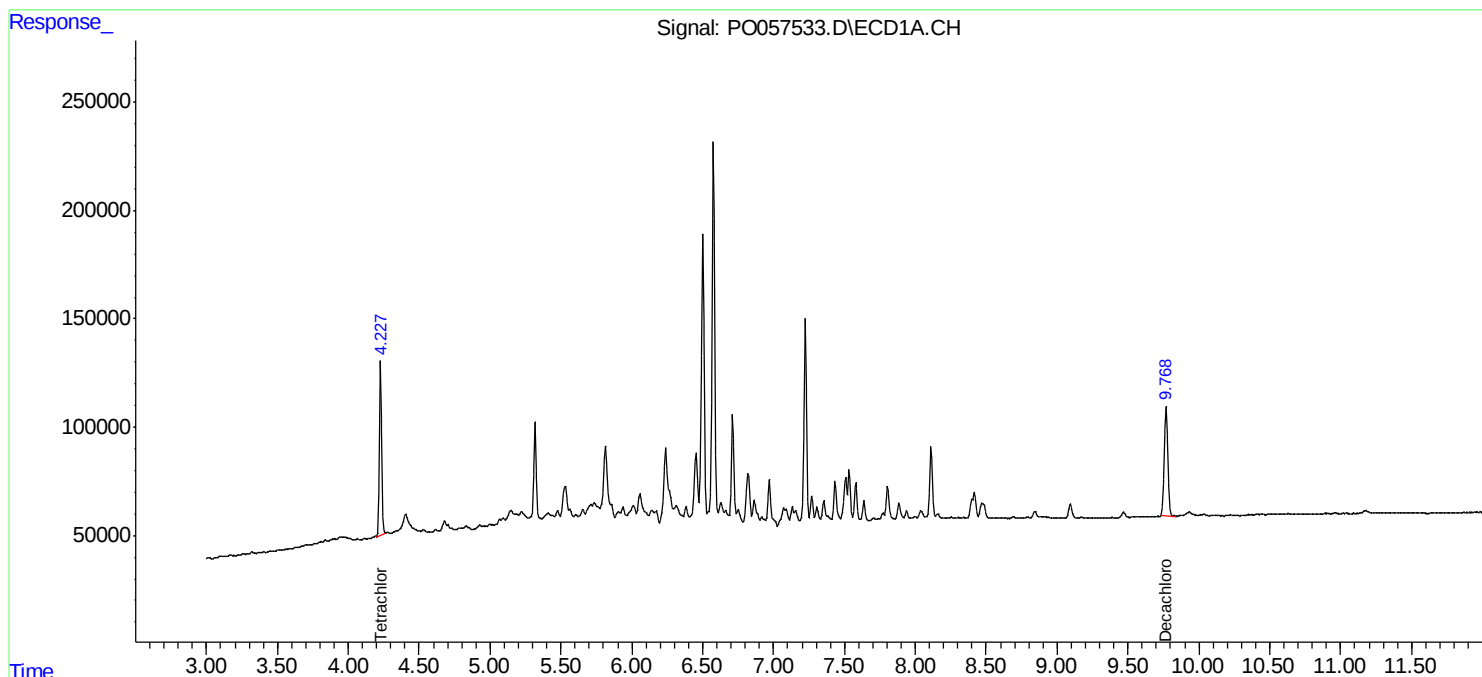


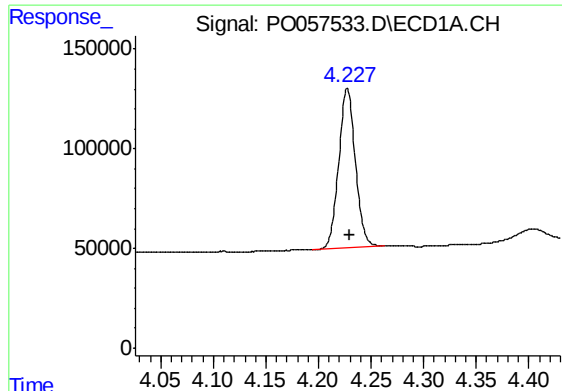

#1 Tetrachloro-m-xylene


R.T.: 4.227 min
Delta R.T.: -0.003 min
Response: 882737
Conc: 22.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-044-A

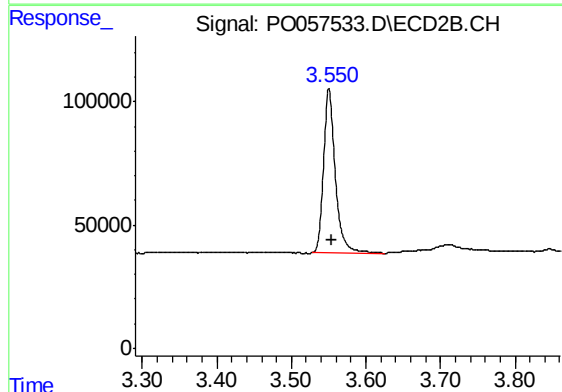


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: -0.005 min
Response: 742441
Conc: 21.11 ng/ml

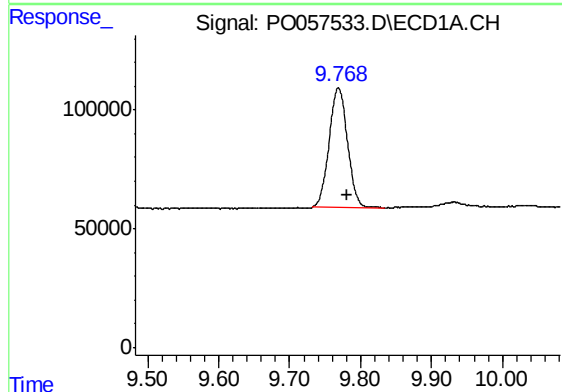

#2 Decachlorobiphenyl

R.T.: 9.768 min
Delta R.T.: -0.013 min
Response: 904085
Conc: 16.08 ng/ml

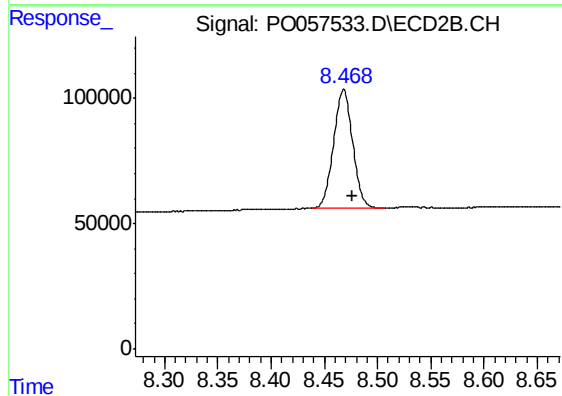

#2 Decachlorobiphenyl

R.T.: 8.468 min
Delta R.T.: -0.009 min
Response: 592931
Conc: 15.85 ng/ml