

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062719\
 Data File : P0057553.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jun 2019 17:46
 Operator : SM/SJ
 Sample : K3533-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-EF-01-013-ABCD

Manual Integrations
 APPROVED

Ankita
 6/28/2019 10:07:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:51:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.218	3.549	929633	746498	23.666	21.230
2) SA Decachlor...	9.756	8.462	1028102	682922	18.283	18.257m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062719\
Data File : P0057553.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jun 2019 17:46
Operator : SM/SJ
Sample : K3533-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-EF-01-013-ABCD


Manual Integrations
APPROVED

Ankita
6/28/2019 10:07:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:51:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

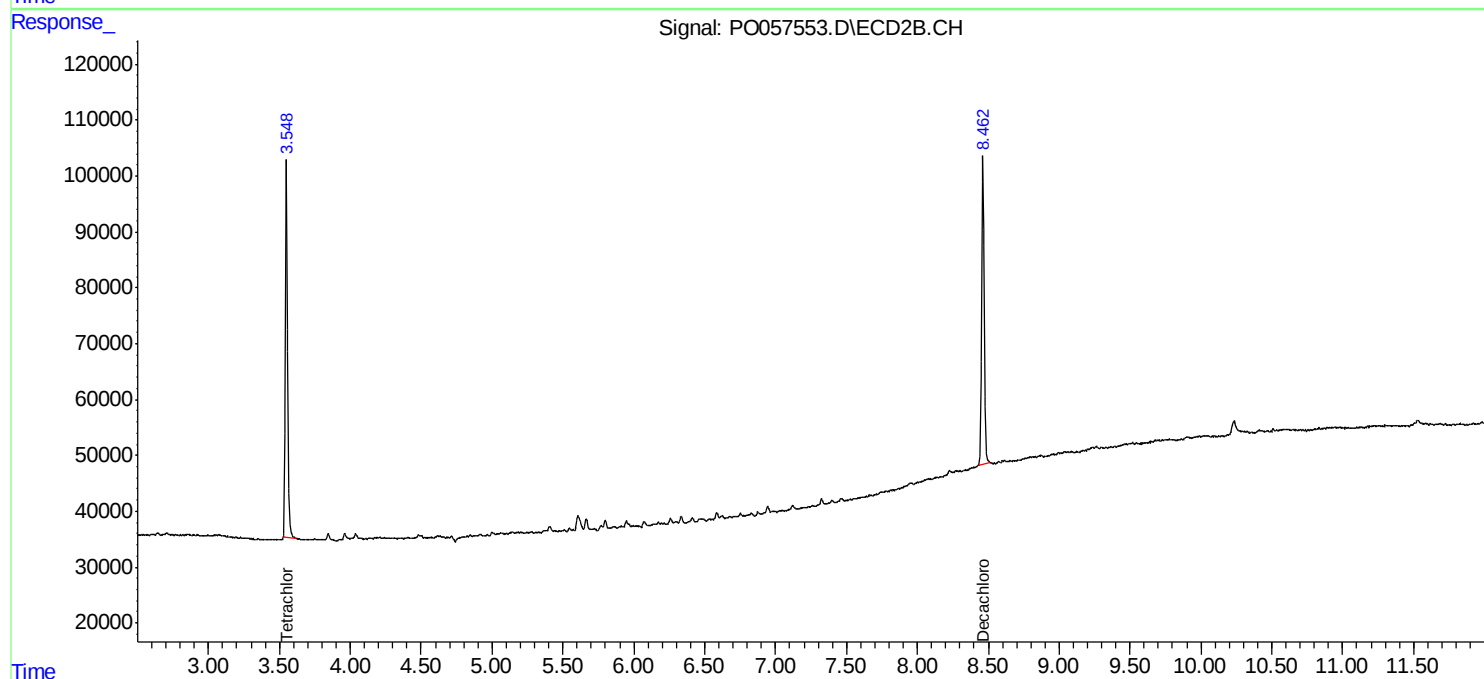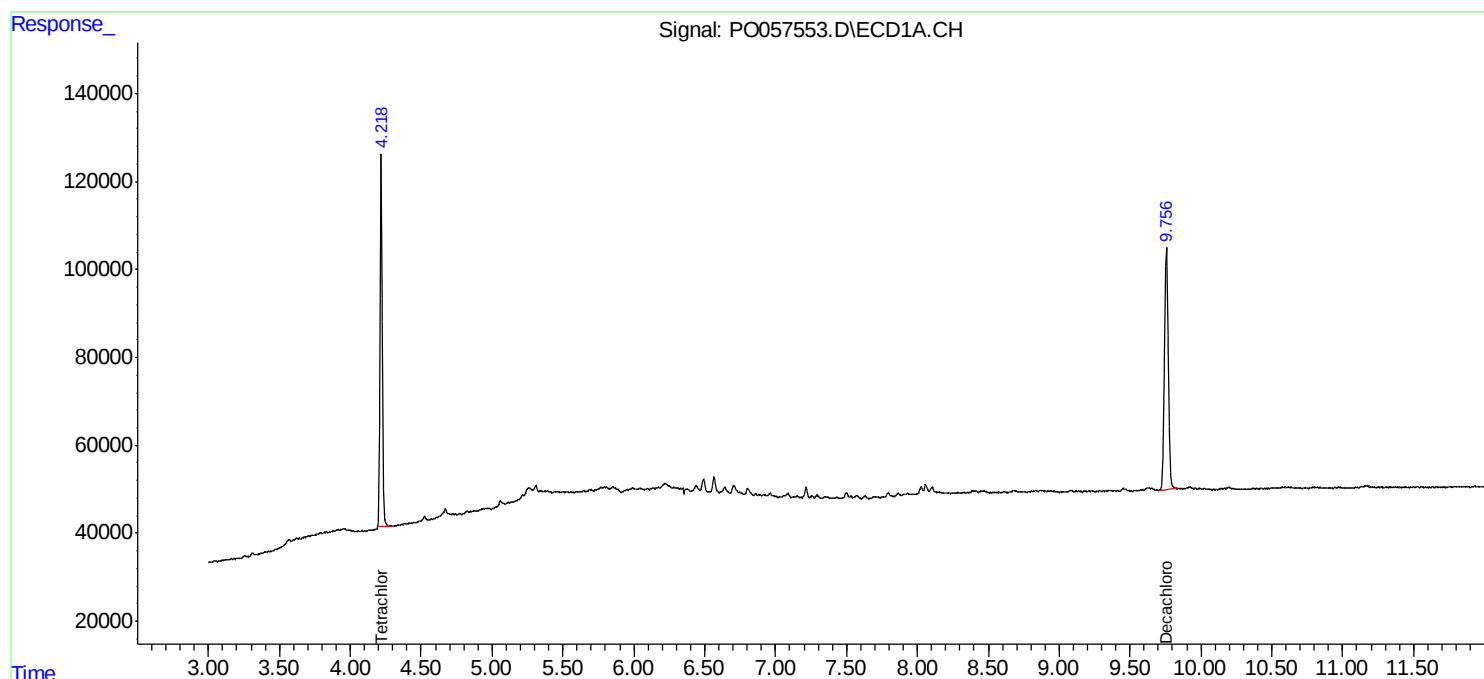

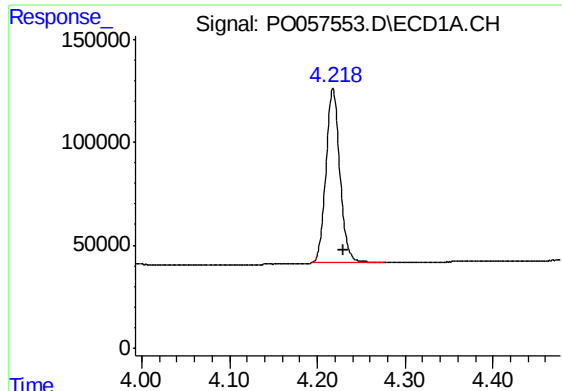


#1 Tetrachloro-m-xylene

R.T.: 4.218 min
Delta R.T.: -0.012 min
Response: 929633
Conc: 23.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-EF-01-013-ABCD


Manual Integrations
APPROVED

Ankita
6/28/2019 10:07:10 AM

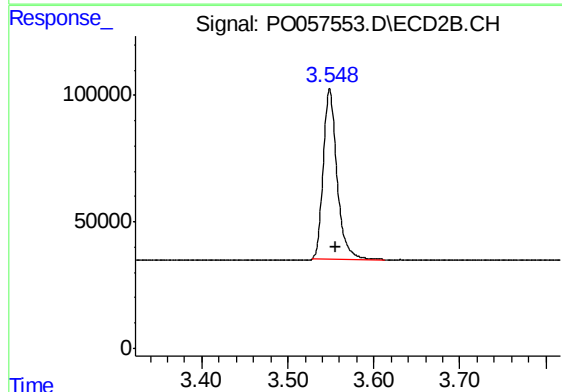


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: -0.007 min
Response: 746498
Conc: 21.23 ng/ml

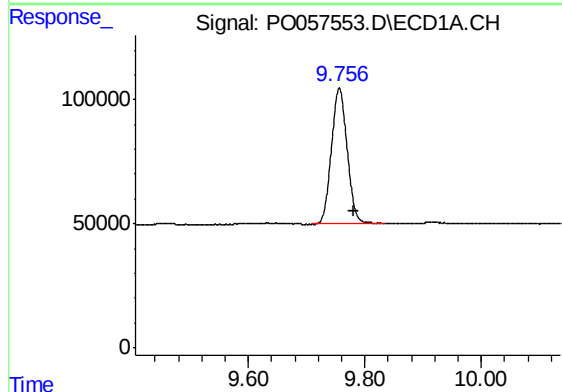

#2 Decachlorobiphenyl

R.T.: 9.756 min
Delta R.T.: -0.025 min
Response: 1028102
Conc: 18.28 ng/ml

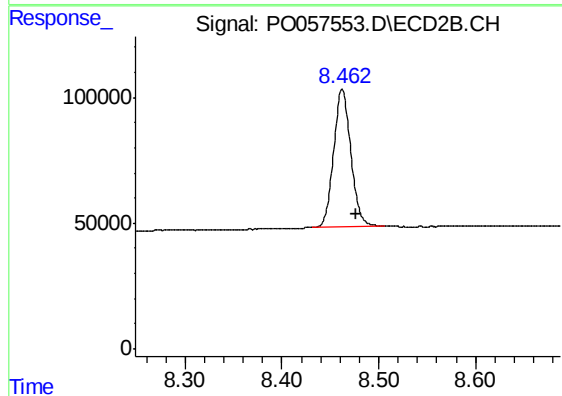

#2 Decachlorobiphenyl

R.T.: 8.462 min
Delta R.T.: -0.015 min
Response: 682922
Conc: 18.26 ng/ml m