

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062719\
 Data File : P0057555.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jun 2019 18:20
 Operator : SM/SJ
 Sample : PB120981BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB120981BL

Manual Integrations
 APPROVED

Ankita
 6/28/2019 10:07:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:53:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.218	3.549	870113	700268	22.151	19.915
2) SA Decachlor...	9.754	8.463	1093980	715708	19.454	19.133m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062719\
Data File : PO057555.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jun 2019 18:20
Operator : SM/SJ
Sample : PB120981BL
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB120981BL


Manual Integrations
APPROVED

Ankita
6/28/2019 10:07:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:53:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

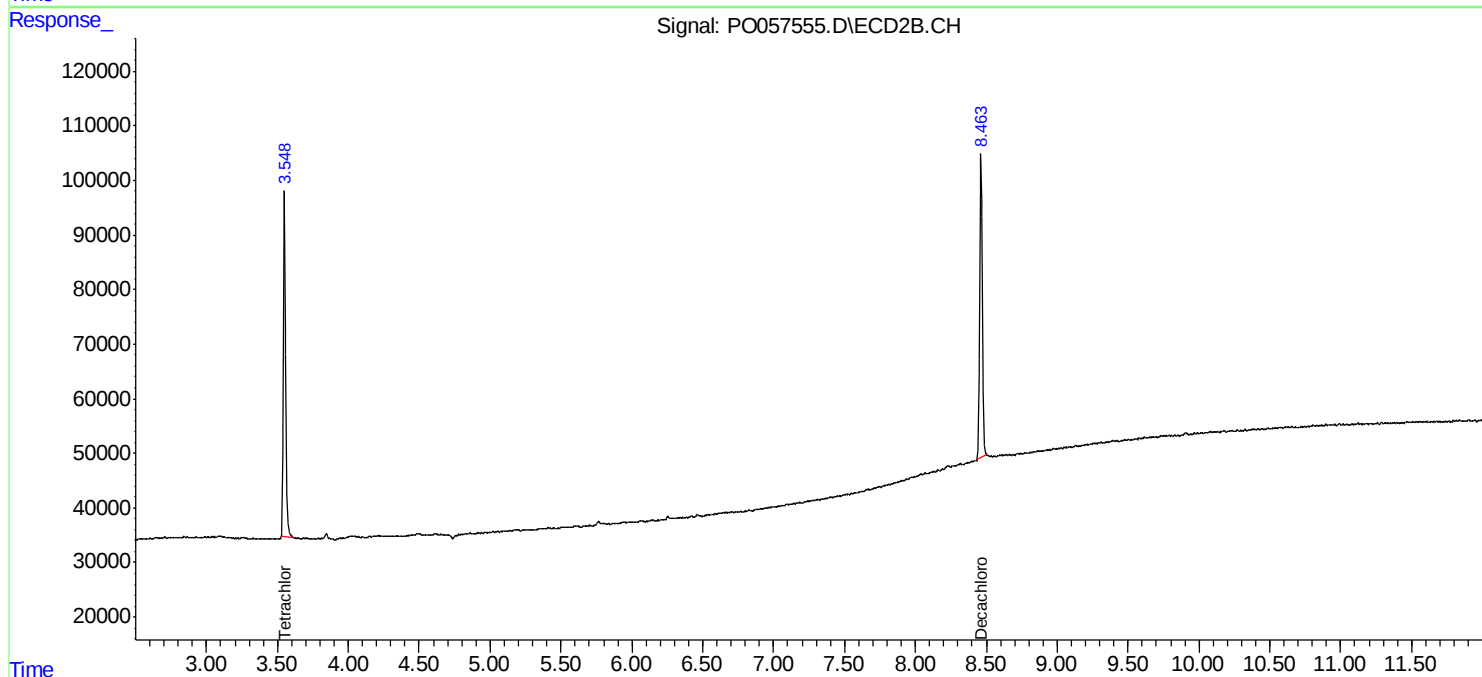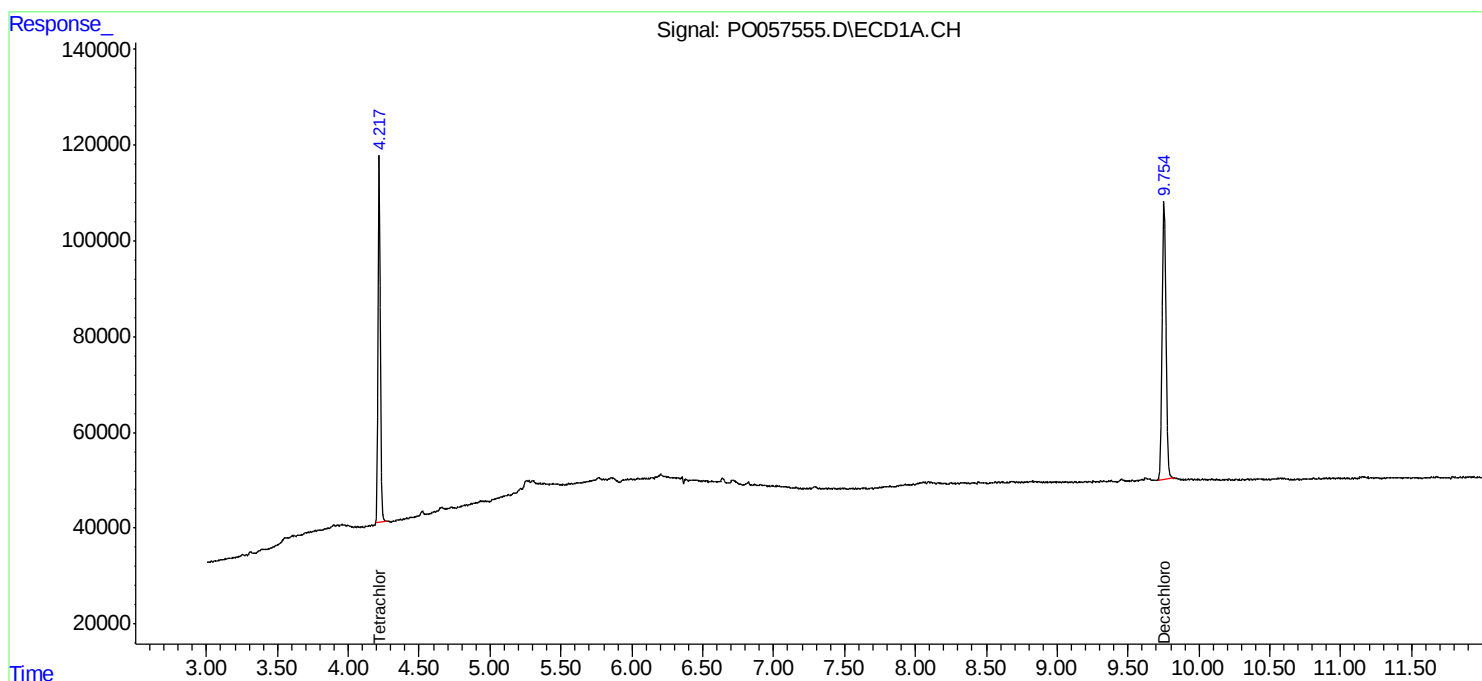

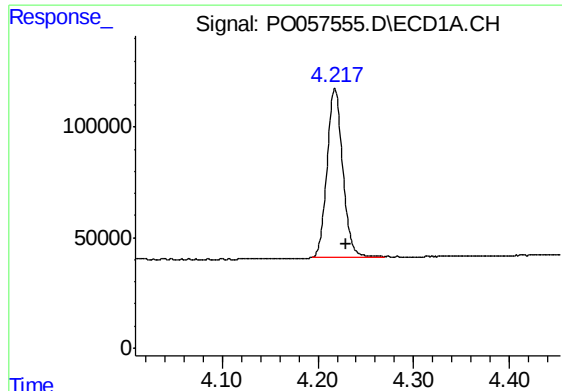


#1 Tetrachloro-m-xylene

R.T.: 4.218 min
Delta R.T.: -0.012 min
Response: 870113
Conc: 22.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB120981BL


Manual Integrations
APPROVED

Ankita
6/28/2019 10:07:12 AM

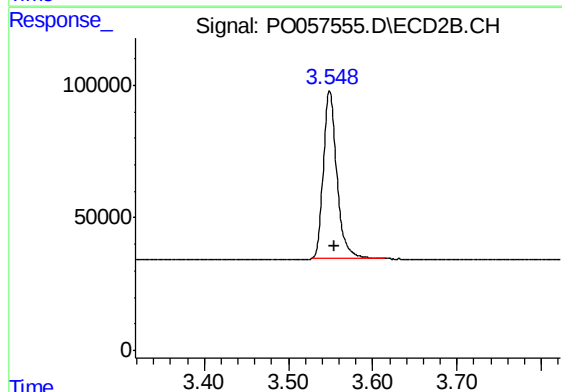


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: -0.006 min
Response: 700268
Conc: 19.91 ng/ml

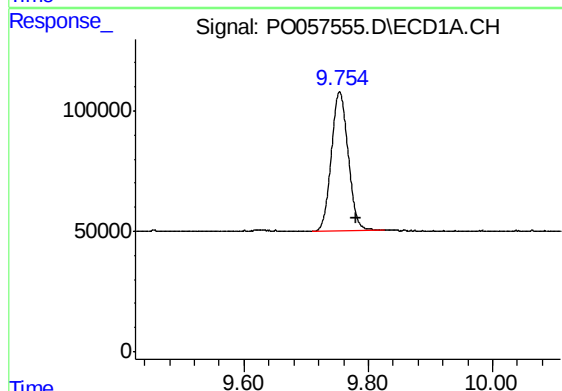

#2 Decachlorobiphenyl

R.T.: 9.754 min
Delta R.T.: -0.027 min
Response: 1093980
Conc: 19.45 ng/ml

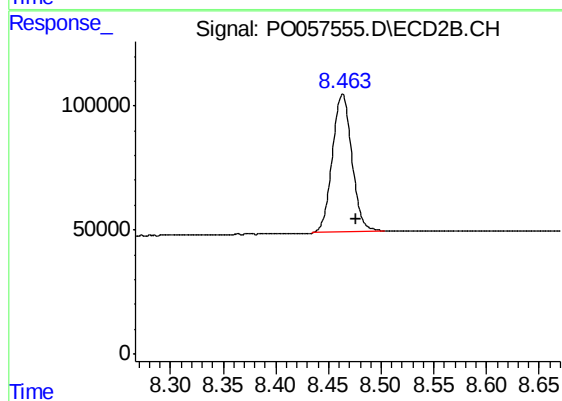

#2 Decachlorobiphenyl

R.T.: 8.463 min
Delta R.T.: -0.014 min
Response: 715708
Conc: 19.13 ng/ml m