

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062719\
 Data File : P0057568.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jun 2019 21:59
 Operator : SM/SJ
 Sample : K3552-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 M-8

Manual Integrations
 APPROVED

Ankita
 6/28/2019 10:07:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 02:15:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.216	3.547	690128	633975	17.569m	18.030m
2)	SA Decachlor...	9.754	8.460	923768	614603	16.428	16.430m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062719\
Data File : P0057568.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jun 2019 21:59
Operator : SM/SJ
Sample : K3552-15
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
M-8


Manual Integrations
APPROVED

Ankita
6/28/2019 10:07:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 02:15:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

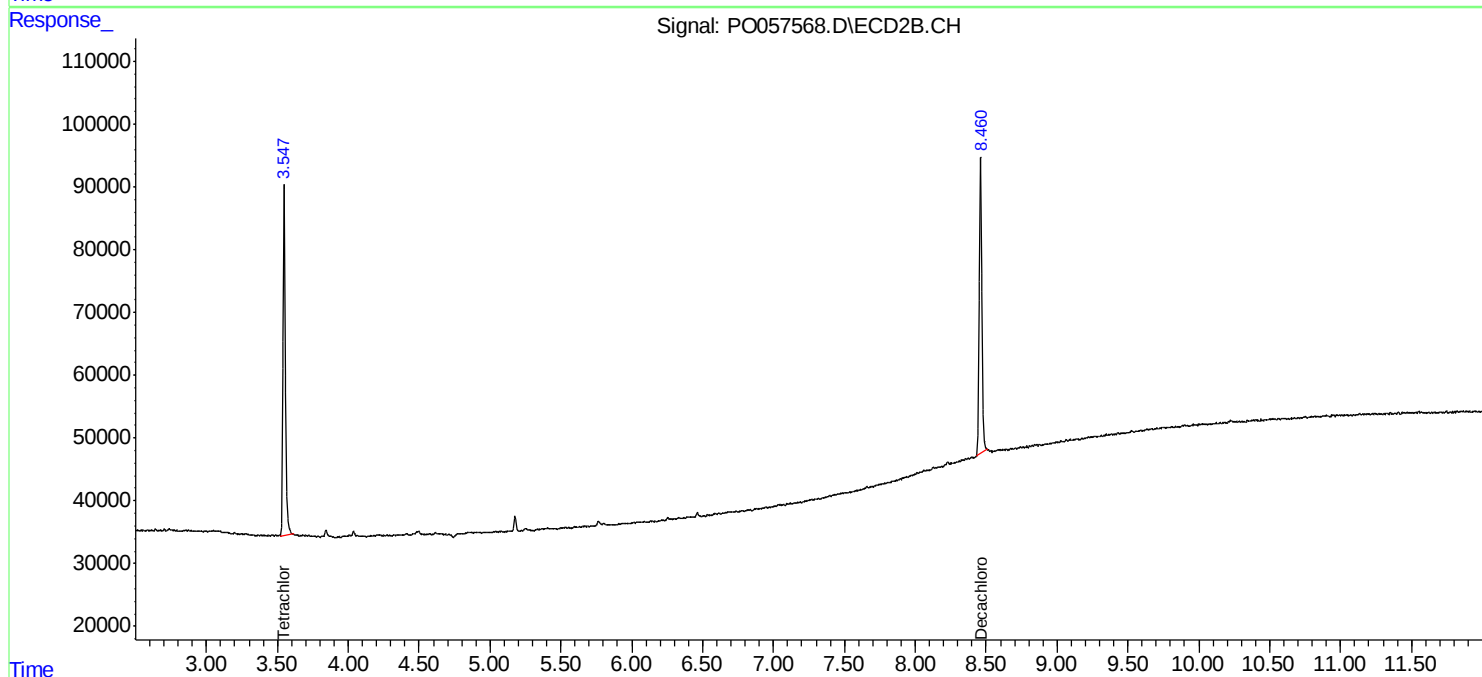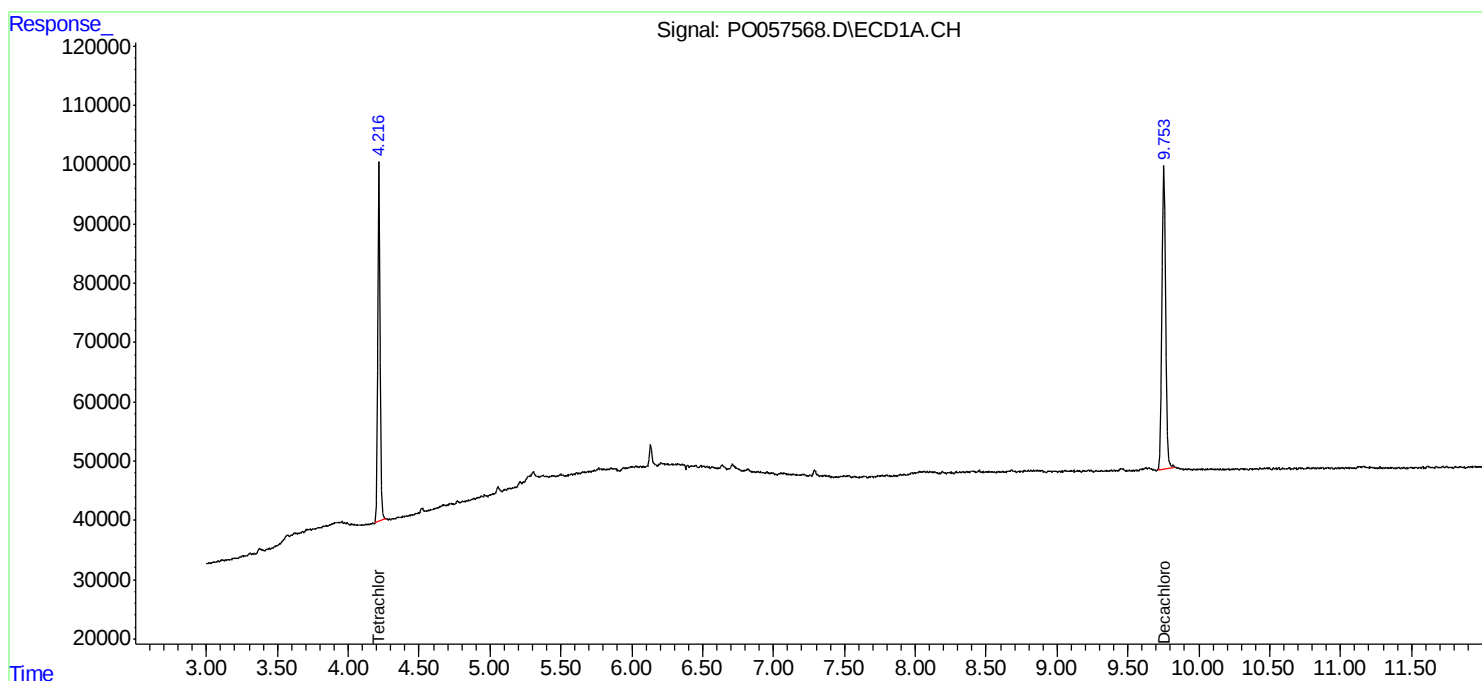

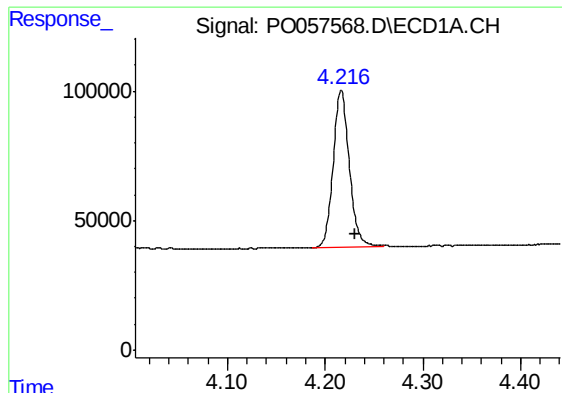


#1 Tetrachloro-m-xylene

R.T.: 4.216 min
Delta R.T.: -0.014 min
Response: 690128
Conc: 17.57 ng/ml m

Instrument :
ECD_O
ClientSampleId :
M-8


Manual Integrations
APPROVED

Ankita
6/28/2019 10:07:27 AM

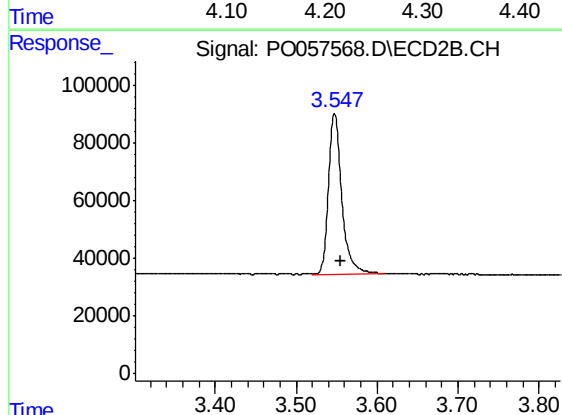


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: -0.008 min
Response: 633975
Conc: 18.03 ng/ml m

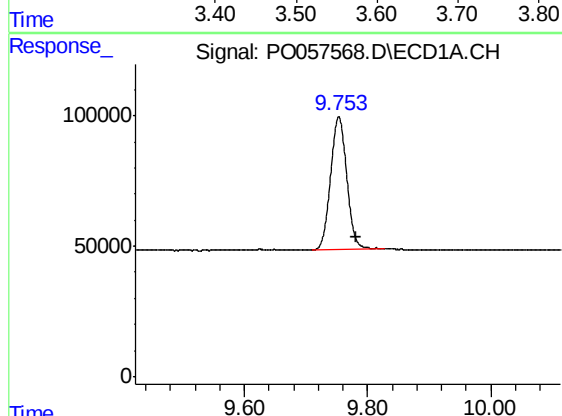

#2 Decachlorobiphenyl

R.T.: 9.754 min
Delta R.T.: -0.028 min
Response: 923768
Conc: 16.43 ng/ml

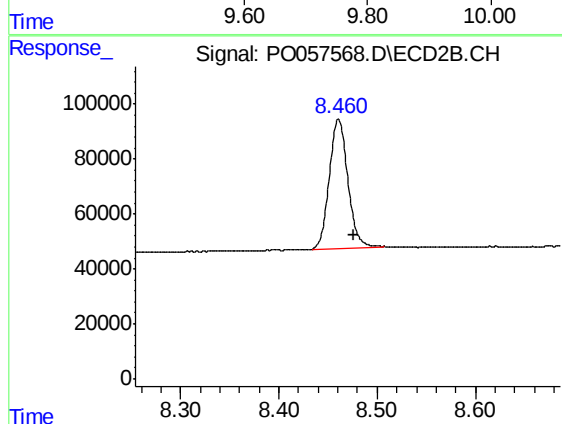

#2 Decachlorobiphenyl

R.T.: 8.460 min
Delta R.T.: -0.016 min
Response: 614603
Conc: 16.43 ng/ml m