

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062722\
 Data File : P0087454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 00:30
 Operator : YP/AJ
 Sample : N3488-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-9-0-2-20220623

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 05:54:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

06/28/2022
 Supervised By :Ankita
 Jodhani

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	06/28/2022
----------	------	------	--------	--------	-------	-------	------------

System Monitoring Compounds

1) SA Tetrachlo...	4.450	3.610	59908382	18301888	23.145	18.600
2) SA Decachlor...	10.300	8.614	45723670	14230338	22.384	17.554m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062722\
Data File : P0087454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 00:30
Operator : YP/AJ
Sample : N3488-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-9-0-2-20220623



Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 05:54:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

06/28/2022
Supervised By :Ankita
Jodhani

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

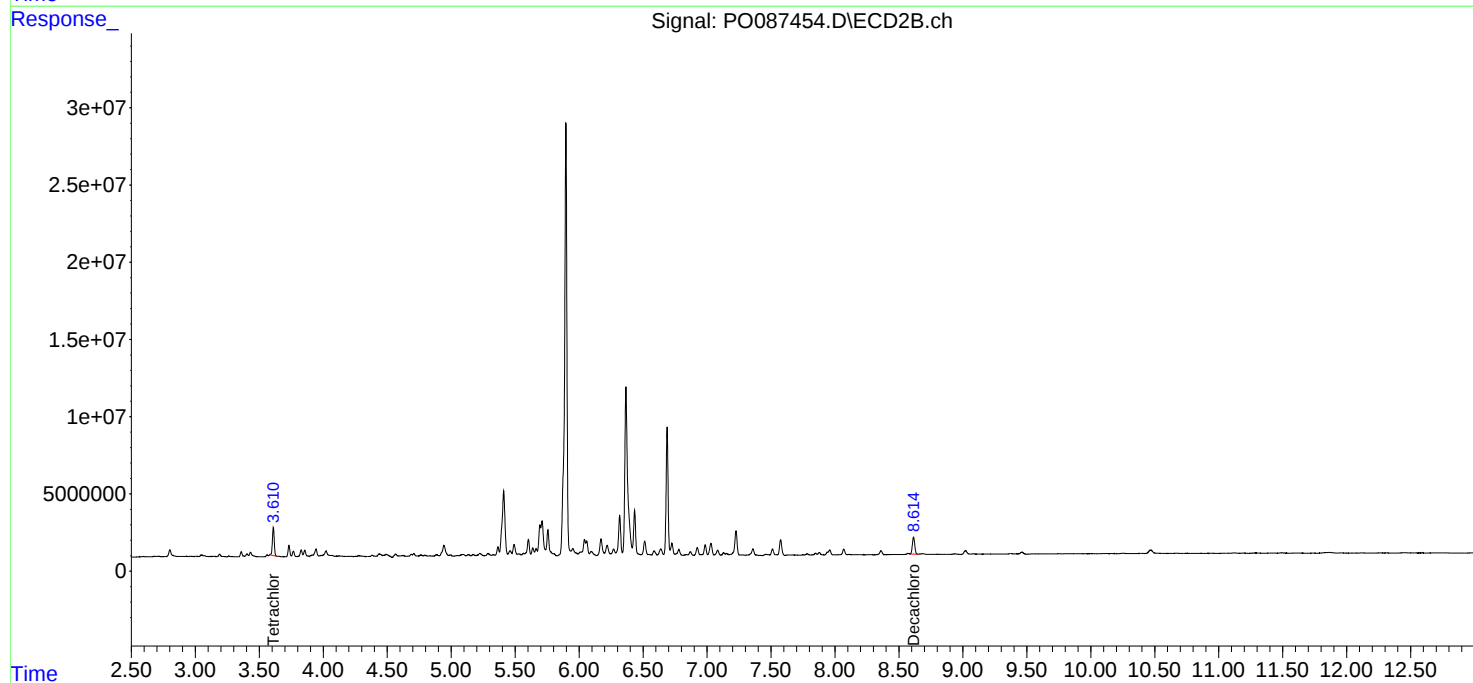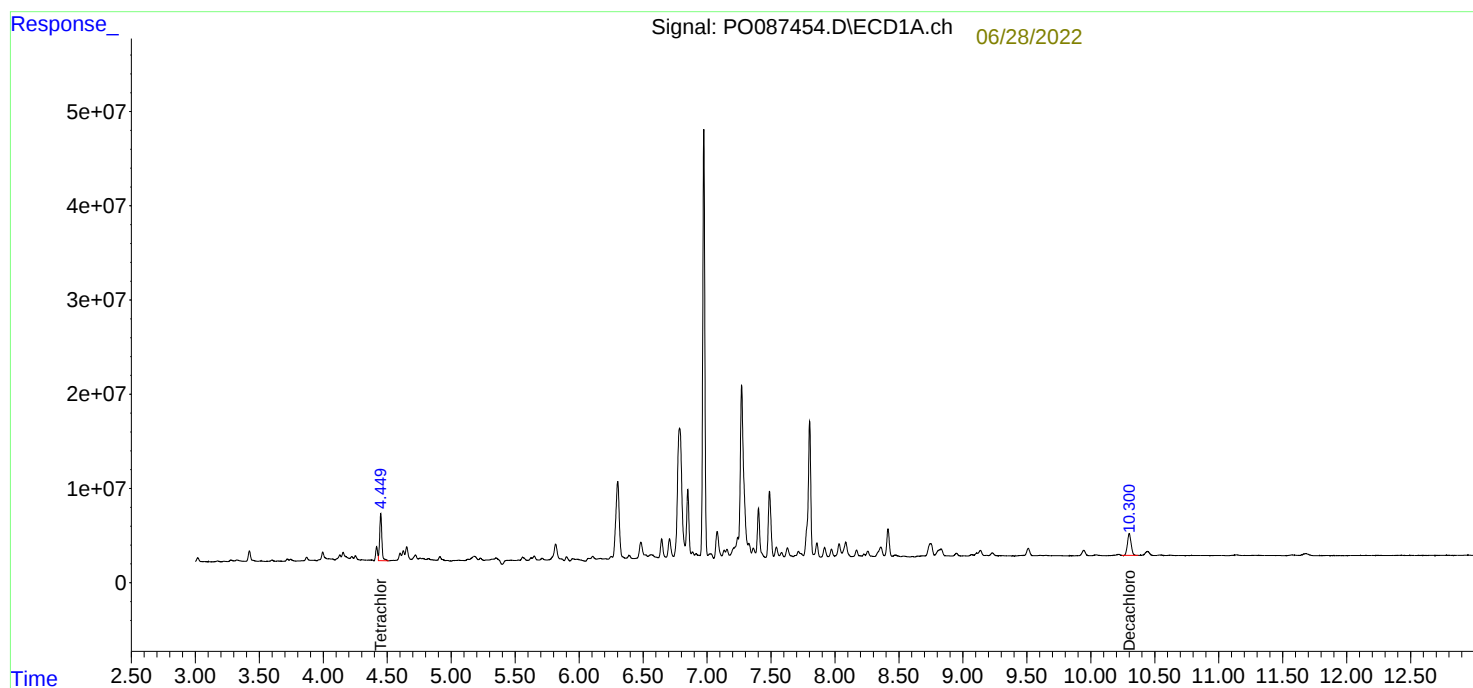

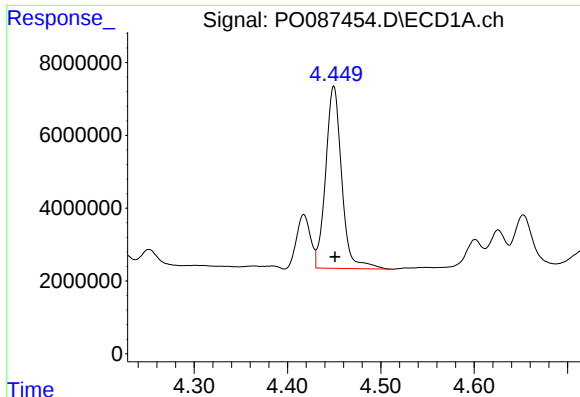


#1 Tetrachloro-m-xylene

R.T.: 4.450 min
Delta R.T.: -0.001 min
Response: 59908382
Conc: 23.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-9-0-2-20220623

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

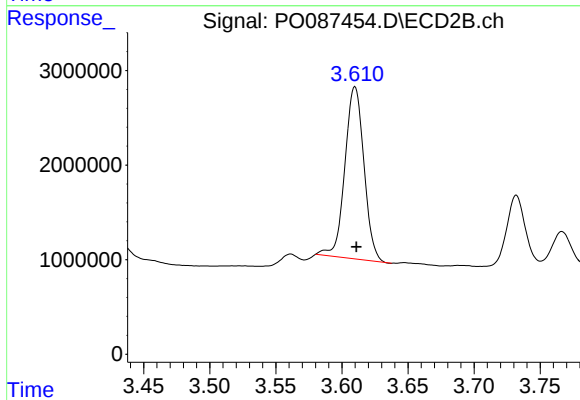


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.001 min
Response: 18301888
Conc: 18.60 ng/ml


06/28/2022
Supervised By :Ankita
Jodhani

06/28/2022

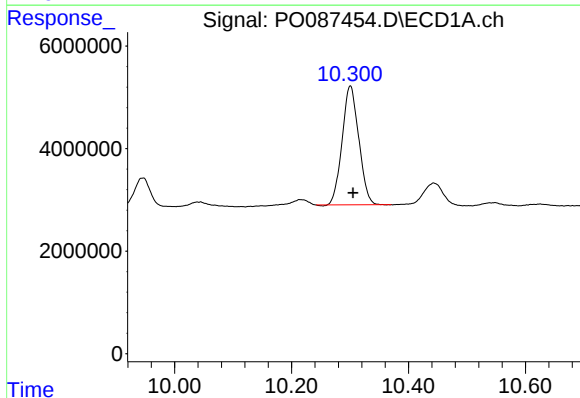

#2 Decachlorobiphenyl

R.T.: 10.300 min
Delta R.T.: -0.005 min
Response: 45723670
Conc: 22.38 ng/ml

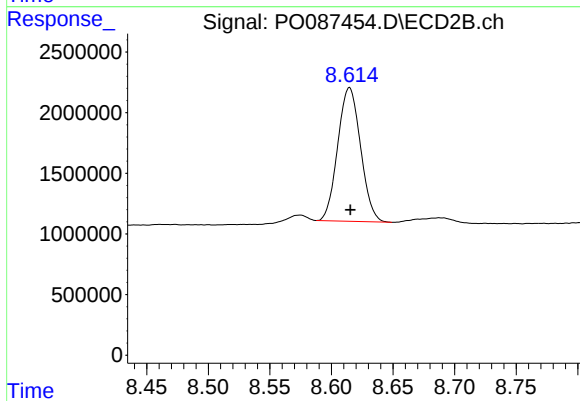

#2 Decachlorobiphenyl

R.T.: 8.614 min
Delta R.T.: 0.000 min
Response: 14230338
Conc: 17.55 ng/ml m