

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062722\
 Data File : P0087475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 07:06
 Operator : YP/AJ
 Sample : N3494-01 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP-EXC-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/28/2022
 Supervised By :Ankita Jodhani 06/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 07:47:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.609	14572696	4842674	5.630	4.921m
2) SA Decachlor...	10.301	8.613	13095185	3833472	6.411	4.729 #
Target Compounds						
31) L7 AR-1260-1	7.239	6.170	4456497	1999641	39.754	35.420
32) L7 AR-1260-2	7.486	6.360	16955448	1604764	124.420	23.719 #
33) L7 AR-1260-3	7.859	6.513	4690140	1879464	50.072	29.753 #
34) L7 AR-1260-4	8.083	6.985	4666591	1733870	44.610	37.284
35) L7 AR-1260-5	8.413	7.227	7436894	3300801	37.700	30.621

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062722\
Data File : PO087475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 07:06
Operator : YP/AJ
Sample : N3494-01 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SP-EXC-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 07:47:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

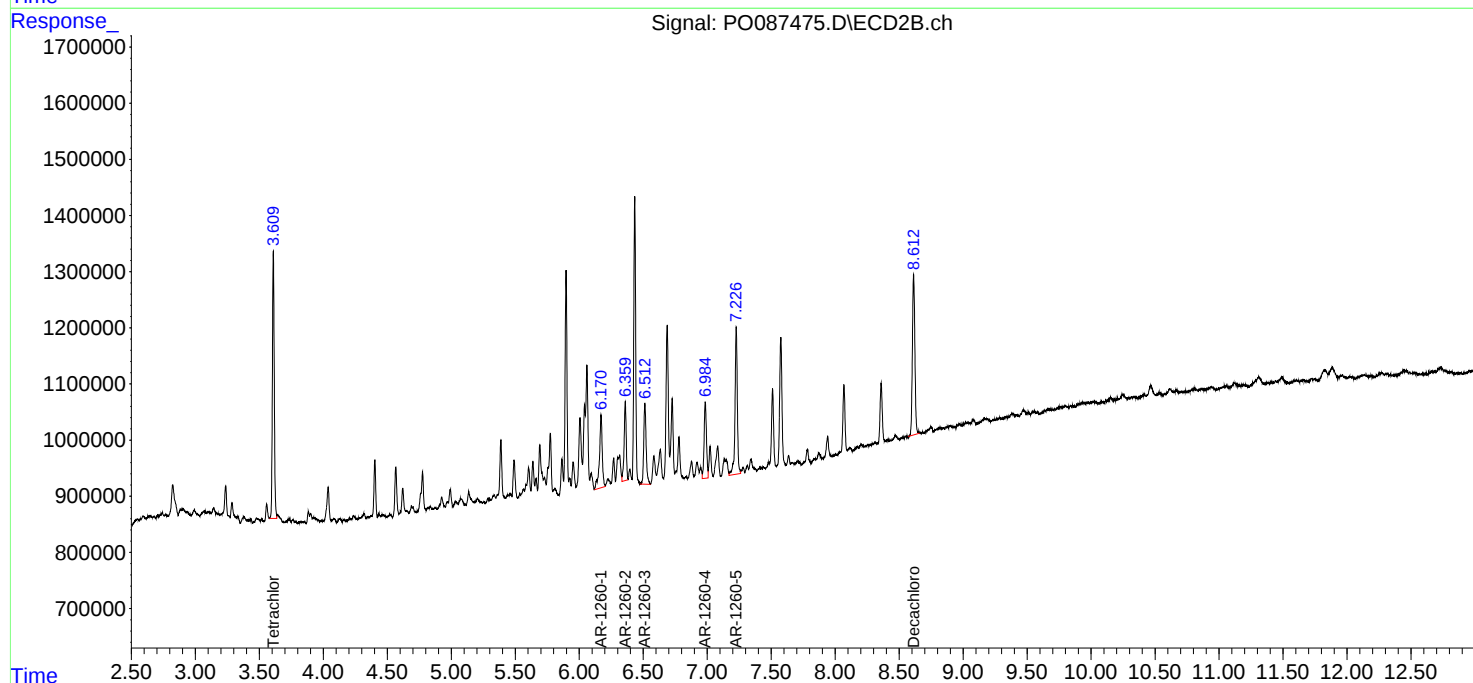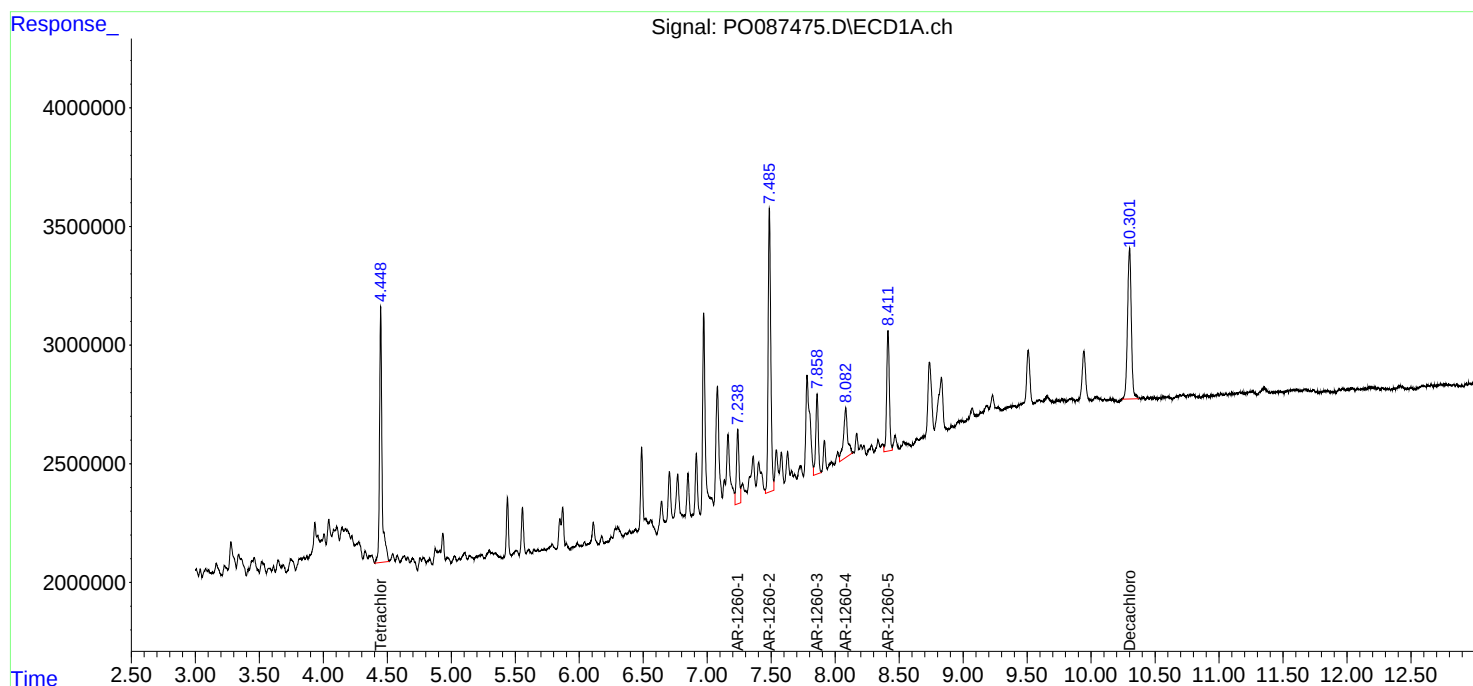

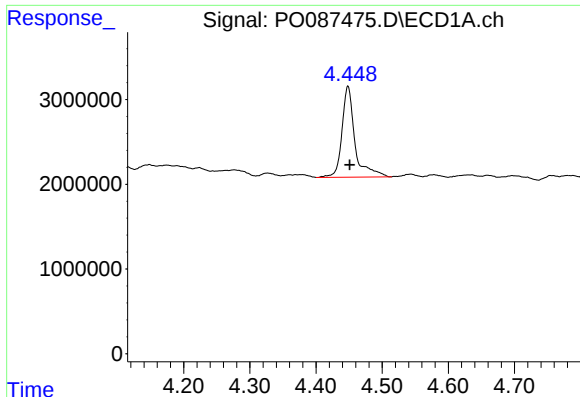


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: -0.003 min
Response: 14572696
Conc: 5.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-EXC-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

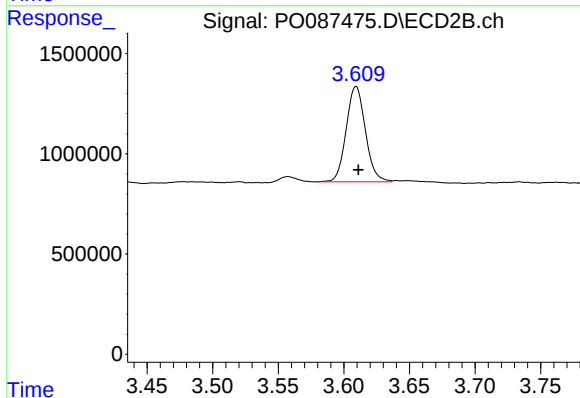


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: -0.002 min
Response: 4842674
Conc: 4.92 ng/ml m

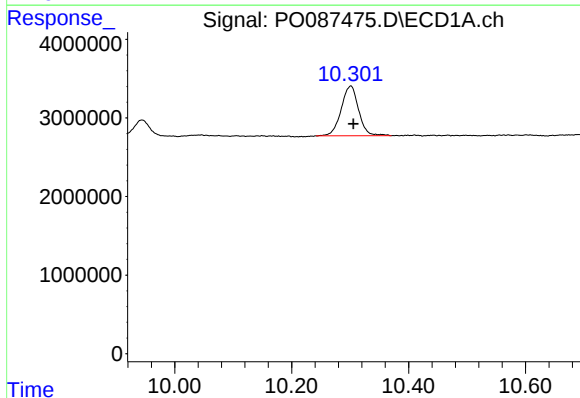


#2 Decachlorobiphenyl

R.T.: 10.301 min
Delta R.T.: -0.004 min
Response: 13095185
Conc: 6.41 ng/ml

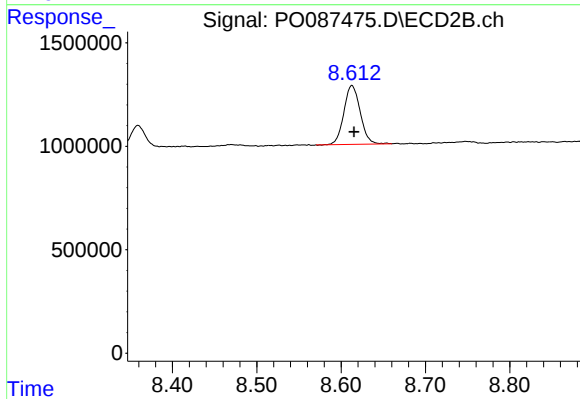

#2 Decachlorobiphenyl

R.T.: 8.613 min
Delta R.T.: -0.003 min
Response: 3833472
Conc: 4.73 ng/ml

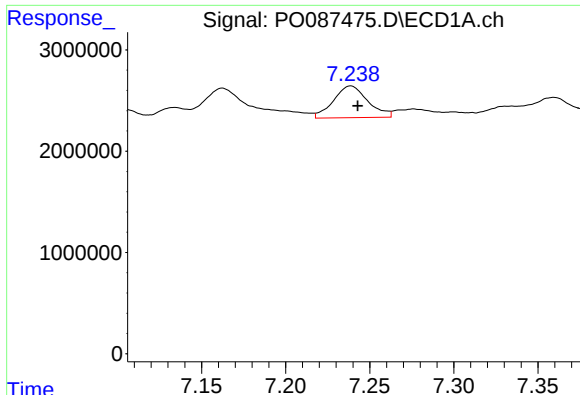


#31 AR-1260-1

R.T.: 7.239 min
Delta R.T.: -0.004 min
Response: 4456497
Conc: 39.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-EXC-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

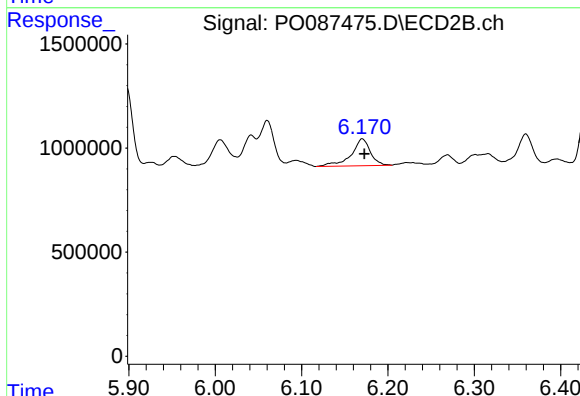


#31 AR-1260-1

R.T.: 6.170 min
Delta R.T.: -0.003 min
Response: 1999641
Conc: 35.42 ng/ml

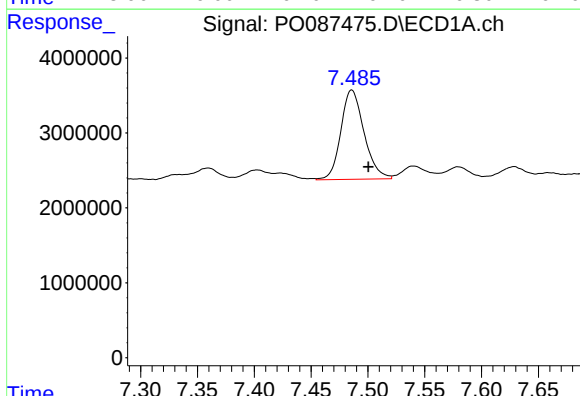


#32 AR-1260-2

R.T.: 7.486 min
Delta R.T.: -0.014 min
Response: 16955448
Conc: 124.42 ng/ml

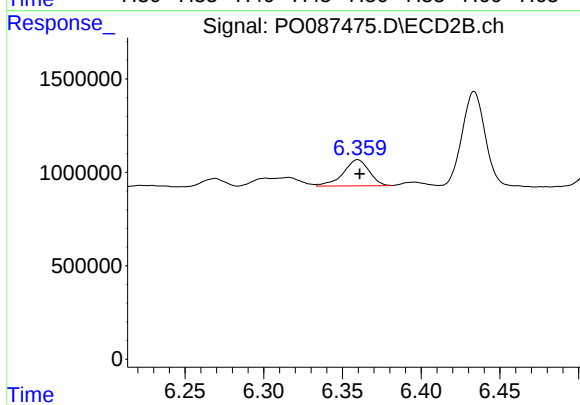

#32 AR-1260-2

R.T.: 6.360 min
Delta R.T.: -0.001 min
Response: 1604764
Conc: 23.72 ng/ml

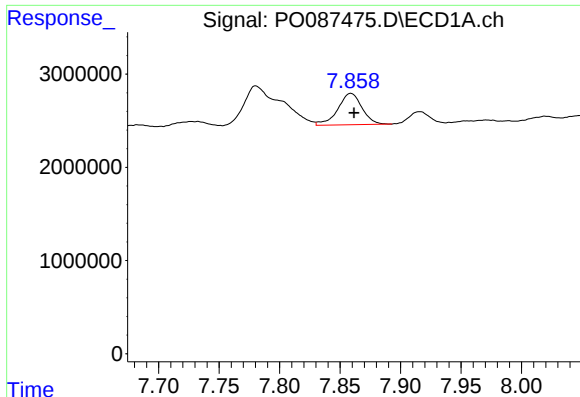


#33 AR-1260-3

R.T.: 7.859 min
Delta R.T.: -0.003 min
Response: 4690140
Conc: 50.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-EXC-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

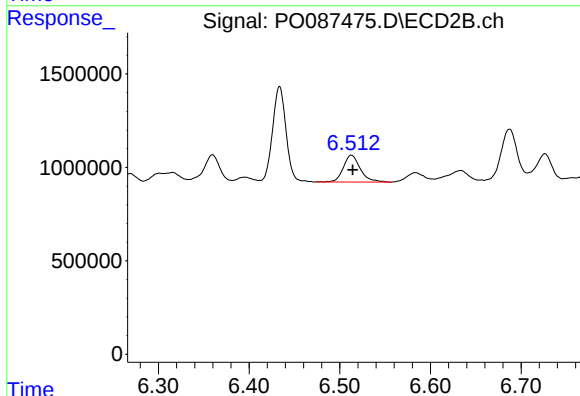


#33 AR-1260-3

R.T.: 6.513 min
Delta R.T.: -0.002 min
Response: 1879464
Conc: 29.75 ng/ml

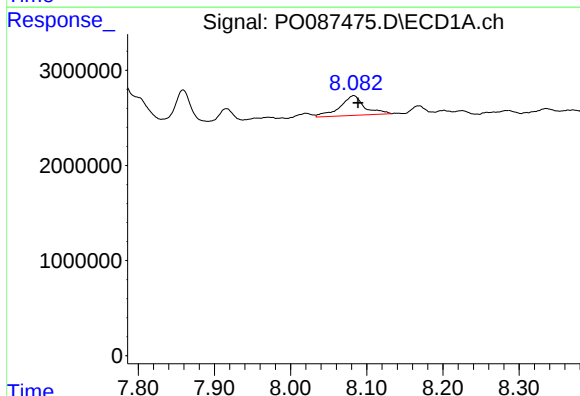


#34 AR-1260-4

R.T.: 8.083 min
Delta R.T.: -0.006 min
Response: 4666591
Conc: 44.61 ng/ml

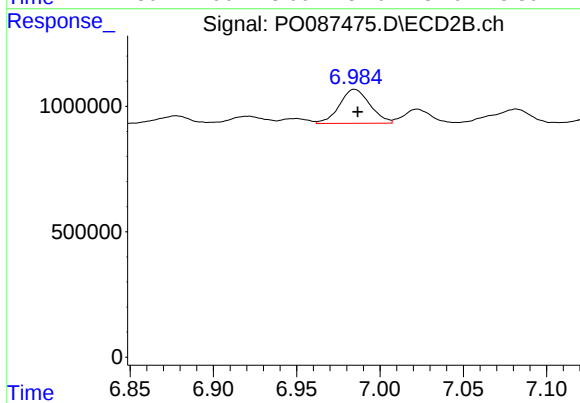

#34 AR-1260-4

R.T.: 6.985 min
Delta R.T.: -0.002 min
Response: 1733870
Conc: 37.28 ng/ml

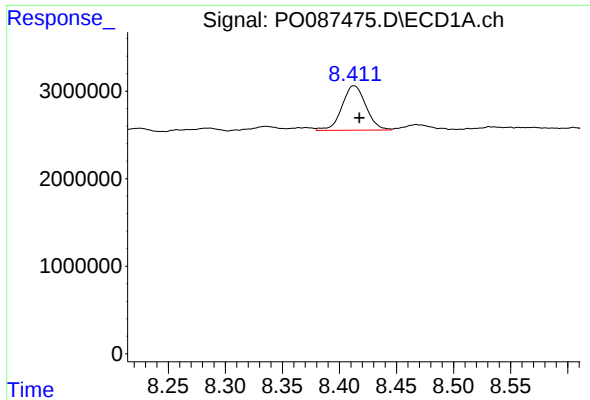


#35 AR-1260-5

R.T.: 8.413 min
Delta R.T.: -0.005 min
Response: 7436894
Conc: 37.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-EXC-3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

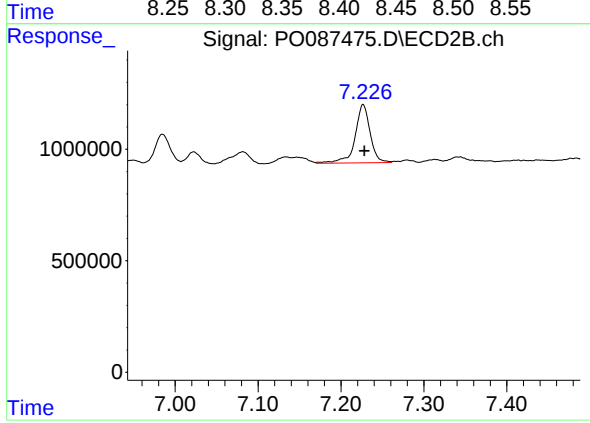

#35 AR-1260-5

R.T.: 7.227 min
Delta R.T.: -0.001 min
Response: 3300801
Conc: 30.62 ng/ml