

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062722\
 Data File : P0087478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 07:56
 Operator : YP/AJ
 Sample : N3494-16 5X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP-EXC-1-6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/28/2022
 Supervised By :Ankita Jodhani 06/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 13:33:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.449	3.610	13283521	5205219	5.132m	5.290
2) SA Decachlor...	10.302	8.615	9987342	2982219	4.889	3.679
Target Compounds						
31) L7 AR-1260-1	7.239	6.174	3433305	1421817	30.626	25.185
32) L7 AR-1260-2	7.487	6.360	38499775	810855	282.513	11.985 #
33) L7 AR-1260-3	7.859	6.514	2538762	1036829	27.104	16.414 #
34) L7 AR-1260-4	8.085	6.986	2472805	717799	23.639m	15.435 #
35) L7 AR-1260-5	8.416	7.227	4310948	1915197	21.854	17.767

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062722\
Data File : PO087478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 07:56
Operator : YP/AJ
Sample : N3494-16 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SP-EXC-1-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 13:33:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

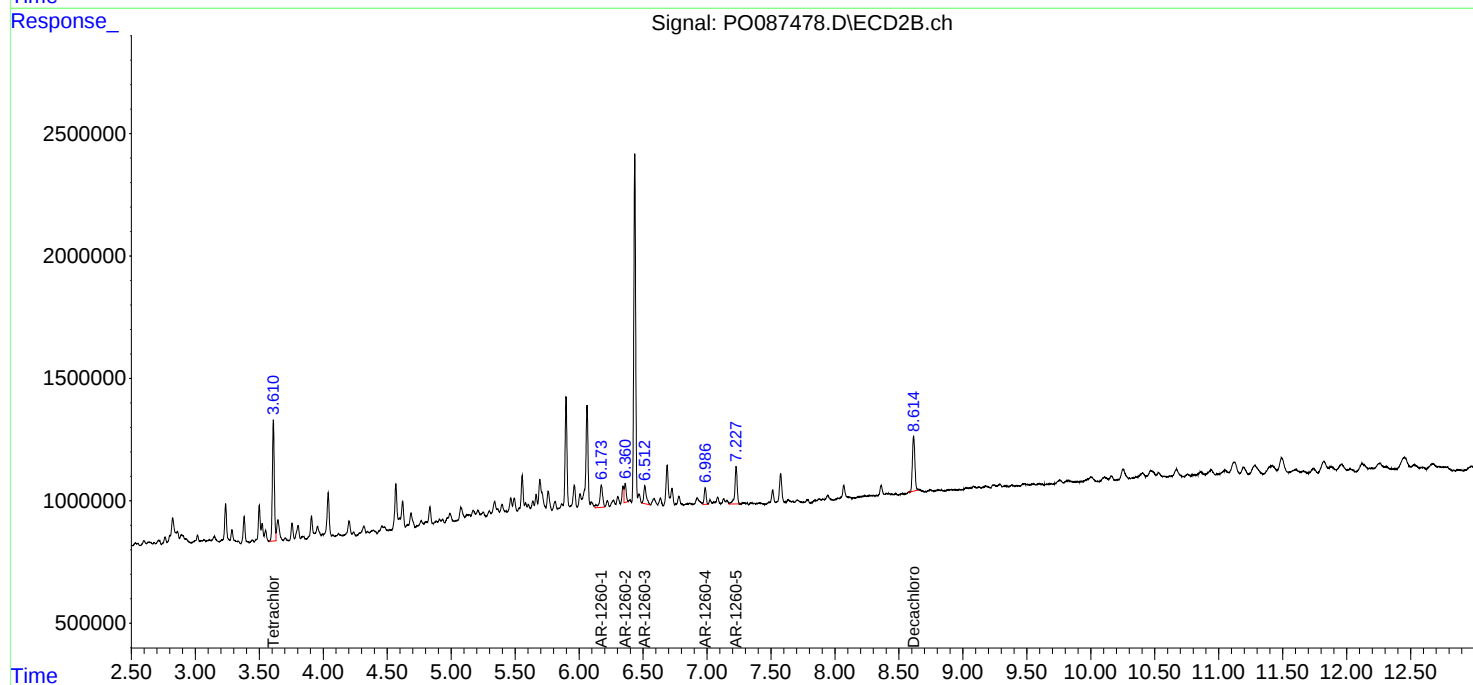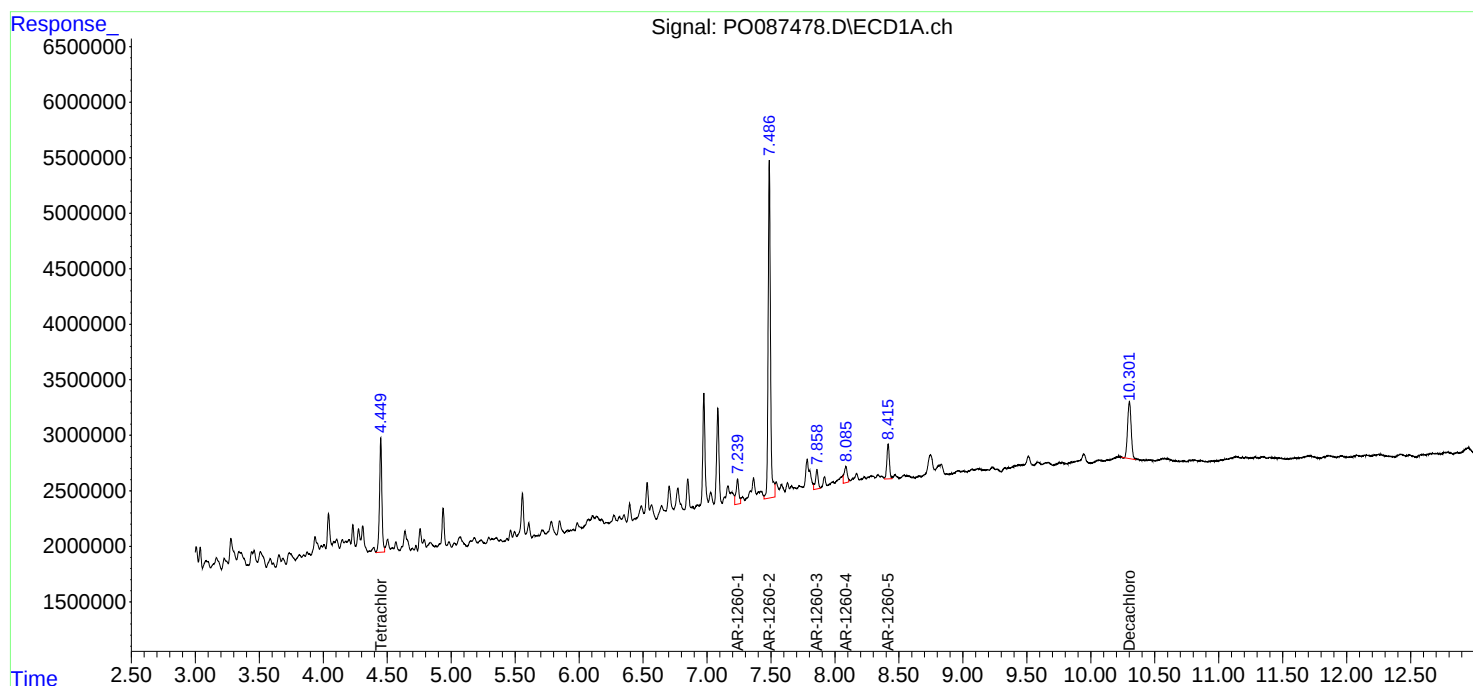

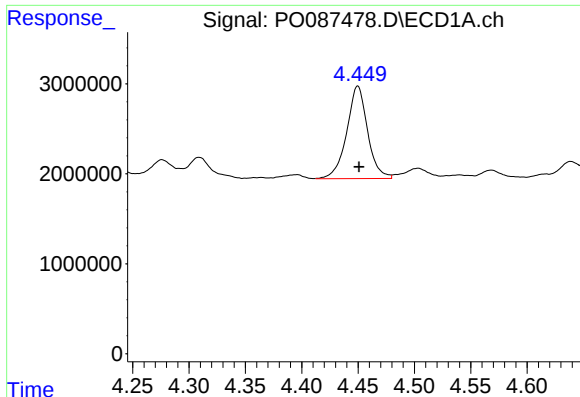


#1 Tetrachloro-m-xylene

R.T.: 4.449 min
Delta R.T.: -0.002 min
Response: 13283521
Conc: 5.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-EXC-1-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

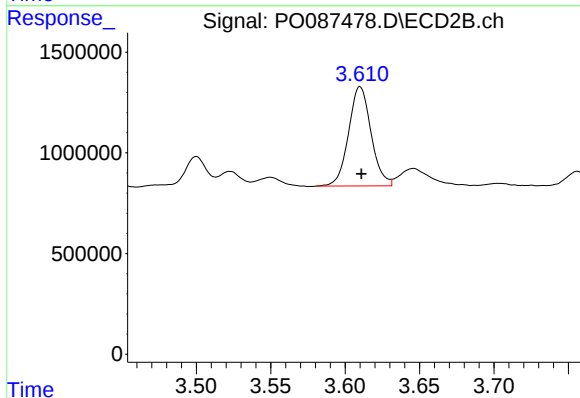


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: 0.000 min
Response: 5205219
Conc: 5.29 ng/ml

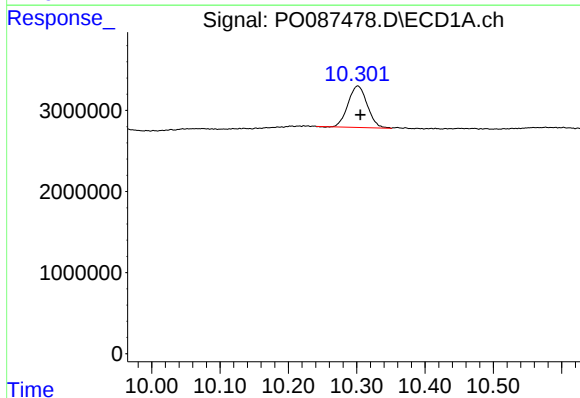


#2 Decachlorobiphenyl

R.T.: 10.302 min
Delta R.T.: -0.004 min
Response: 9987342
Conc: 4.89 ng/ml

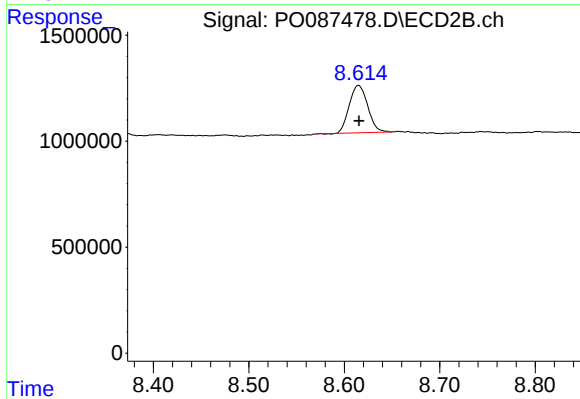

#2 Decachlorobiphenyl

R.T.: 8.615 min
Delta R.T.: 0.000 min
Response: 2982219
Conc: 3.68 ng/ml

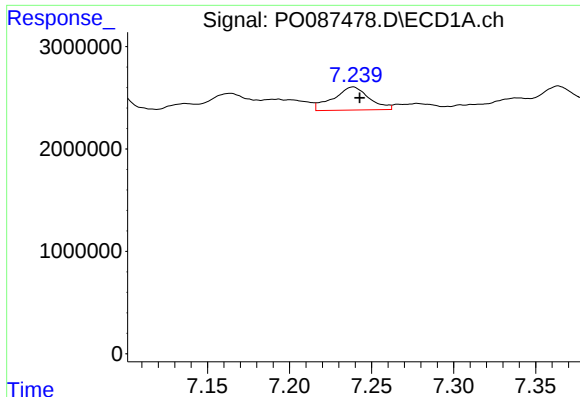


#31 AR-1260-1

R.T.: 7.239 min
Delta R.T.: -0.004 min
Response: 3433305
Conc: 30.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-EXC-1-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

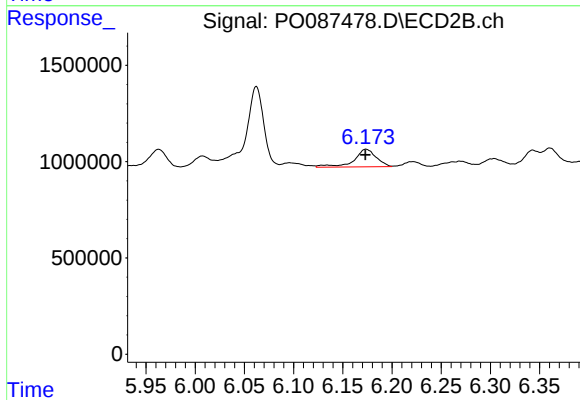


#31 AR-1260-1

R.T.: 6.174 min
Delta R.T.: 0.000 min
Response: 1421817
Conc: 25.18 ng/ml

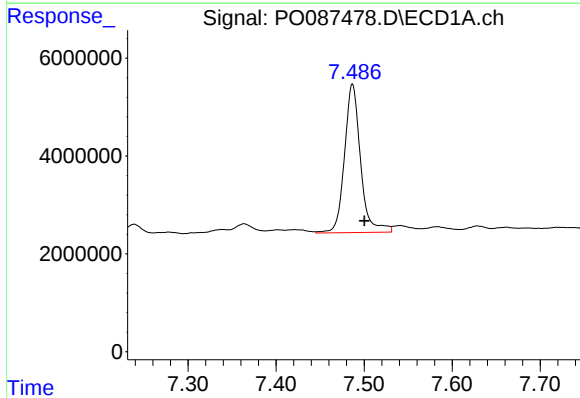


#32 AR-1260-2

R.T.: 7.487 min
Delta R.T.: -0.013 min
Response: 38499775
Conc: 282.51 ng/ml

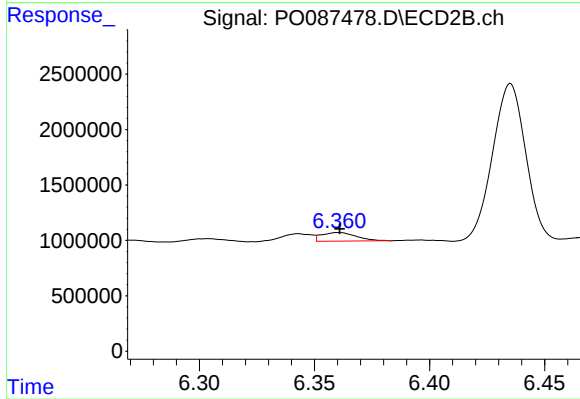

#32 AR-1260-2

R.T.: 6.360 min
Delta R.T.: 0.000 min
Response: 810855
Conc: 11.98 ng/ml

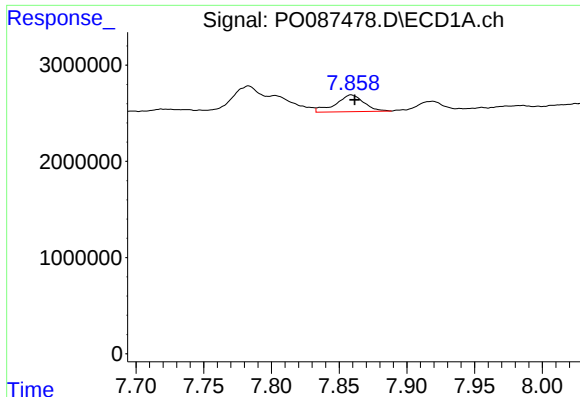

#33 AR-1260-3

R.T.: 7.859 min
Delta R.T.: -0.003 min
Response: 2538762
Conc: 27.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-EXC-1-6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

#33 AR-1260-3


R.T.: 6.514 min
Delta R.T.: 0.000 min
Response: 1036829
Conc: 16.41 ng/ml

#34 AR-1260-4

R.T.: 8.085 min
Delta R.T.: -0.004 min
Response: 2472805
Conc: 23.64 ng/ml m

#34 AR-1260-4

R.T.: 6.986 min
Delta R.T.: -0.001 min
Response: 717799
Conc: 15.44 ng/ml

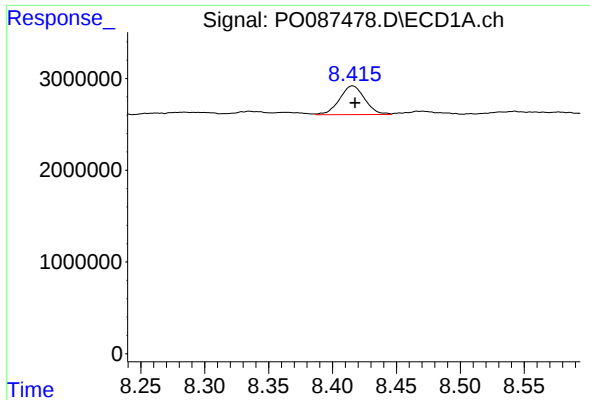


#35 AR-1260-5

R.T.: 8.416 min
Delta R.T.: -0.002 min
Response: 4310948
Conc: 21.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-EXC-1-6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

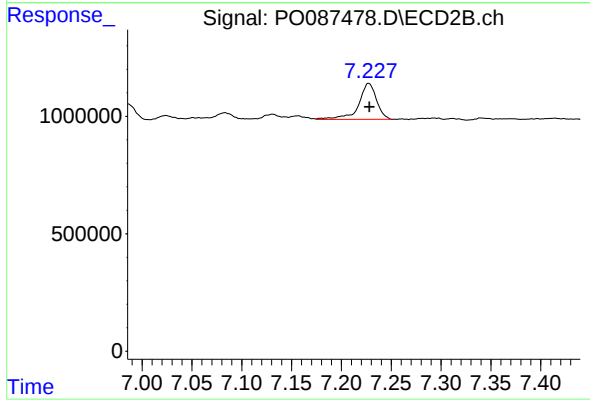

#35 AR-1260-5

R.T.: 7.227 min
Delta R.T.: 0.000 min
Response: 1915197
Conc: 17.77 ng/ml