

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062722\
 Data File : P0087479.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 08:12
 Operator : YP/AJ
 Sample : N3494-21 5X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP-EXC-1-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/28/2022
 Supervised By :Ankita Jodhani 06/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 12:07:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.450	3.610	10887212	4581431	4.206	4.656
2) SA Decachlor...	10.299	8.615	9084875	3161268	4.448	3.900
Target Compounds						
31) L7 AR-1260-1	7.239	6.173	4839485	1443834	43.170	25.575 #
32) L7 AR-1260-2	7.486	6.360	24052953	952079	176.502	14.072m#
33) L7 AR-1260-3	7.859	6.513	2844491	1293536	30.368	20.477 #
34) L7 AR-1260-4	8.085	6.985	3867676	1030968	36.973m	22.169 #
35) L7 AR-1260-5	8.415	7.227	5493796	2271856	27.850	21.076

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062722\
Data File : P0087479.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 08:12
Operator : YP/AJ
Sample : N3494-21 5X
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SP-EXC-1-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 12:07:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

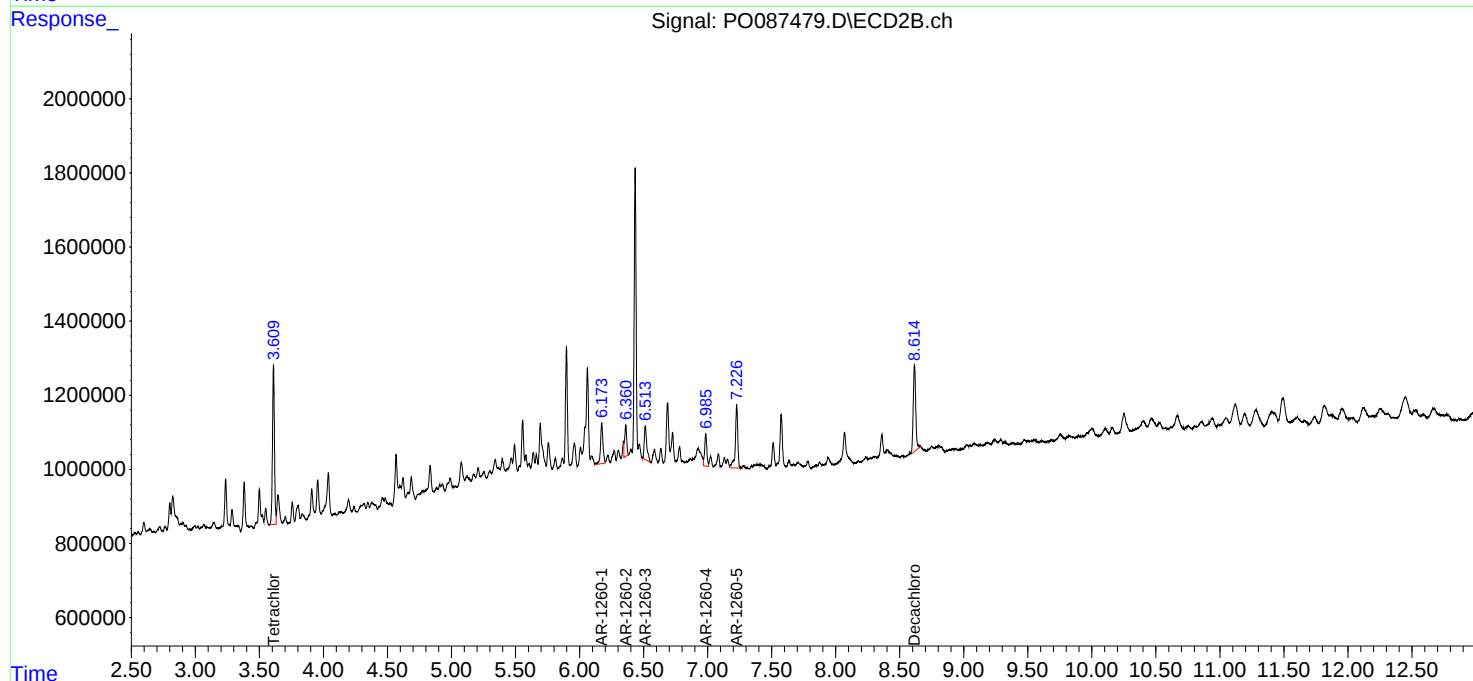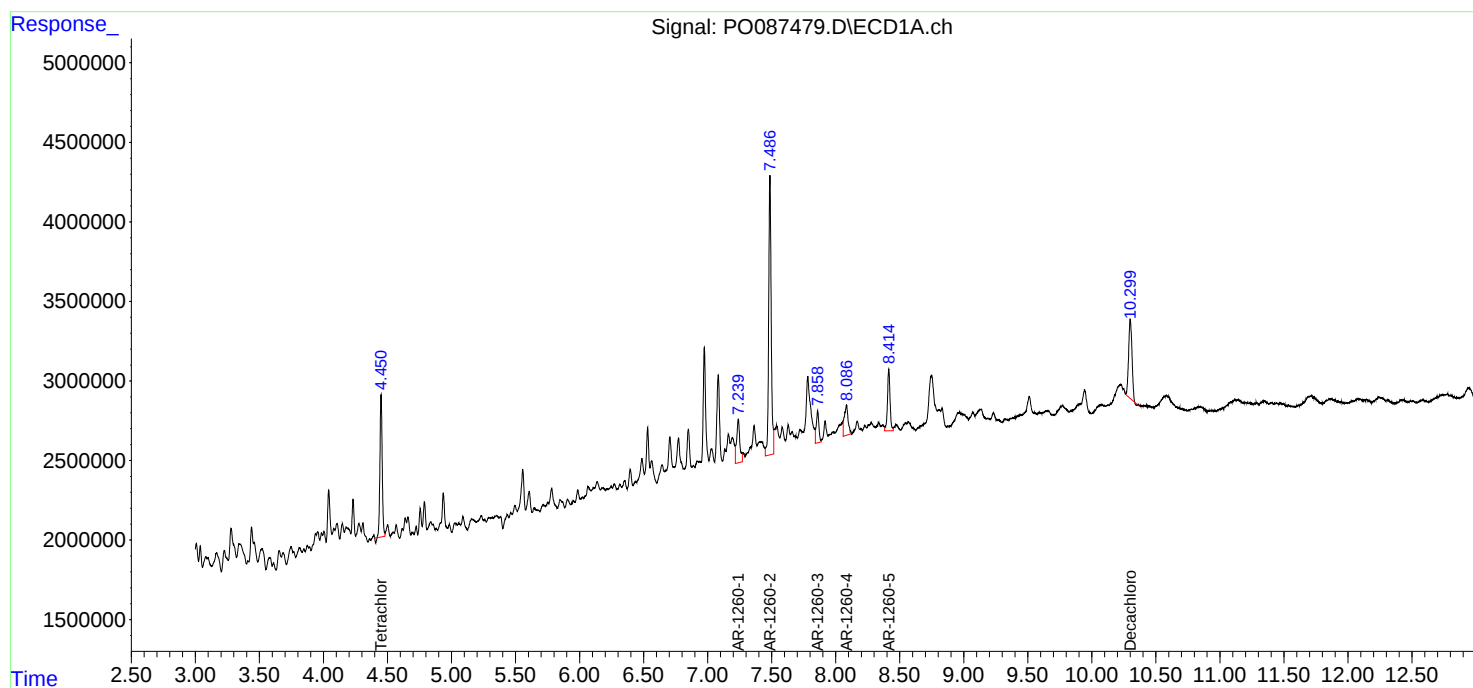

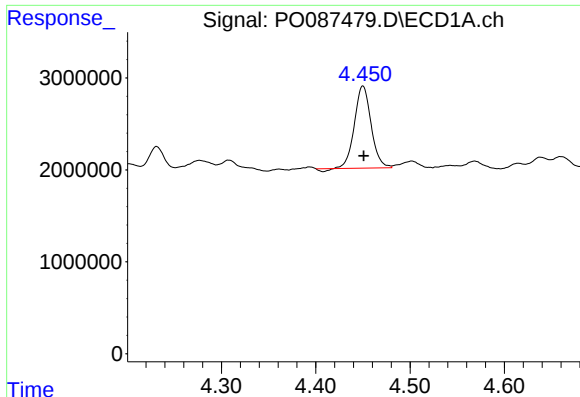


#1 Tetrachloro-m-xylene

R.T.: 4.450 min
Delta R.T.: 0.000 min
Response: 10887212
Conc: 4.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-EXC-1-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

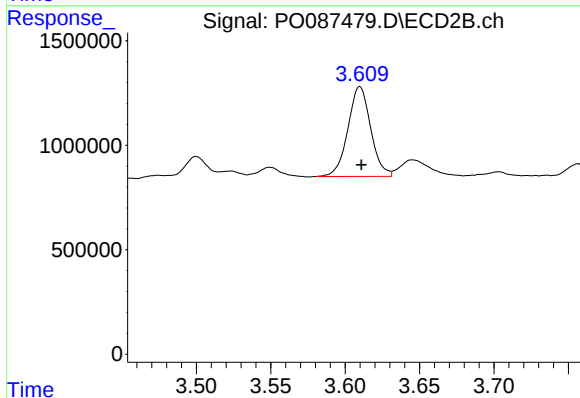


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.001 min
Response: 4581431
Conc: 4.66 ng/ml

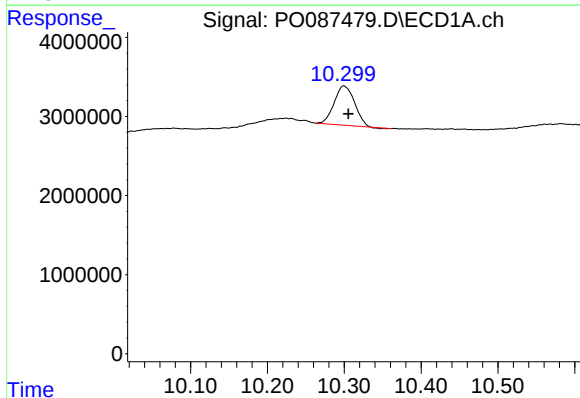


#2 Decachlorobiphenyl

R.T.: 10.299 min
Delta R.T.: -0.006 min
Response: 9084875
Conc: 4.45 ng/ml

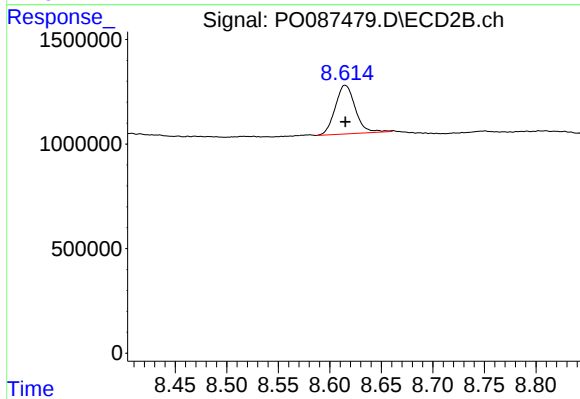

#2 Decachlorobiphenyl

R.T.: 8.615 min
Delta R.T.: 0.000 min
Response: 3161268
Conc: 3.90 ng/ml

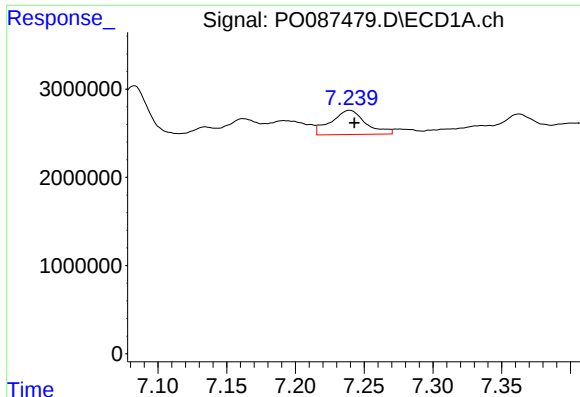


#31 AR-1260-1

R.T.: 7.239 min
Delta R.T.: -0.003 min
Response: 4839485
Conc: 43.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-EXC-1-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

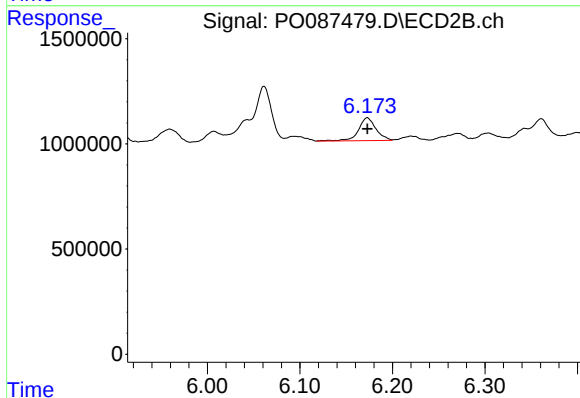


#31 AR-1260-1

R.T.: 6.173 min
Delta R.T.: 0.000 min
Response: 1443834
Conc: 25.57 ng/ml

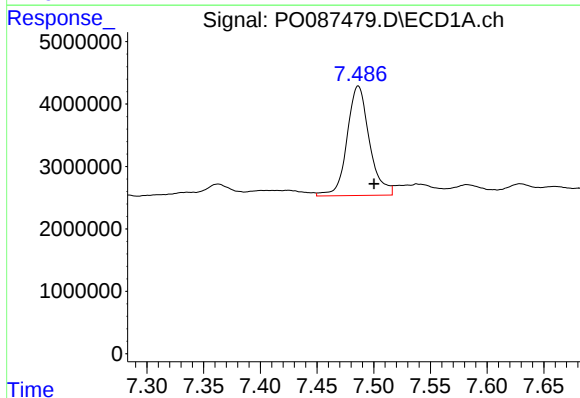


#32 AR-1260-2

R.T.: 7.486 min
Delta R.T.: -0.014 min
Response: 24052953
Conc: 176.50 ng/ml

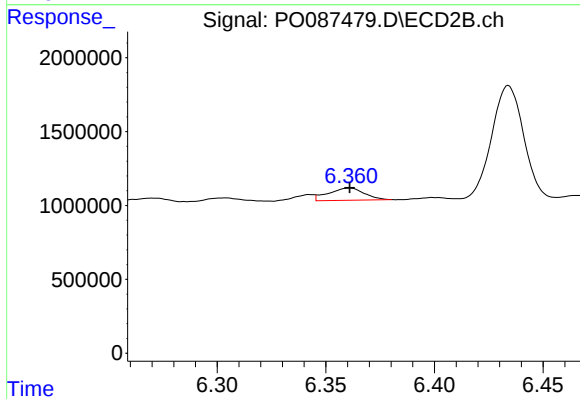

#32 AR-1260-2

R.T.: 6.360 min
Delta R.T.: 0.000 min
Response: 952079
Conc: 14.07 ng/ml m

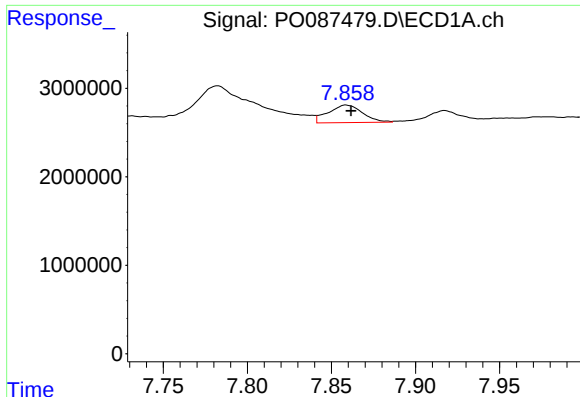


#33 AR-1260-3

R.T.: 7.859 min
Delta R.T.: -0.003 min
Response: 2844491
Conc: 30.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-EXC-1-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

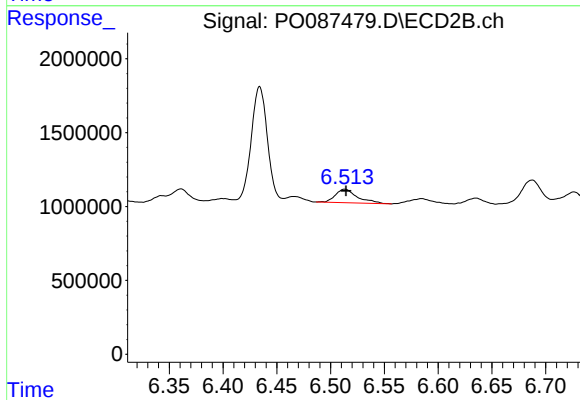


#33 AR-1260-3

R.T.: 6.513 min
Delta R.T.: -0.001 min
Response: 1293536
Conc: 20.48 ng/ml

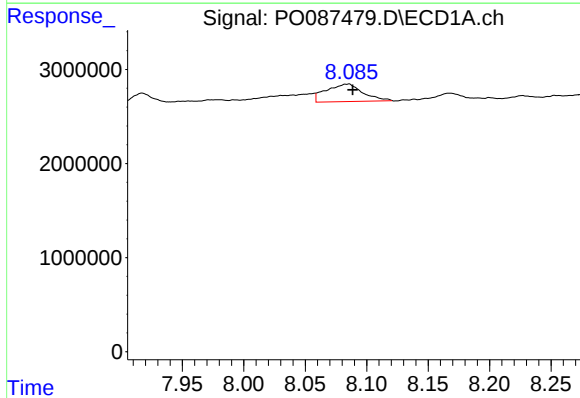


#34 AR-1260-4

R.T.: 8.085 min
Delta R.T.: -0.003 min
Response: 3867676
Conc: 36.97 ng/ml m

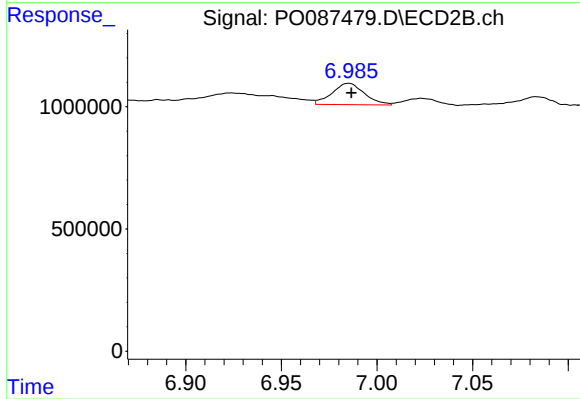

#34 AR-1260-4

R.T.: 6.985 min
Delta R.T.: -0.001 min
Response: 1030968
Conc: 22.17 ng/ml

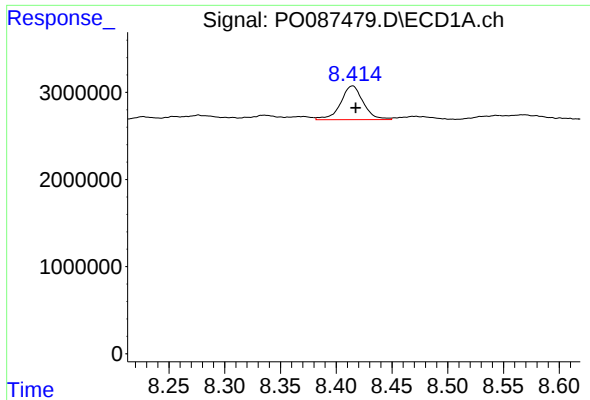


#35 AR-1260-5

R.T.: 8.415 min
Delta R.T.: -0.003 min
Response: 5493796
Conc: 27.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-EXC-1-3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2022
Supervised By :Ankita Jodhani 06/28/2022

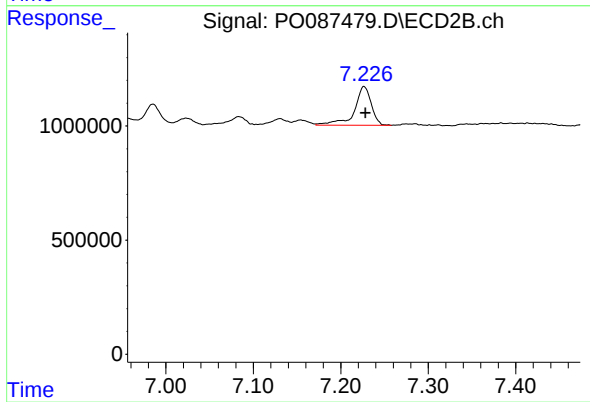

#35 AR-1260-5

R.T.: 7.227 min
Delta R.T.: -0.001 min
Response: 2271856
Conc: 21.08 ng/ml