

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062724\
 Data File : P0104493.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2024 11:53
 Operator : YP/AJ
 Sample : P3069-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 611

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/28/2024
 Supervised By :Ankita Jodhani 06/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 13:24:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 21 04:29:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.405	3.550	162.8E6	41132039	20.499m	27.405 #
2) SA Decachlor...	10.115	8.468	113.1E6	62489975	21.053	19.471

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062724\
Data File : PO104493.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2024 11:53
Operator : YP/AJ
Sample : P3069-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
611


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2024
Supervised By :Ankita Jodhani 06/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 13:24:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062024.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 21 04:29:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

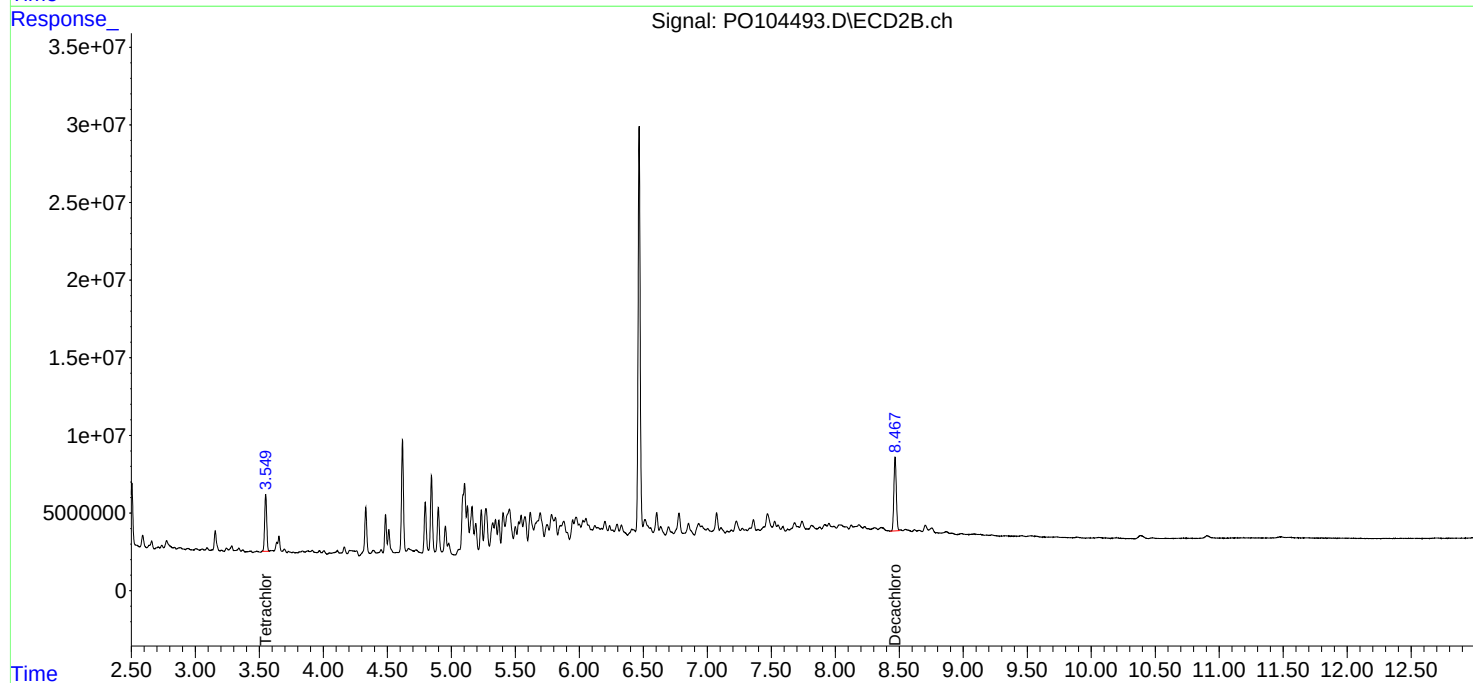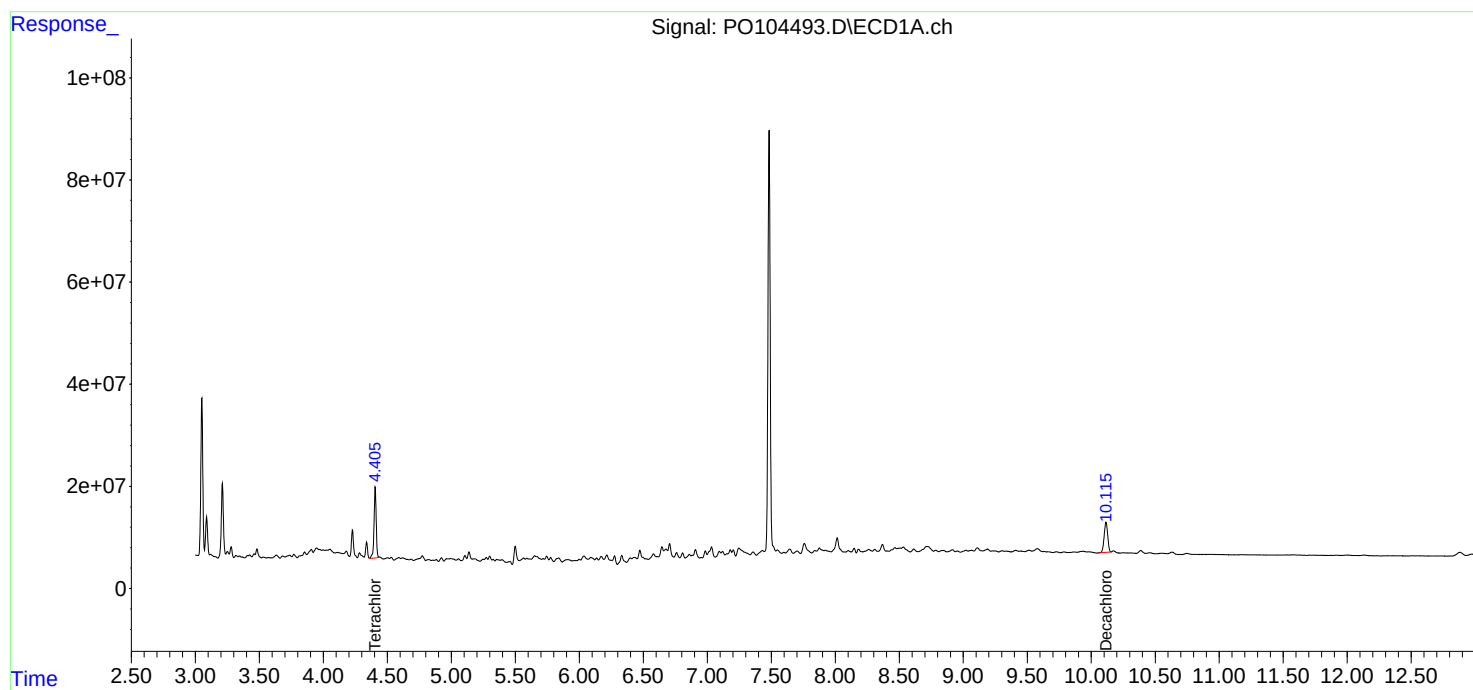

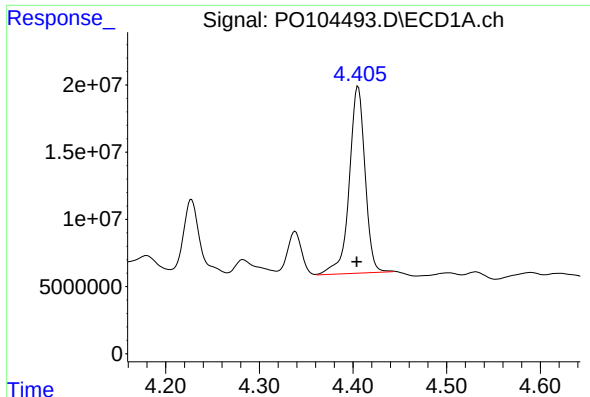


#1 Tetrachloro-m-xylene

R.T.: 4.405 min
Delta R.T.: 0.000 min
Response: 162837992
Conc: 20.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
611


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2024
Supervised By :Ankita Jodhani 06/28/2024

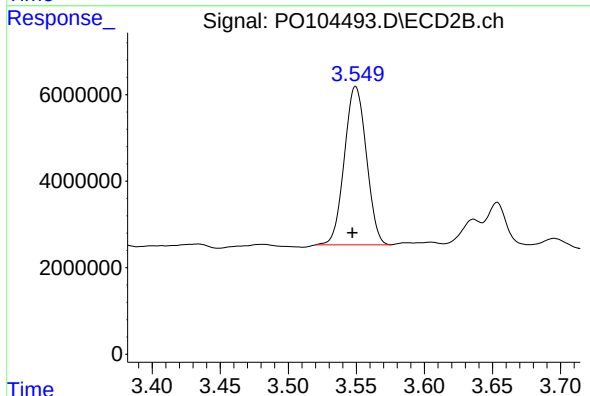


#1 Tetrachloro-m-xylene

R.T.: 3.550 min
Delta R.T.: 0.002 min
Response: 41132039
Conc: 27.40 ng/ml

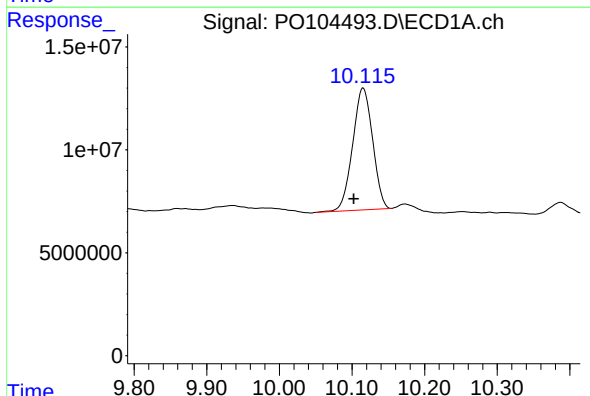

#2 Decachlorobiphenyl

R.T.: 10.115 min
Delta R.T.: 0.013 min
Response: 113114074
Conc: 21.05 ng/ml

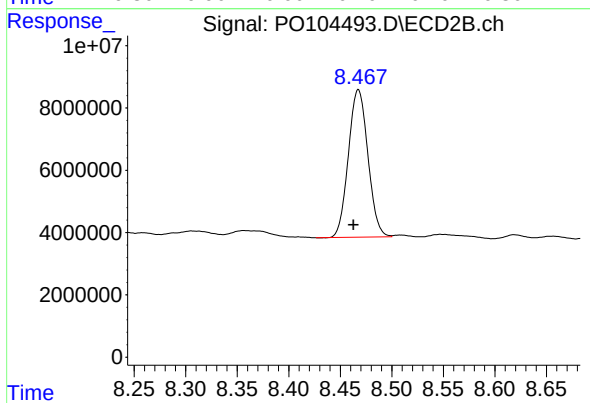

#2 Decachlorobiphenyl

R.T.: 8.468 min
Delta R.T.: 0.005 min
Response: 62489975
Conc: 19.47 ng/ml