

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062724\
 Data File : P0104495.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2024 12:27
 Operator : YP/AJ
 Sample : P3071-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 414

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/28/2024
 Supervised By :Ankita Jodhani 06/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 13:25:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 21 04:29:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.406	3.547	182.6E6	32295852	22.993	21.518m
2) SA Decachlor...	10.117	8.468	100.4E6	58526697	18.678	18.236

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062724\
Data File : PO104495.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2024 12:27
Operator : YP/AJ
Sample : P3071-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
414


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2024
Supervised By :Ankita Jodhani 06/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 13:25:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062024.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 21 04:29:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

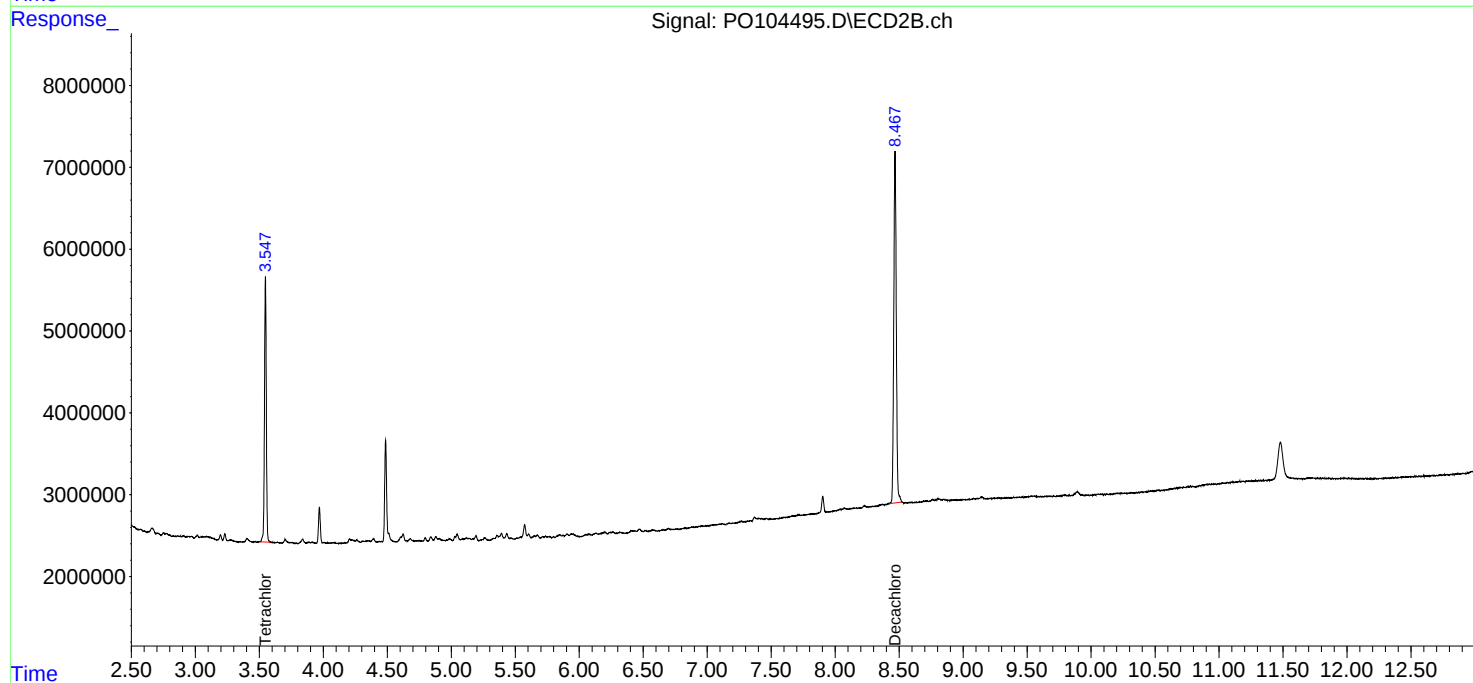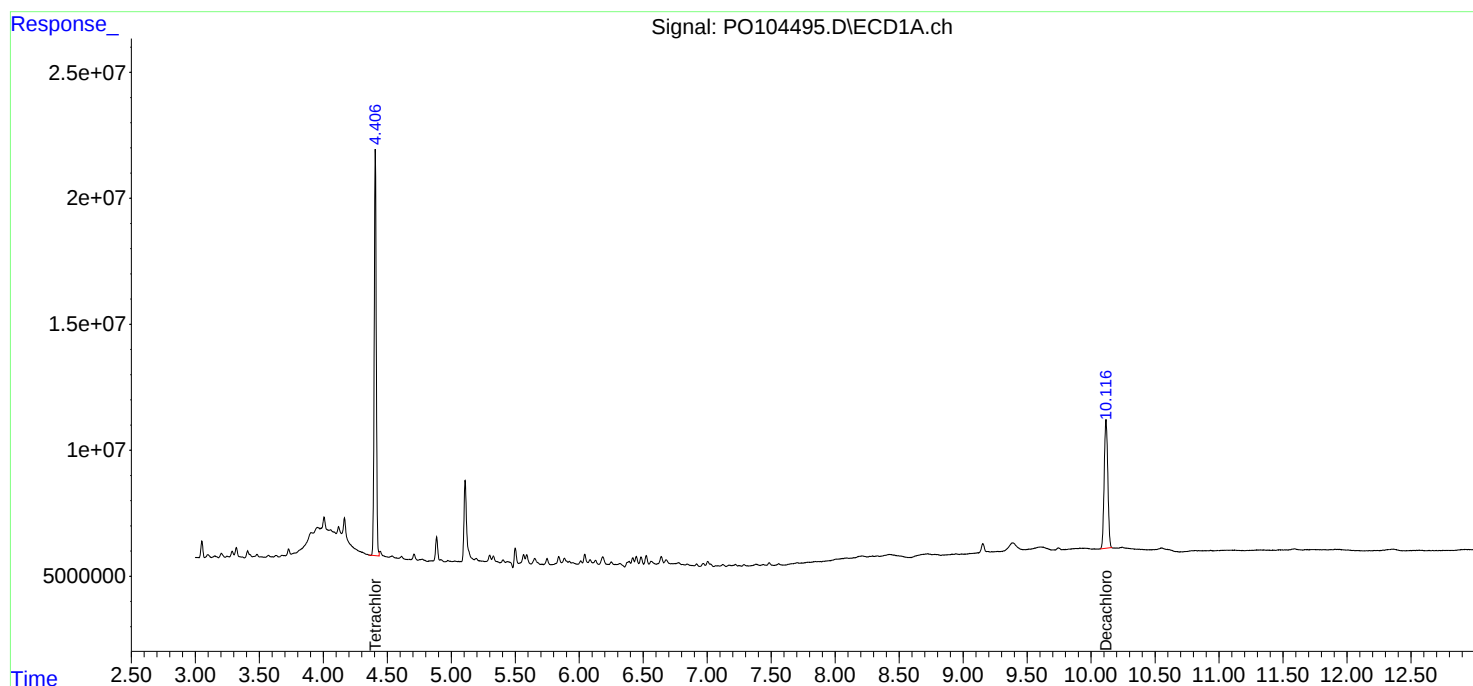

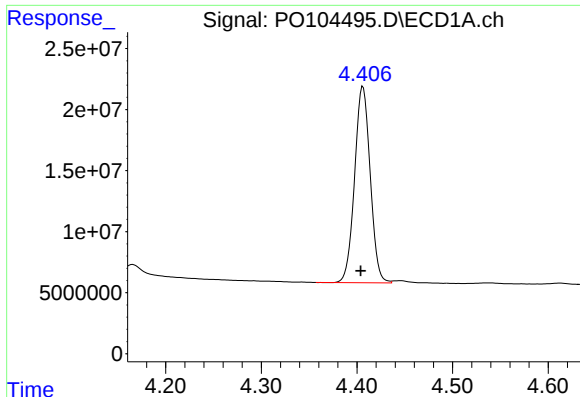


#1 Tetrachloro-m-xylene

R.T.: 4.406 min
Delta R.T.: 0.002 min
Response: 182643852
Conc: 22.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
414


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2024
Supervised By :Ankita Jodhani 06/28/2024

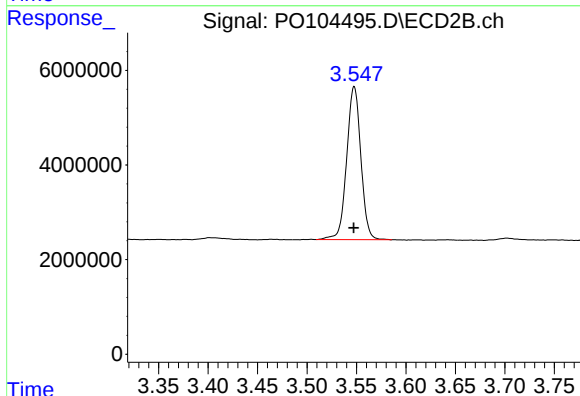


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 32295852
Conc: 21.52 ng/ml m

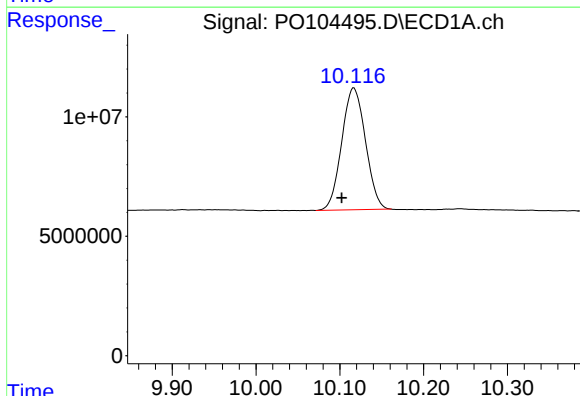

#2 Decachlorobiphenyl

R.T.: 10.117 min
Delta R.T.: 0.014 min
Response: 100354051
Conc: 18.68 ng/ml

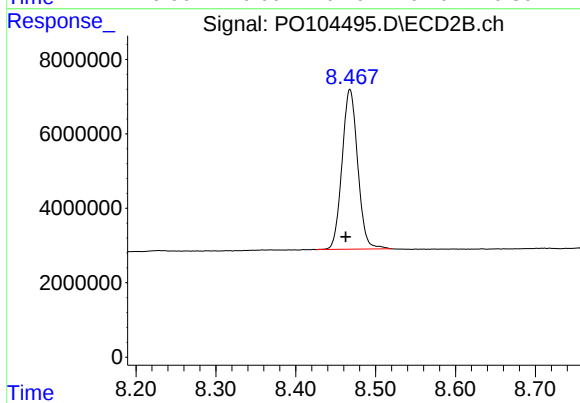

#2 Decachlorobiphenyl

R.T.: 8.468 min
Delta R.T.: 0.005 min
Response: 58526697
Conc: 18.24 ng/ml