

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062724\
 Data File : P0104522.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2024 20:41
 Operator : YP/AJ
 Sample : P3076-13
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 7-B-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/28/2024
 Supervised By :Ankita Jodhani 06/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 01:31:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 21 04:29:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.406	3.547	173.3E6	29842628	21.819	19.883
2) SA Decachlor...	10.117	8.468	112.5E6	69583149	20.937m	21.681m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062724\
Data File : PO104522.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2024 20:41
Operator : YP/AJ
Sample : P3076-13
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
7-B-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2024
Supervised By :Ankita Jodhani 06/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 01:31:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062024.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 21 04:29:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

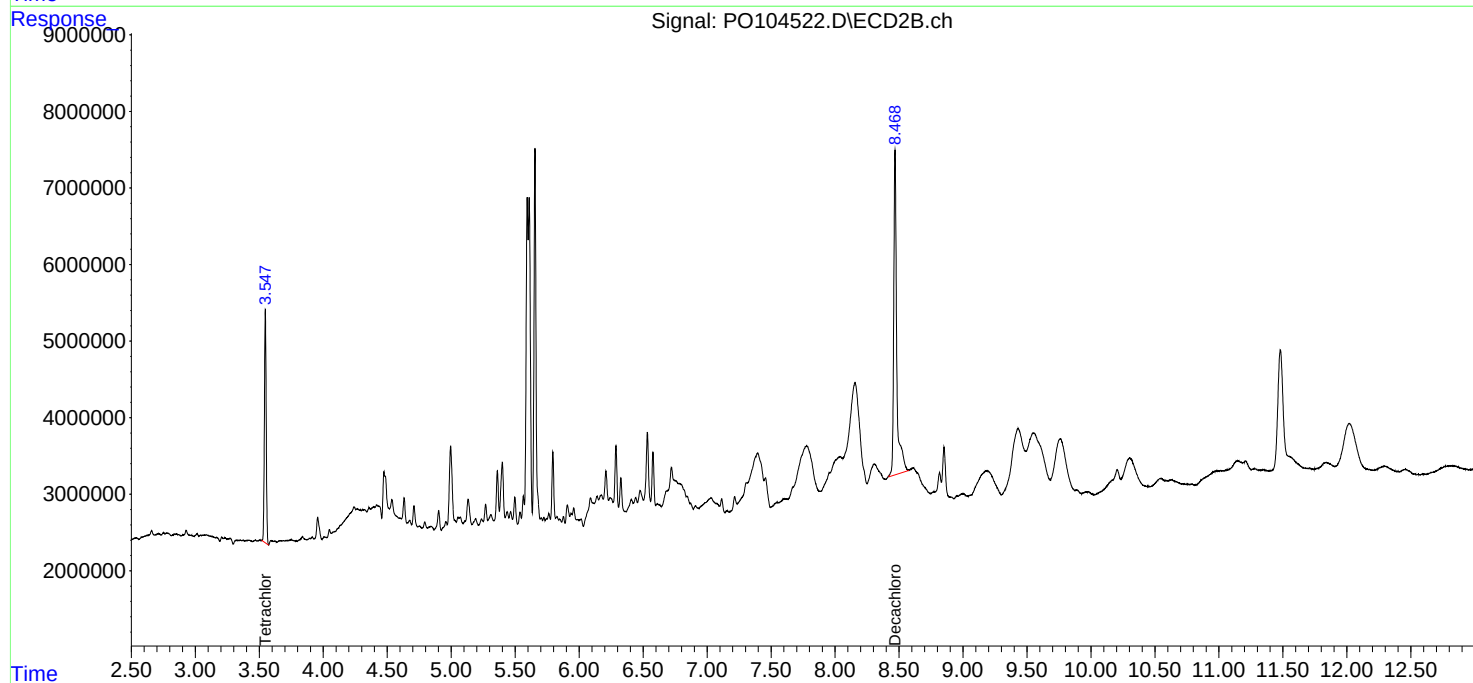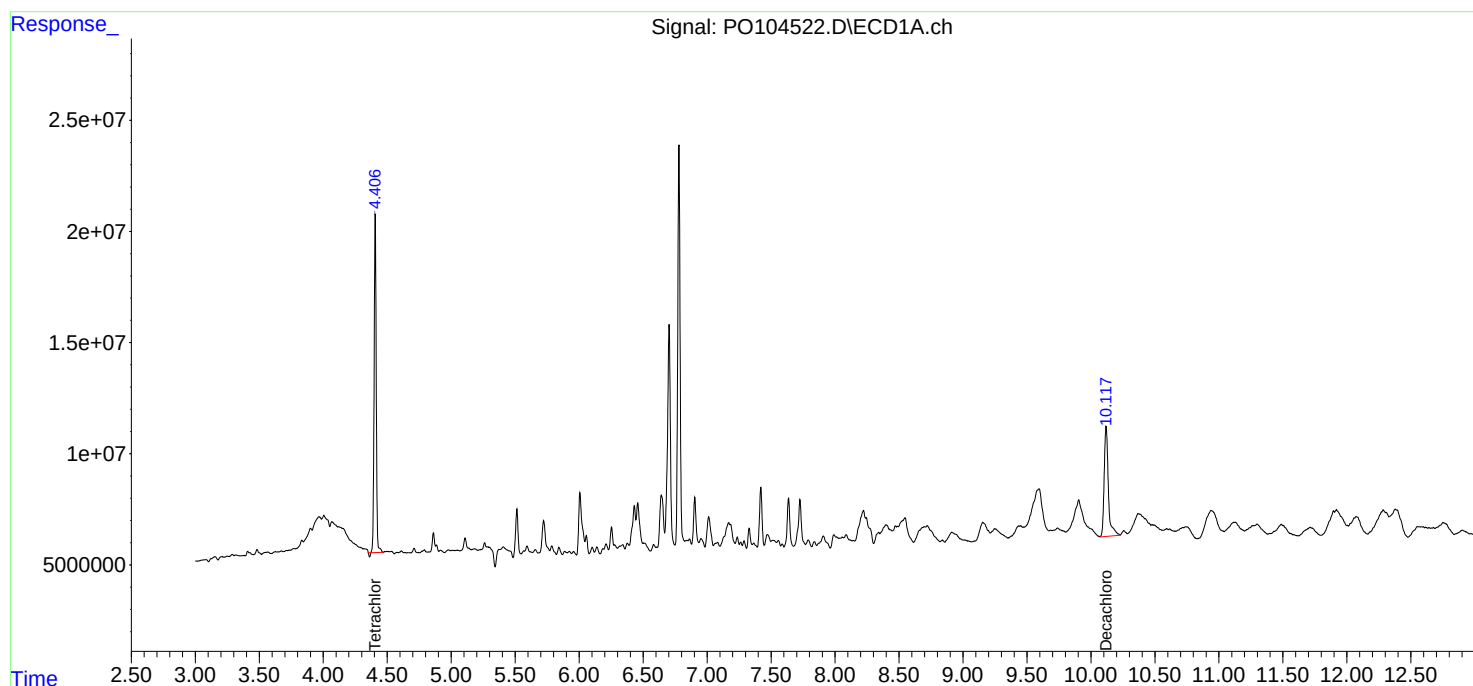

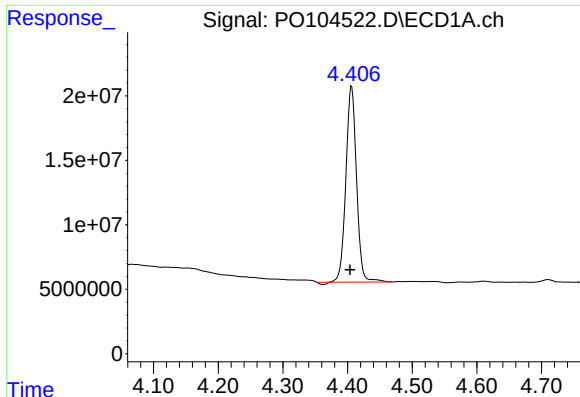


#1 Tetrachloro-m-xylene

R.T.: 4.406 min
Delta R.T.: 0.002 min
Response: 173319427
Conc: 21.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
7-B-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/28/2024
Supervised By :Ankita Jodhani 06/28/2024

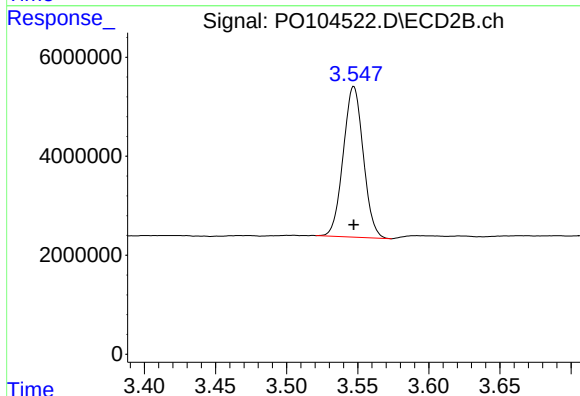


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 29842628
Conc: 19.88 ng/ml

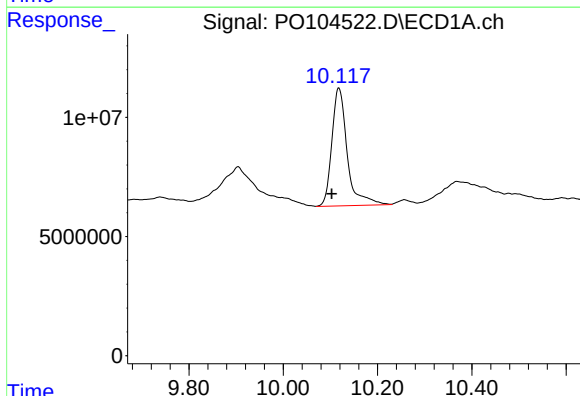

#2 Decachlorobiphenyl

R.T.: 10.117 min
Delta R.T.: 0.015 min
Response: 112489952
Conc: 20.94 ng/ml m

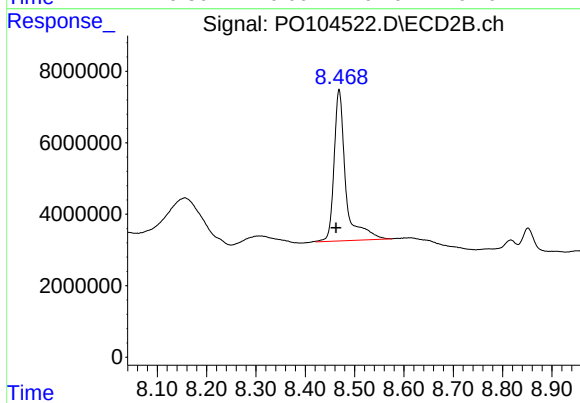

#2 Decachlorobiphenyl

R.T.: 8.468 min
Delta R.T.: 0.006 min
Response: 69583149
Conc: 21.68 ng/ml m