

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062821\
 Data File : P0079208.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jun 2021 12:29
 Operator : DD\AJ
 Sample : M2847-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1970-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 02:41:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.353f	3.637f	764486	411088	9.687m	13.832m#
2) SA Decachlor...	9.929	8.779	945019	433589	15.131	14.551

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062821\
Data File : P0079208.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jun 2021 12:29
Operator : DD\AJ
Sample : M2847-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
1970-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 02:41:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

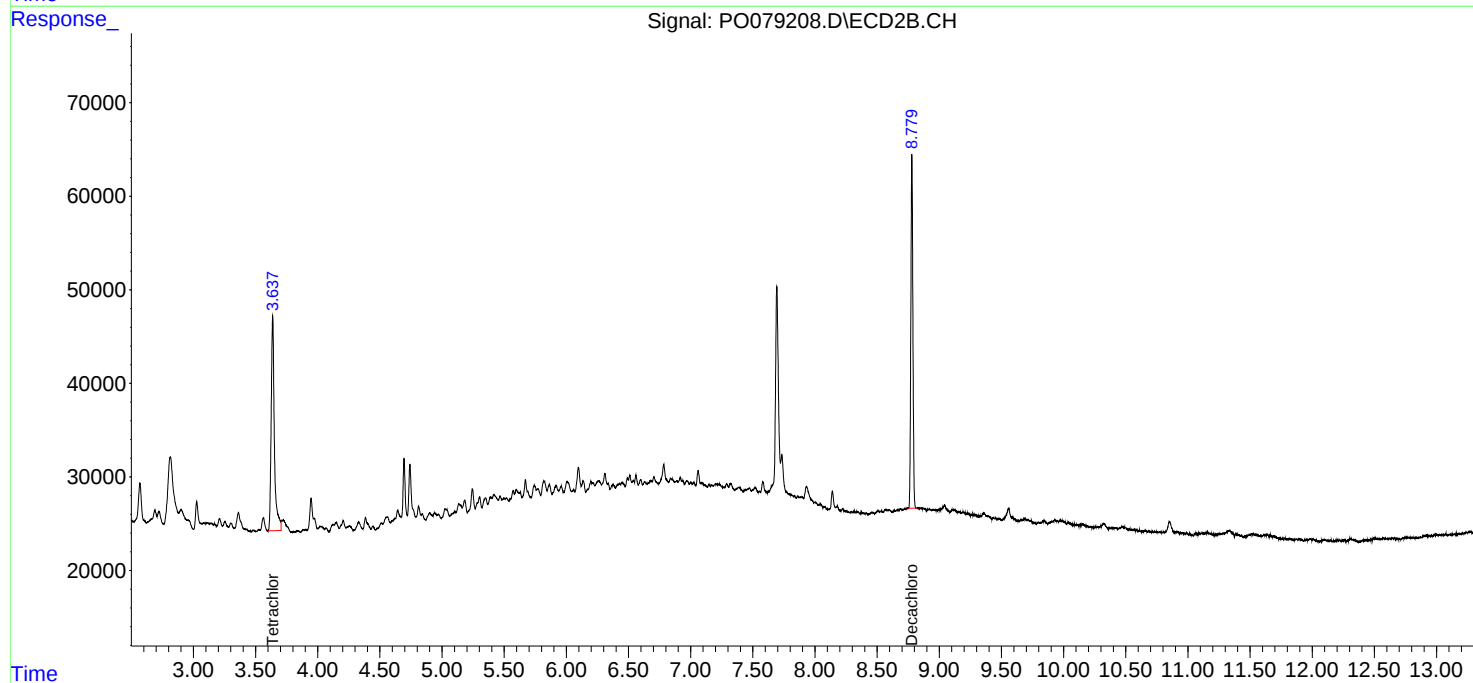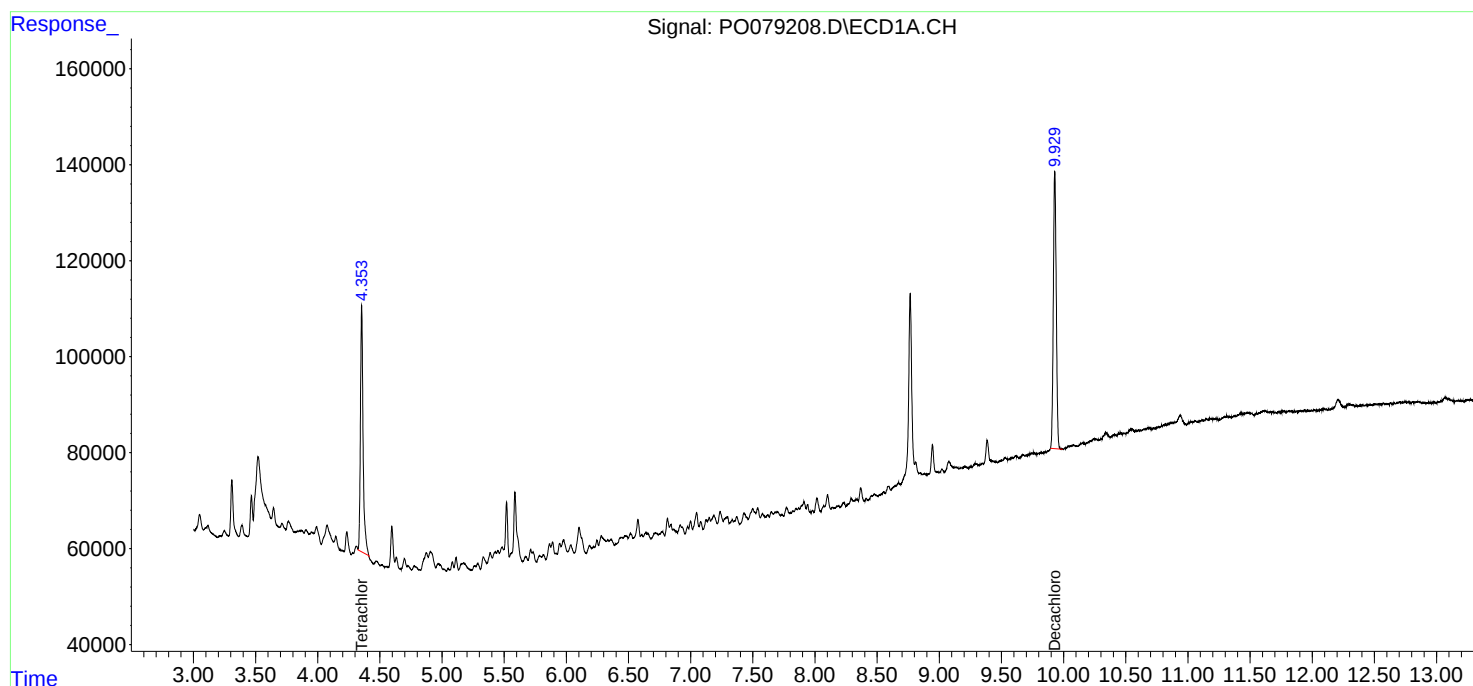


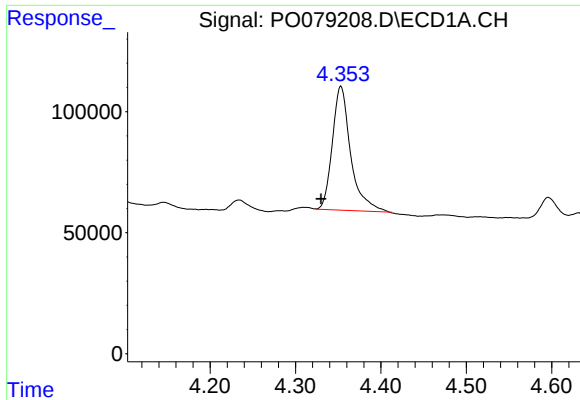

#1 Tetrachloro-m-xylene


R.T.: 4.353 min
Delta R.T.: 0.023 min
Response: 764486
Conc: 9.69 ng/ml m

Instrument :
ECD_O
ClientSampleId :
1970-WATER

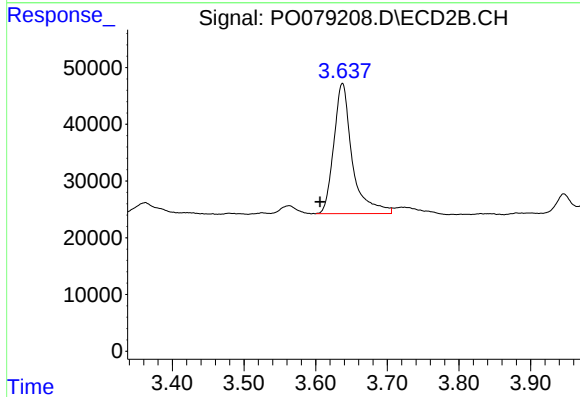


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: 0.031 min
Response: 411088
Conc: 13.83 ng/ml m

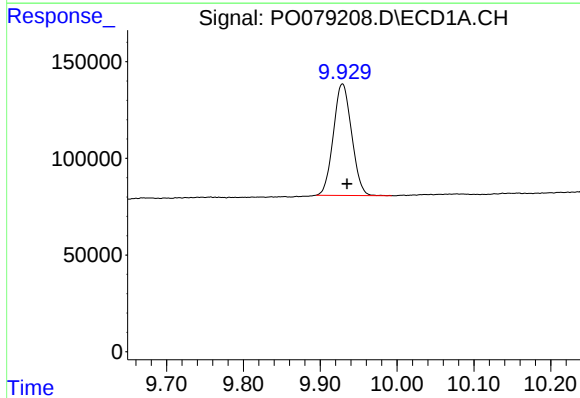

#2 Decachlorobiphenyl

R.T.: 9.929 min
Delta R.T.: -0.006 min
Response: 945019
Conc: 15.13 ng/ml

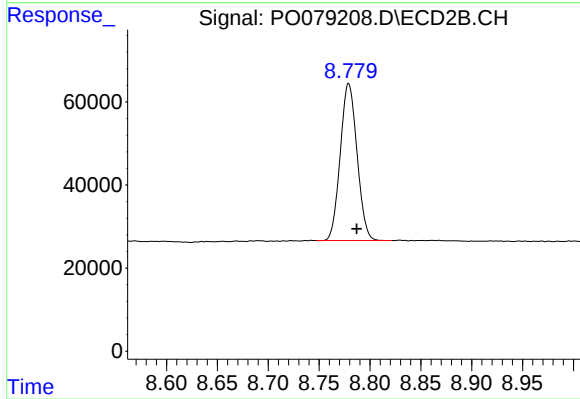

#2 Decachlorobiphenyl

R.T.: 8.779 min
Delta R.T.: -0.008 min
Response: 433589
Conc: 14.55 ng/ml