

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062822\
 Data File : P0087503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 16:53
 Operator : YP/AJ
 Sample : N3499-04 (Sig #1); N3499-4 (Sig #2)
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 31052-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 17:35:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.460	3.624	67712640	19386385	26.161	19.702
2) SA Decachlor...	10.310	8.622	33208693	11805134	16.258	14.562

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062822\
Data File : P0087503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 16:53
Operator : YP/AJ
Sample : N3499-04 (Sig #1); N3499-4 (Sig #2)
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
31052-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 17:35:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

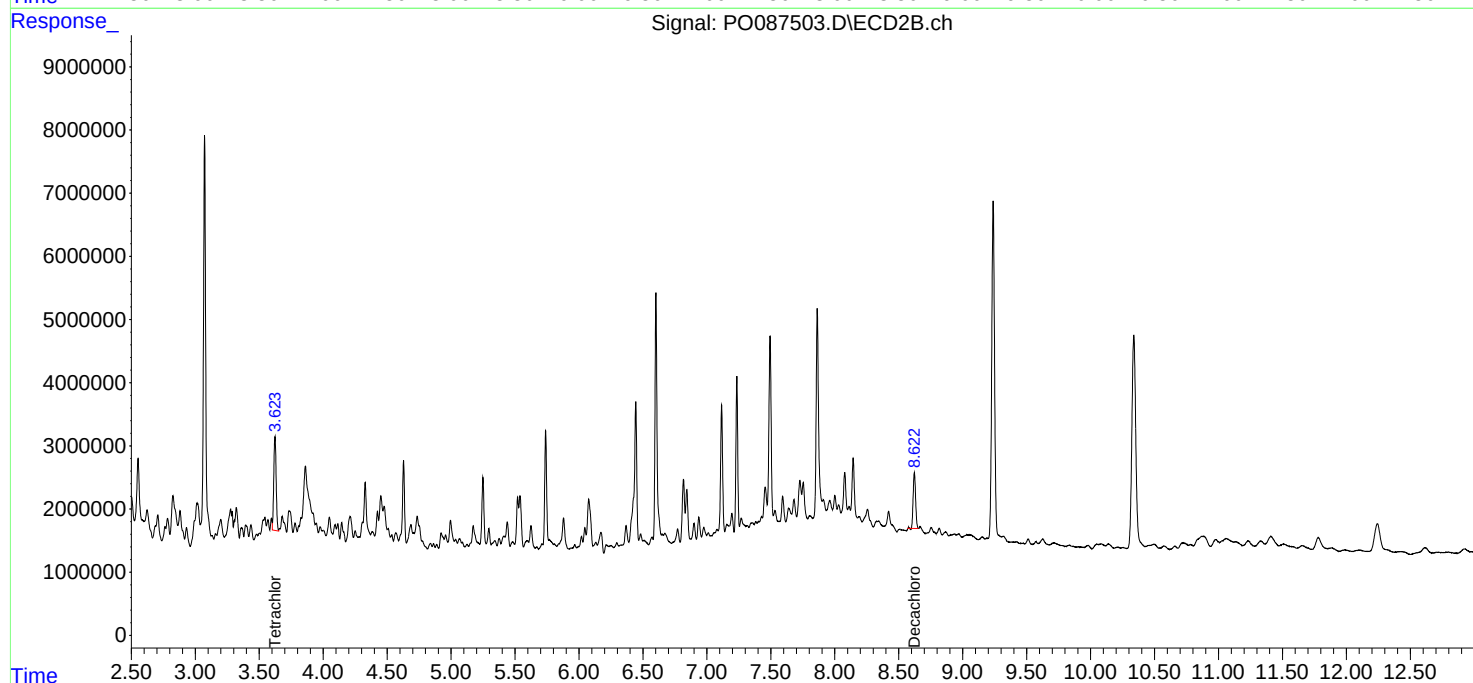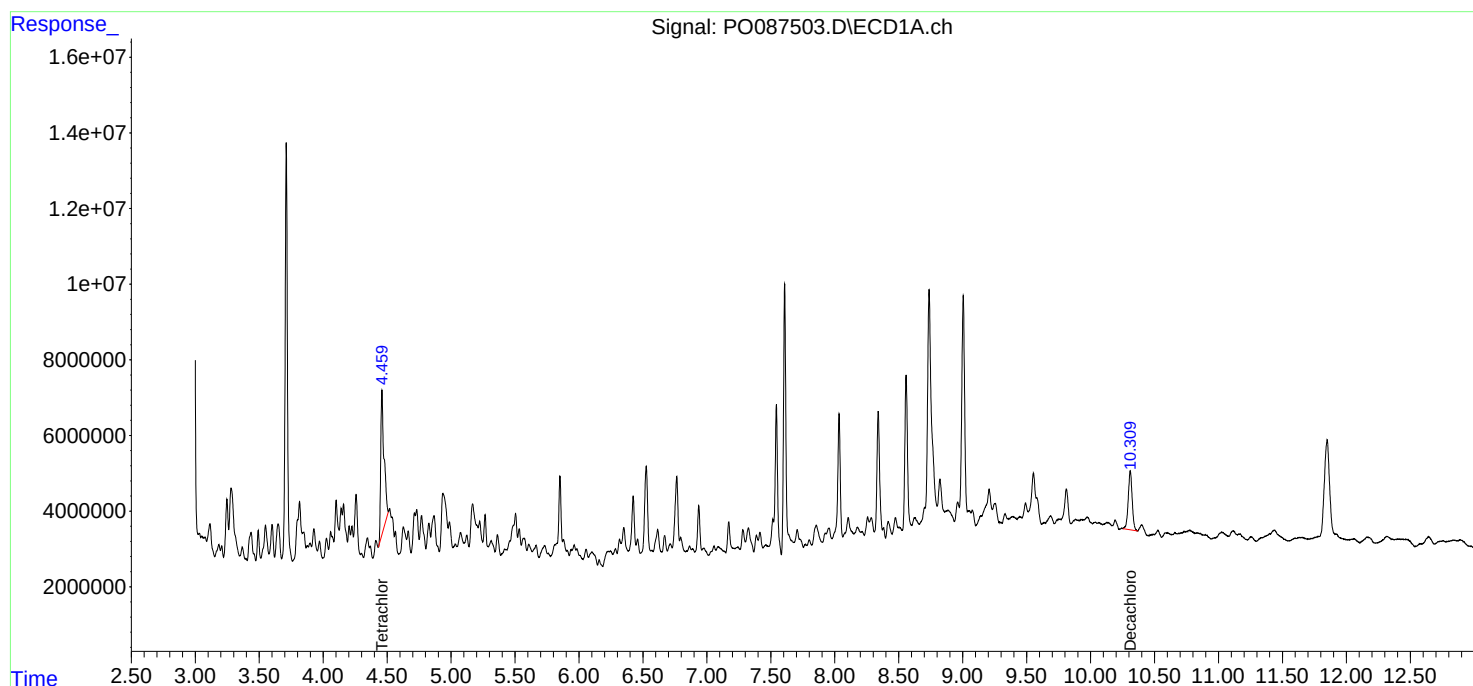


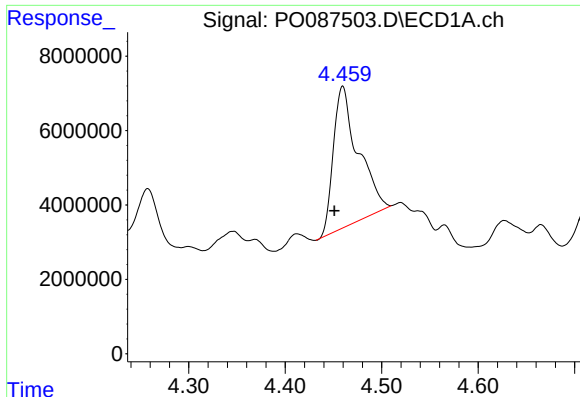

#1 Tetrachloro-m-xylene


R.T.: 4.460 min
Delta R.T.: 0.009 min
Response: 67712640
Conc: 26.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
31052-WATER

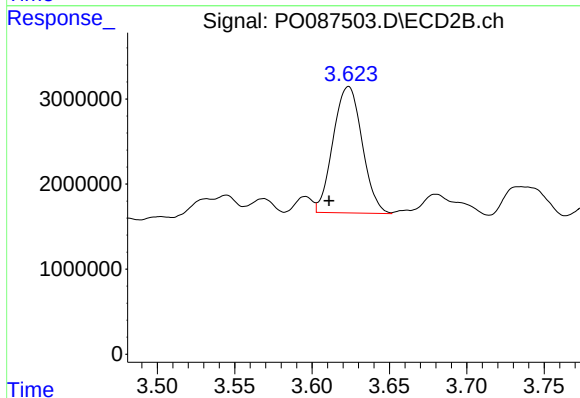


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: 0.013 min
Response: 19386385
Conc: 19.70 ng/ml

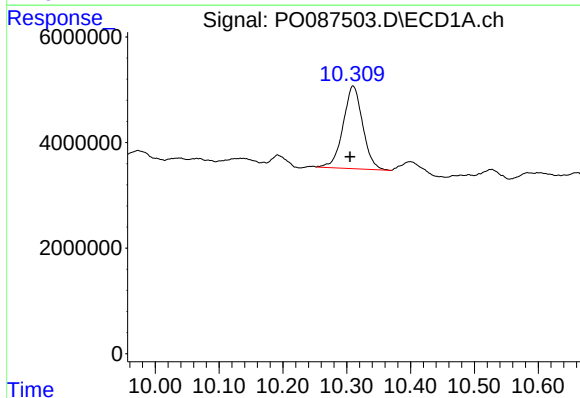

#2 Decachlorobiphenyl

R.T.: 10.310 min
Delta R.T.: 0.005 min
Response: 33208693
Conc: 16.26 ng/ml

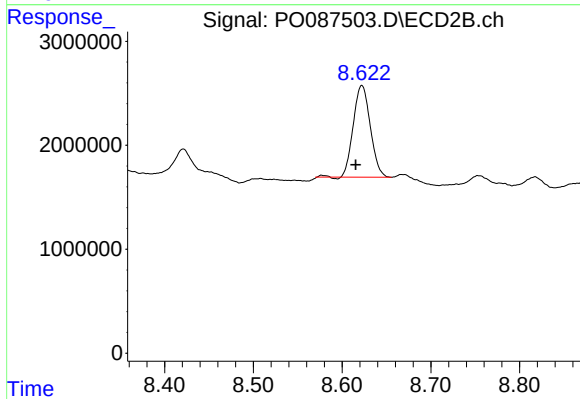

#2 Decachlorobiphenyl

R.T.: 8.622 min
Delta R.T.: 0.007 min
Response: 11805134
Conc: 14.56 ng/ml