

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062920\
 Data File : P0069285.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jun 2020 14:57
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 01:34:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.399	3.563	639426	687346	21.615	17.858
2)	SA Decachlor...	10.063	8.773	808754	777278	17.028	14.279
Target Compounds							
26)	L6 AR-1254-1	6.550	0.000	47824	0	32.561	N.D. #
28)	L6 AR-1254-3	0.000	6.206	0	111474	N.D.	32.707 #
31)	L7 AR-1260-1	7.397	0.000	423614	0	221.970	N.D. #
32)	L7 AR-1260-2	7.692	0.000	457363	0	195.411	N.D. #
38)	L8 AR-1262-3	8.788	0.000	146247	0	68.873	N.D. #
39)	L8 AR-1262-4	8.915	0.000	456919	0	186.127	N.D. #
41)	L9 AR-1268-1	8.788	0.000	146247	0	21.817	N.D. #
42)	L9 AR-1268-2	8.915	0.000	456919	0	71.551	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062920\
Data File : P0069285.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jun 2020 14:57
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 01:34:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

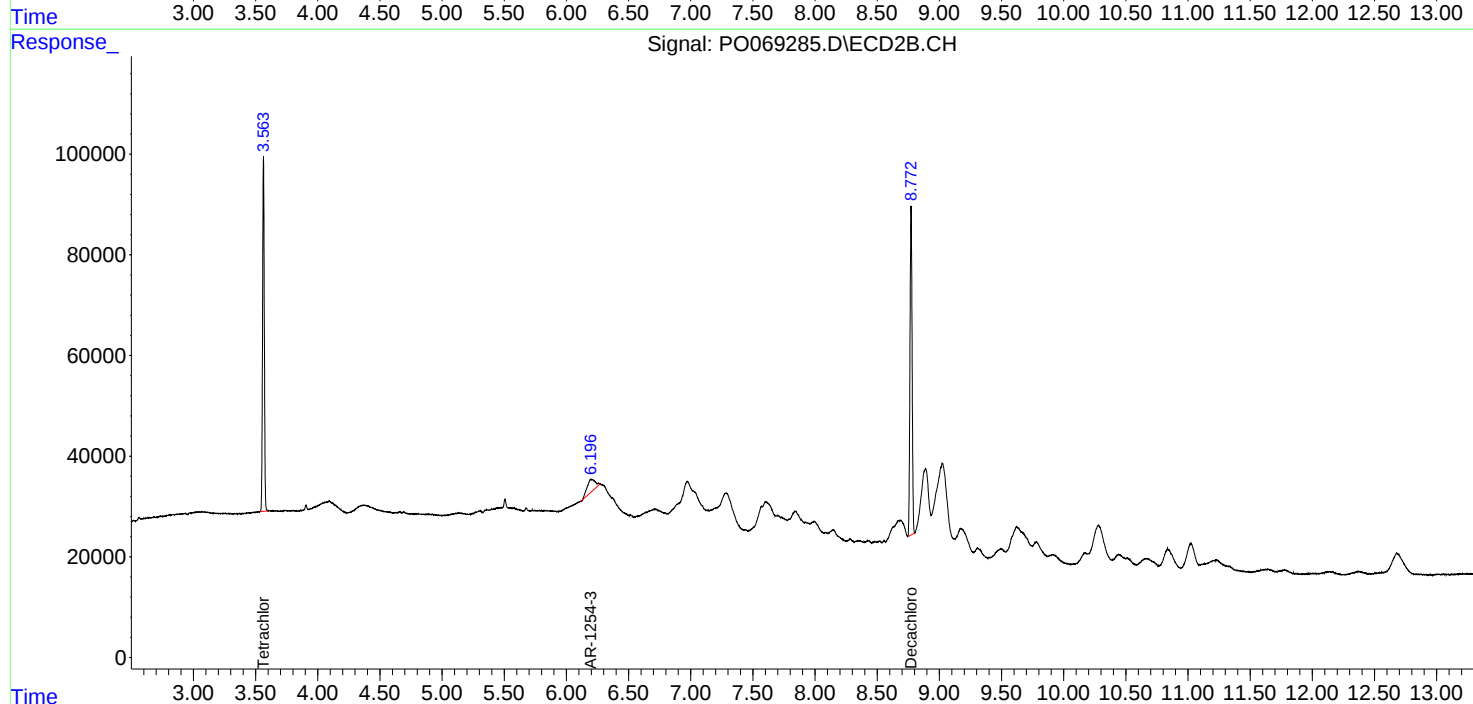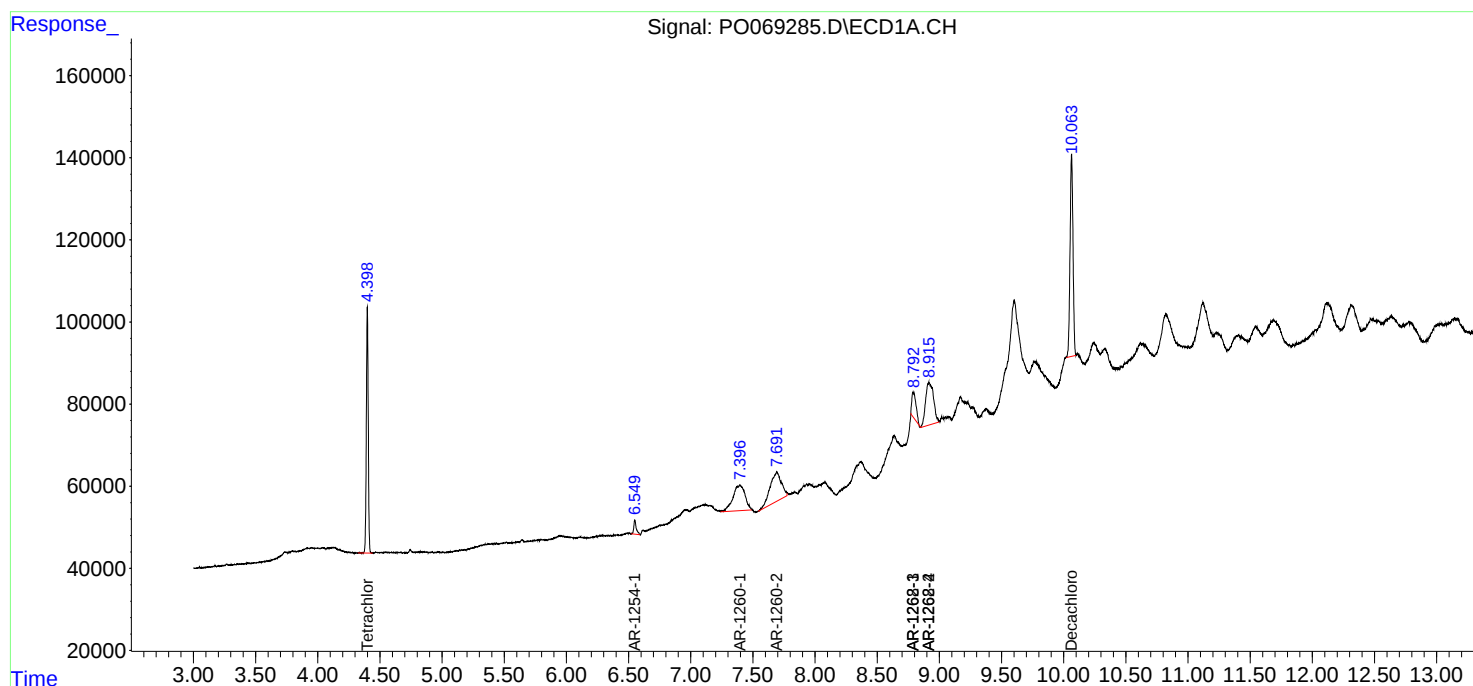


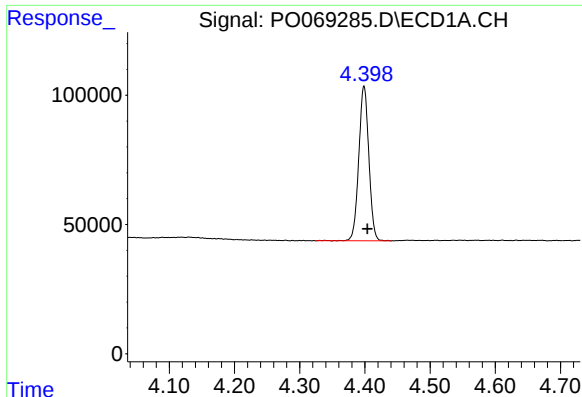

#1 Tetrachloro-m-xylene


R.T.: 4.399 min
Delta R.T.: -0.005 min
Response: 639426
Conc: 21.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

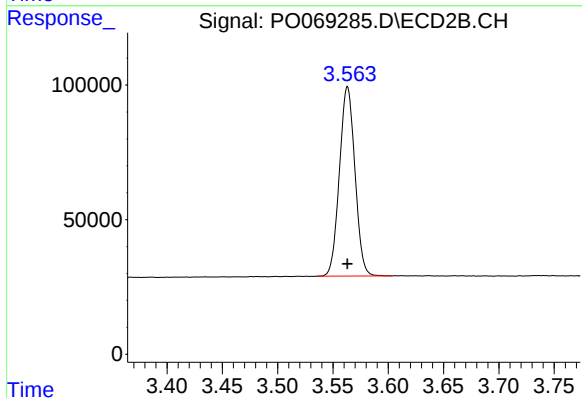


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 687346
Conc: 17.86 ng/ml

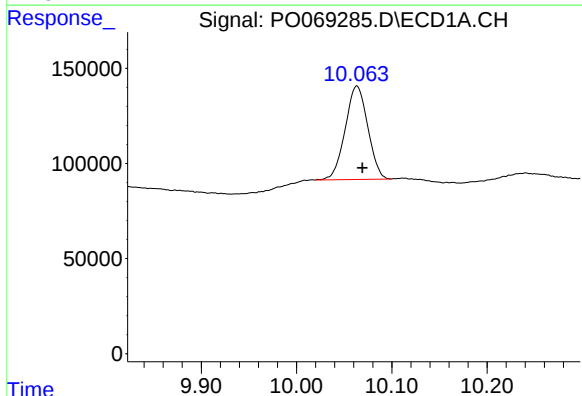


#2 Decachlorobiphenyl

R.T.: 10.063 min
Delta R.T.: -0.006 min
Response: 808754
Conc: 17.03 ng/ml

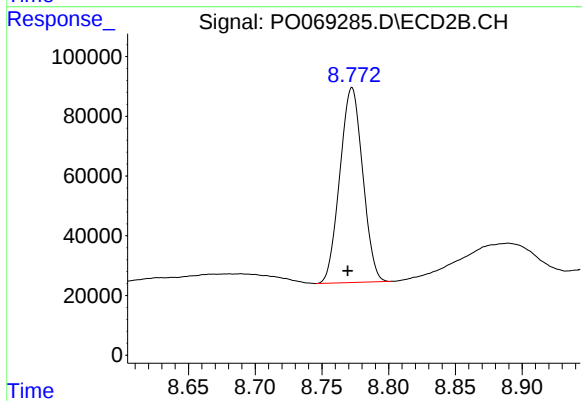

#2 Decachlorobiphenyl


R.T.: 8.773 min
Delta R.T.: 0.003 min
Response: 777278
Conc: 14.28 ng/ml

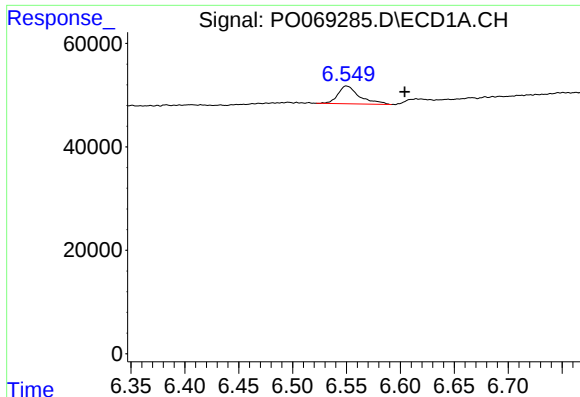

#26 AR-1254-1


R.T.: 6.550 min
Delta R.T.: -0.054 min
Response: 47824
Conc: 32.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

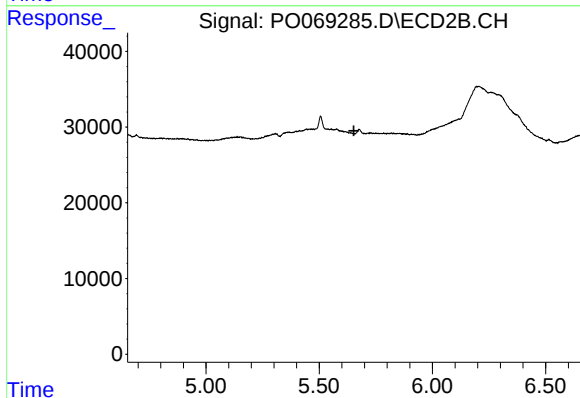


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.653 min
Response: 0
Conc: N.D.

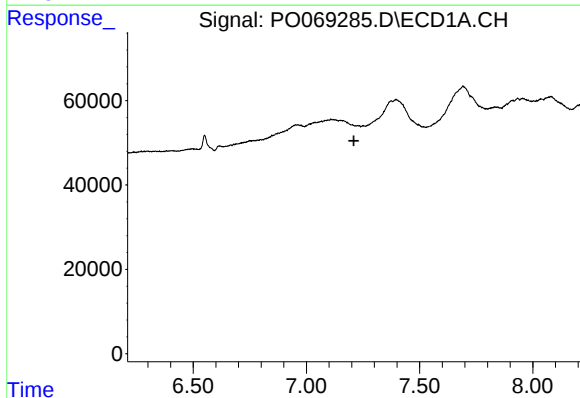


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 7.209 min
Response: 0
Conc: N.D.

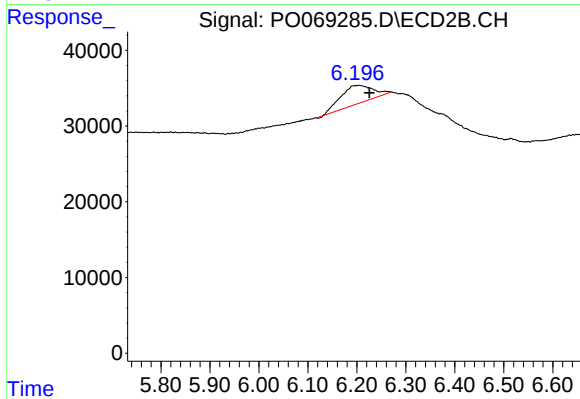

#28 AR-1254-3


R.T.: 6.206 min
Delta R.T.: -0.020 min
Response: 111474
Conc: 32.71 ng/ml

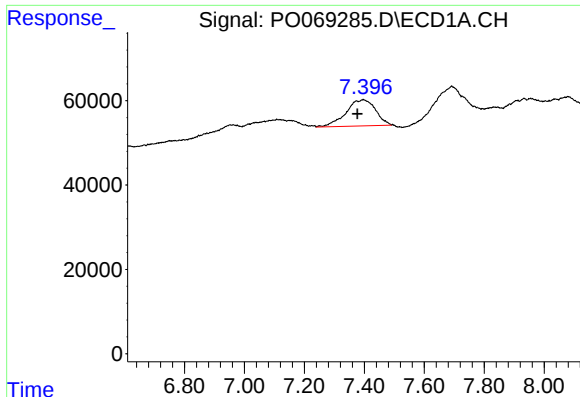

#31 AR-1260-1


R.T.: 7.397 min
Delta R.T.: 0.019 min
Response: 423614
Conc: 221.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

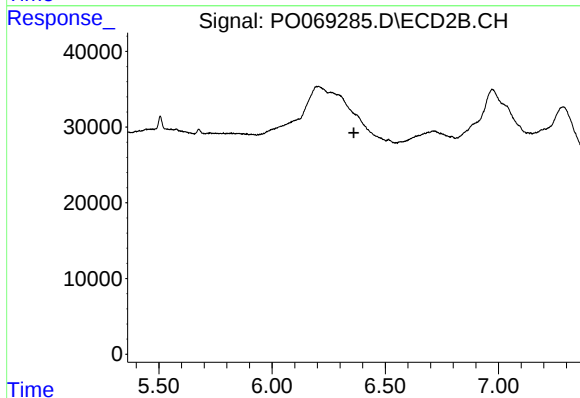


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.362 min
Response: 0
Conc: N.D.

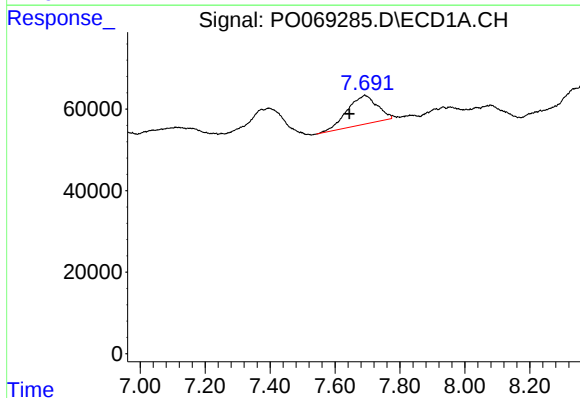


#32 AR-1260-2

R.T.: 7.692 min
Delta R.T.: 0.047 min
Response: 457363
Conc: 195.41 ng/ml

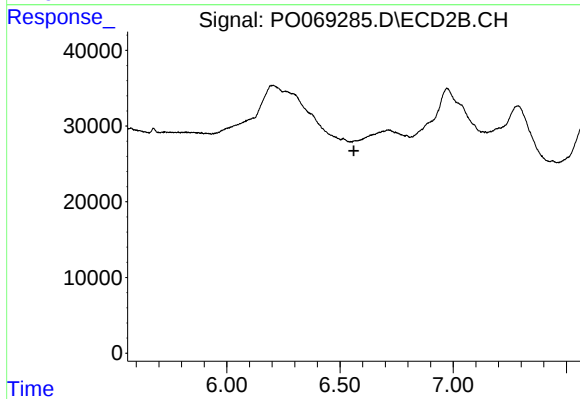

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.561 min
Response: 0
Conc: N.D.

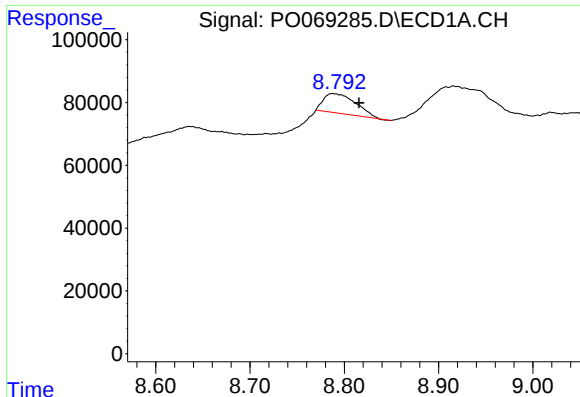

#38 AR-1262-3


R.T.: 8.788 min
Delta R.T.: -0.028 min
Response: 146247
Conc: 68.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

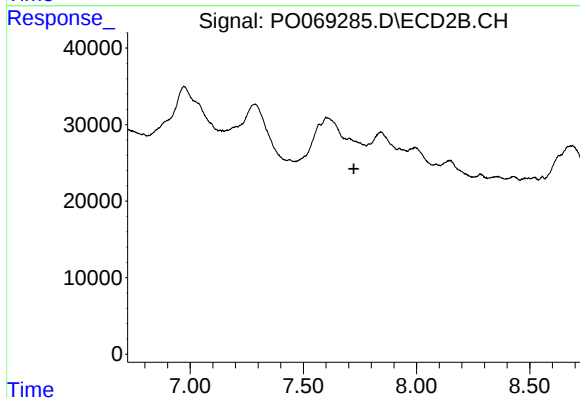


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 7.723 min
Response: 0
Conc: N.D.

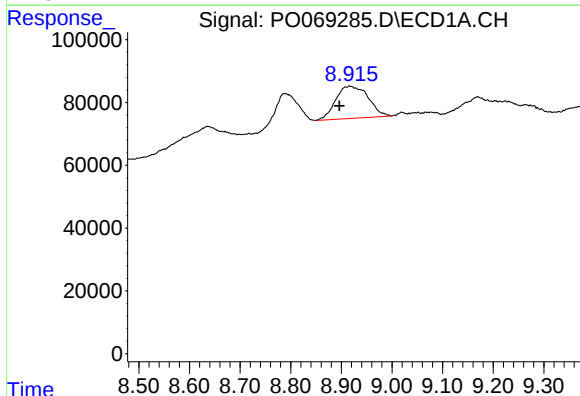


#39 AR-1262-4

R.T.: 8.915 min
Delta R.T.: 0.019 min
Response: 456919
Conc: 186.13 ng/ml

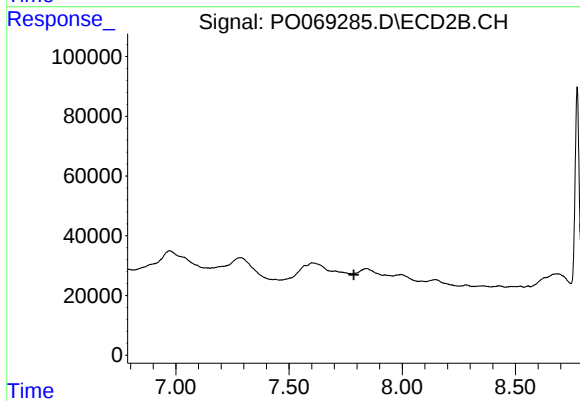

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 7.786 min
Response: 0
Conc: N.D.

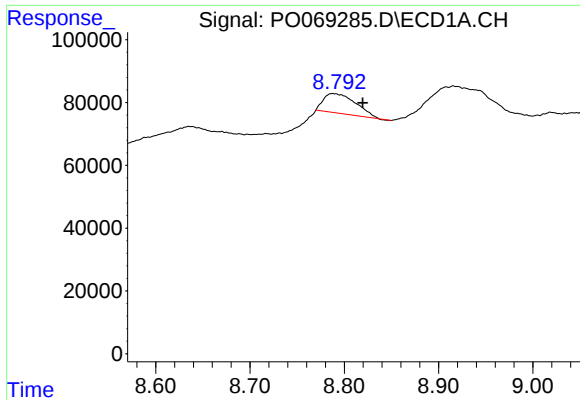

#41 AR-1268-1


R.T.: 8.788 min
Delta R.T.: -0.032 min
Response: 146247
Conc: 21.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

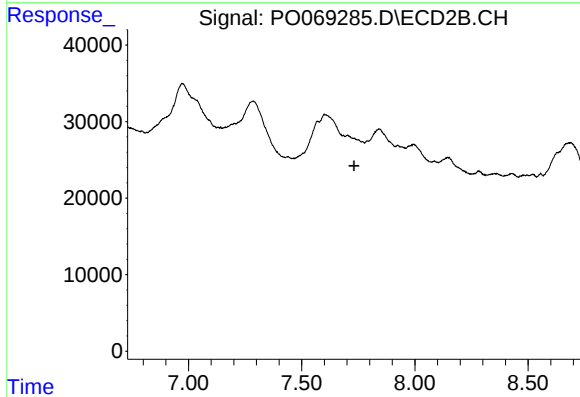


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.731 min
Response: 0
Conc: N.D.

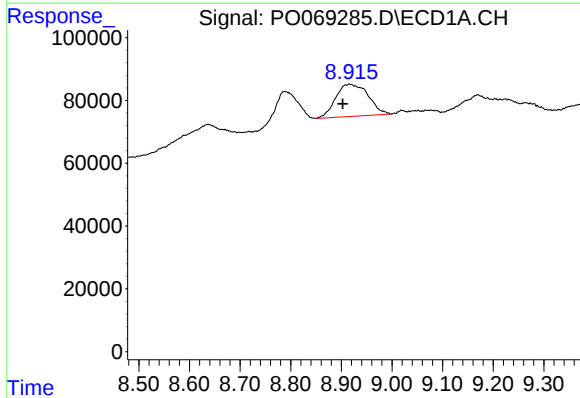

#42 AR-1268-2

R.T.: 8.915 min
Delta R.T.: 0.012 min
Response: 456919
Conc: 71.55 ng/ml

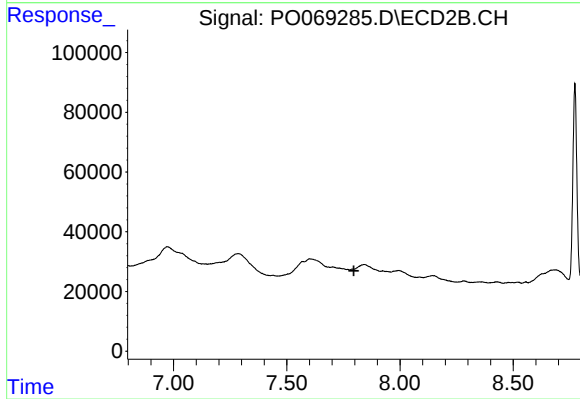

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.797 min
Response: 0
Conc: N.D.