

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062920\
 Data File : P0069303.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jun 2020 21:13
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 01:42:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.400	3.564	625856	643119	21.156	16.709
2) SA Decachlor...	10.063	8.774	882063	862200	18.571	15.839
Target Compounds						
26) L6 AR-1254-1	6.552	0.000	64395	0	43.843	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062920\
Data File : P0069303.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jun 2020 21:13
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 01:42:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

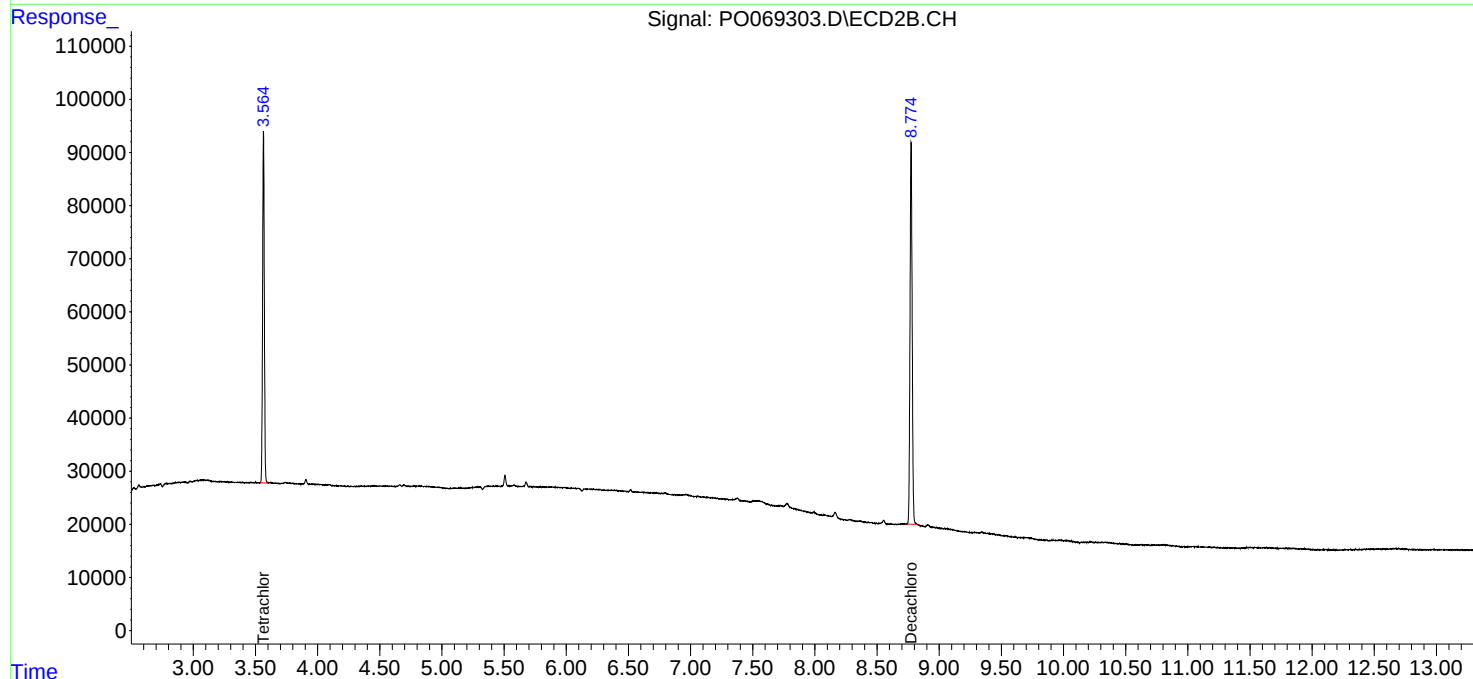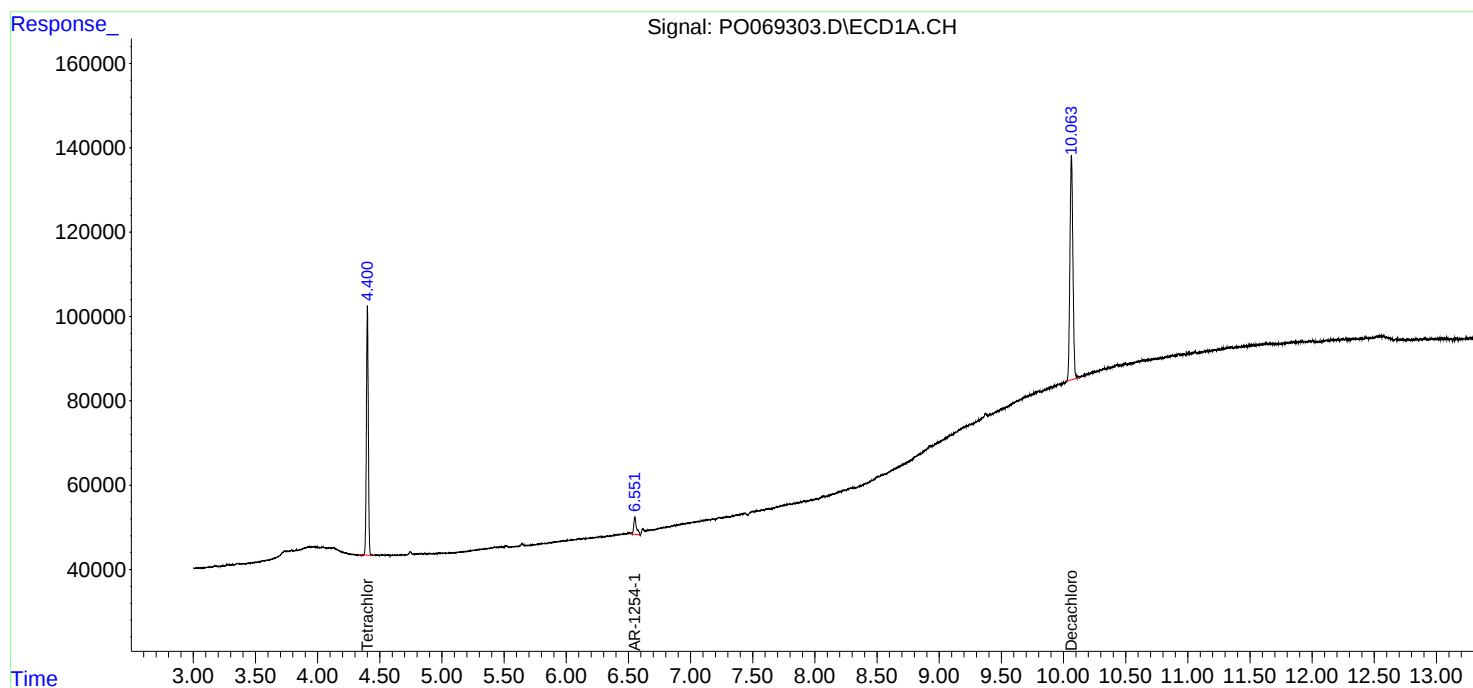


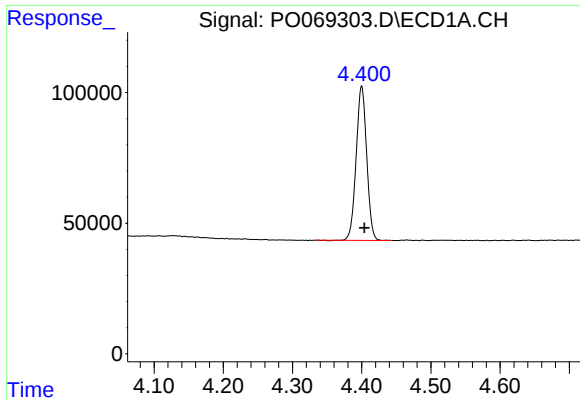

#1 Tetrachloro-m-xylene


R.T.: 4.400 min
Delta R.T.: -0.004 min
Response: 625856
Conc: 21.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

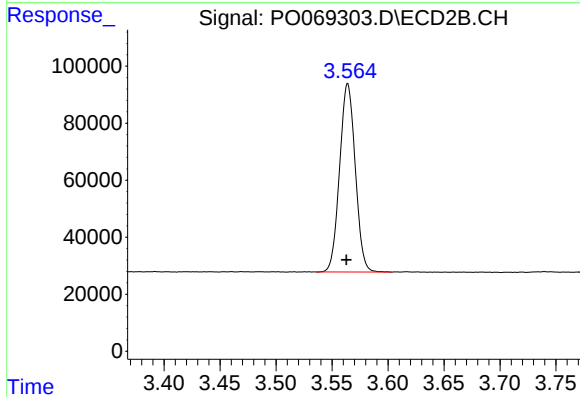


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.001 min
Response: 643119
Conc: 16.71 ng/ml

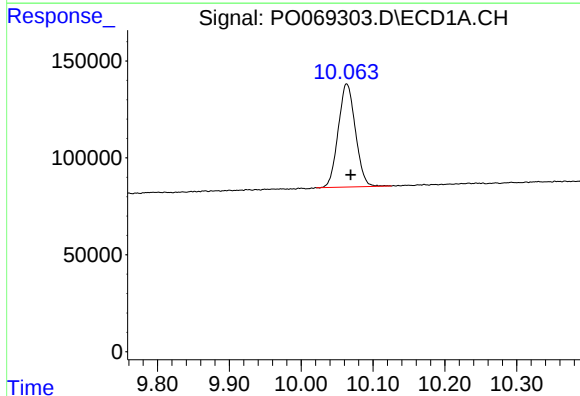


#2 Decachlorobiphenyl

R.T.: 10.063 min
Delta R.T.: -0.006 min
Response: 882063
Conc: 18.57 ng/ml

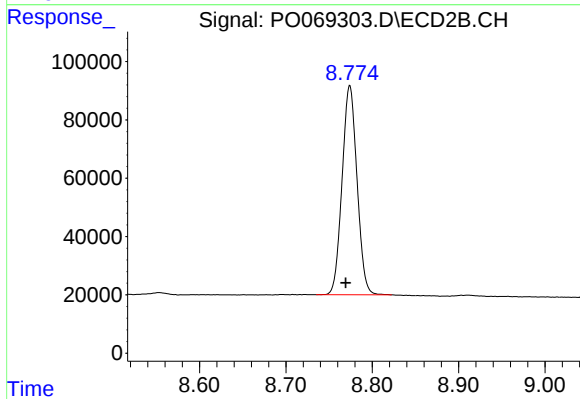

#2 Decachlorobiphenyl


R.T.: 8.774 min
Delta R.T.: 0.005 min
Response: 862200
Conc: 15.84 ng/ml

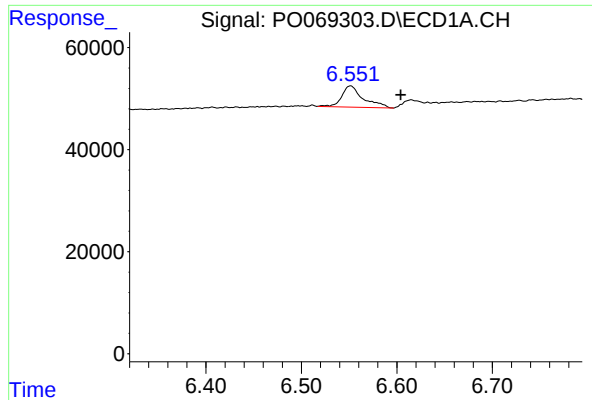

#26 AR-1254-1

R.T.: 6.552 min
Delta R.T.: -0.052 min
Response: 64395
Conc: 43.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

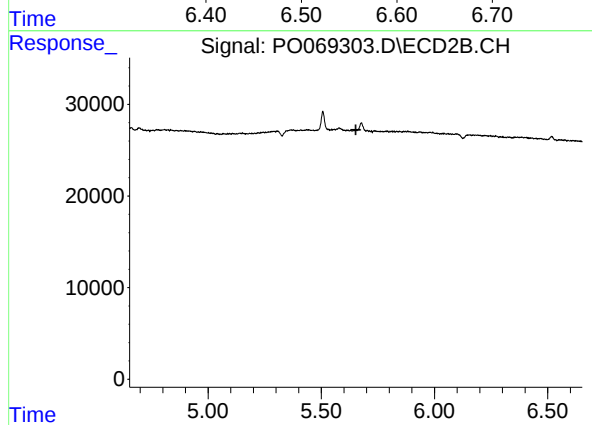

#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.653 min
Response: 0
Conc: N.D.