

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062921\
 Data File : P0079225.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jun 2021 11:37
 Operator : DD\AJ
 Sample : M2847-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1970-WATER

Manual Integrations
 APPROVED

mohammad
 6/30/2021 2:06:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 15:35:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.352f	3.638f	836273	411353	10.596m	13.841m#
2) SA Decachlor...	9.931	8.781	1020131	450890	16.334	15.131

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062921\
Data File : P0079225.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jun 2021 11:37
Operator : DD\AJ
Sample : M2847-03
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1970-WATER


Manual Integrations
APPROVED

mohammad
6/30/2021 2:06:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 15:35:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

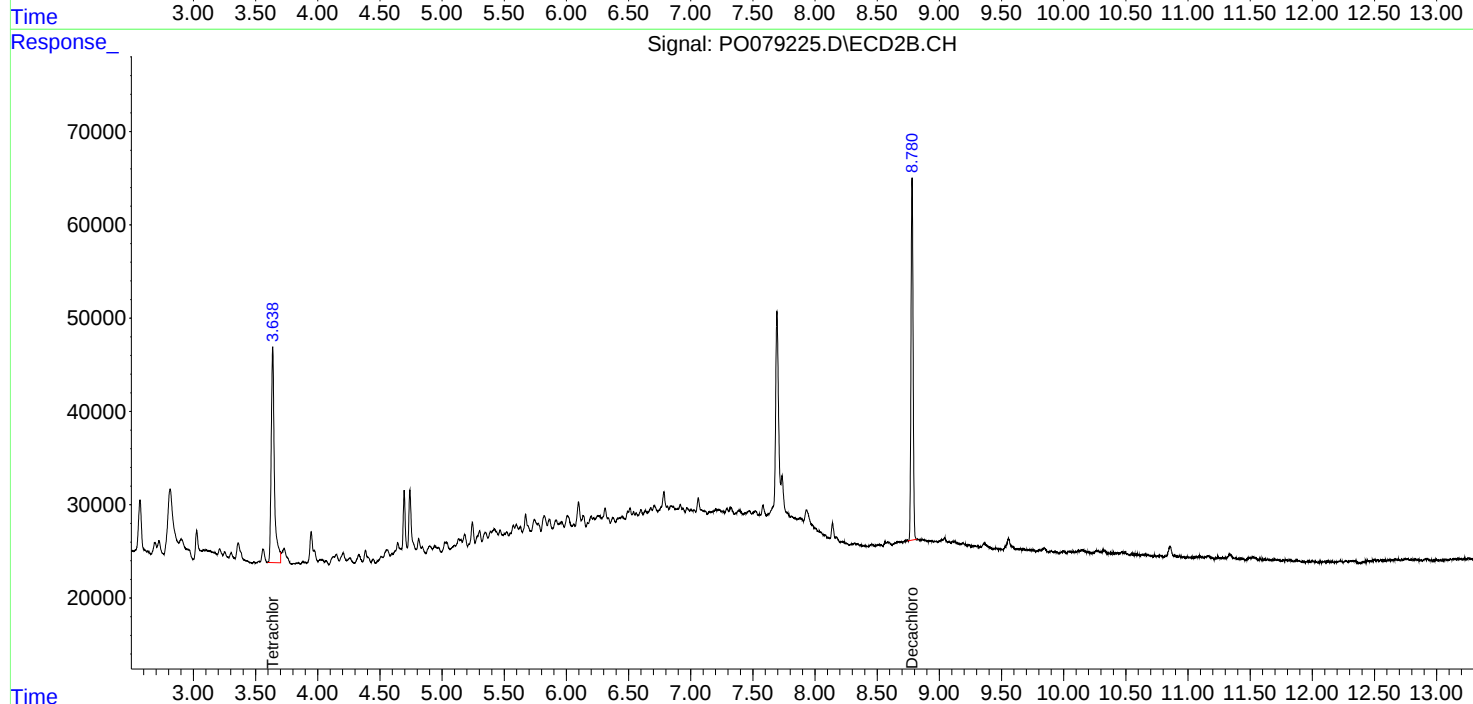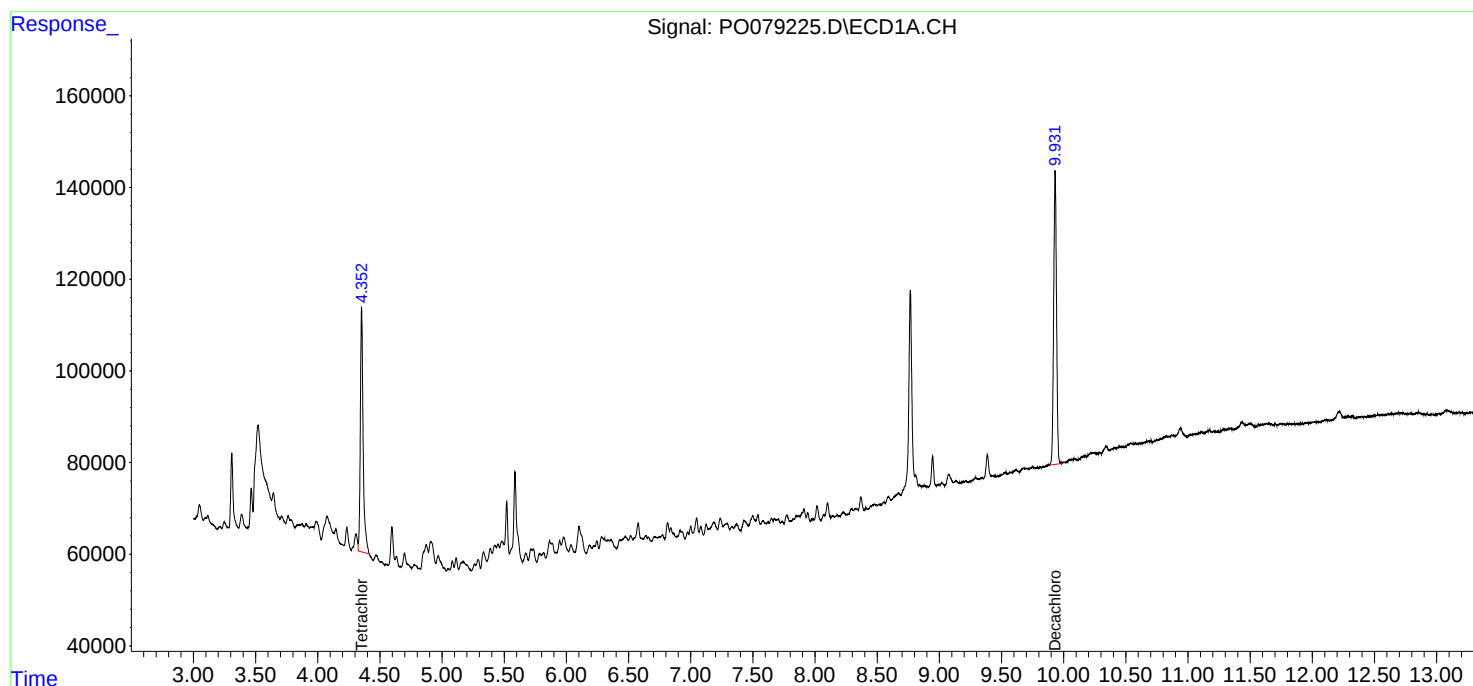

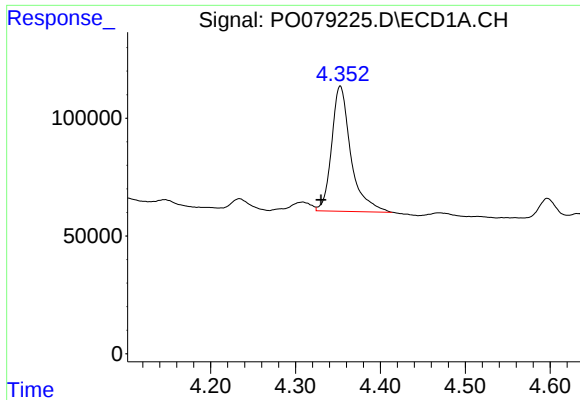


#1 Tetrachloro-m-xylene

R.T.: 4.352 min
Delta R.T.: 0.022 min
Response: 836273
Conc: 10.60 ng/ml m

Instrument :
ECD_O
ClientSampleId :
1970-WATER


Manual Integrations
APPROVED

mohammad
6/30/2021 2:06:41 PM

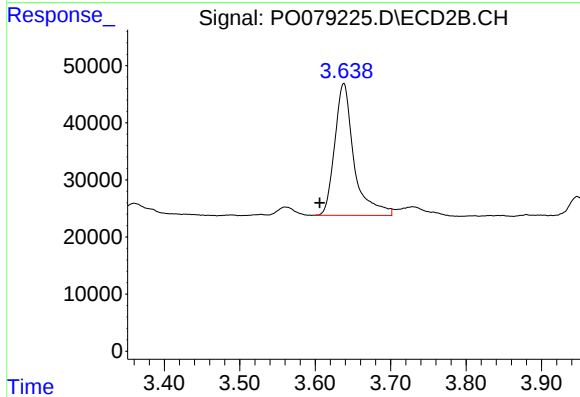


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: 0.031 min
Response: 411353
Conc: 13.84 ng/ml m

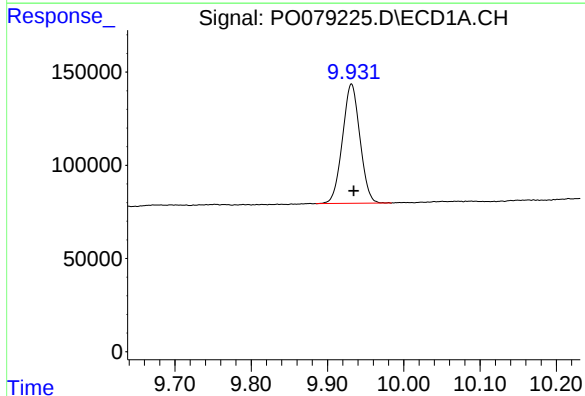

#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.003 min
Response: 1020131
Conc: 16.33 ng/ml

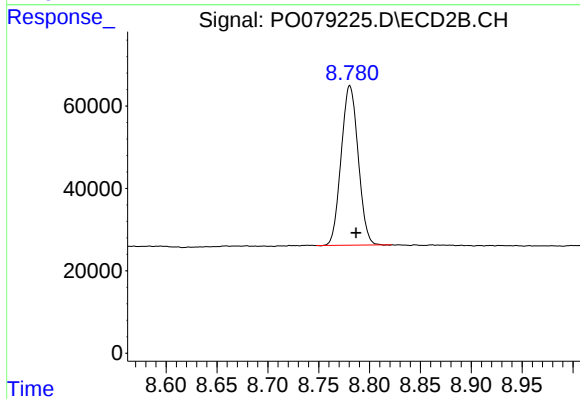

#2 Decachlorobiphenyl

R.T.: 8.781 min
Delta R.T.: -0.006 min
Response: 450890
Conc: 15.13 ng/ml