

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062922\
 Data File : P0087571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2022 17:17
 Operator : YP/AJ
 Sample : N3214-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 03:36:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.449	3.609	47940865	19427180	18.522	19.743
2)	SA Decachlor...	10.300	8.613	44463700	14299827	21.767	17.640
Target Compounds							
26)	L6 AR-1254-1	6.487	5.490	2982800	1557366	29.757	28.173
27)	L6 AR-1254-2	6.707	5.638	4258604	1304686	27.906	26.669
28)	L6 AR-1254-3	7.075	6.041	4551422	2027990	29.882	26.725
29)	L6 AR-1254-4	7.363	6.270	4449054	1085749	40.418	23.916 #
30)	L6 AR-1254-5	7.782	6.687	2891753	1485066	24.092	23.230



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062922\
Data File : PO087571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2022 17:17
Operator : YP/AJ
Sample : N3214-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 03:36:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

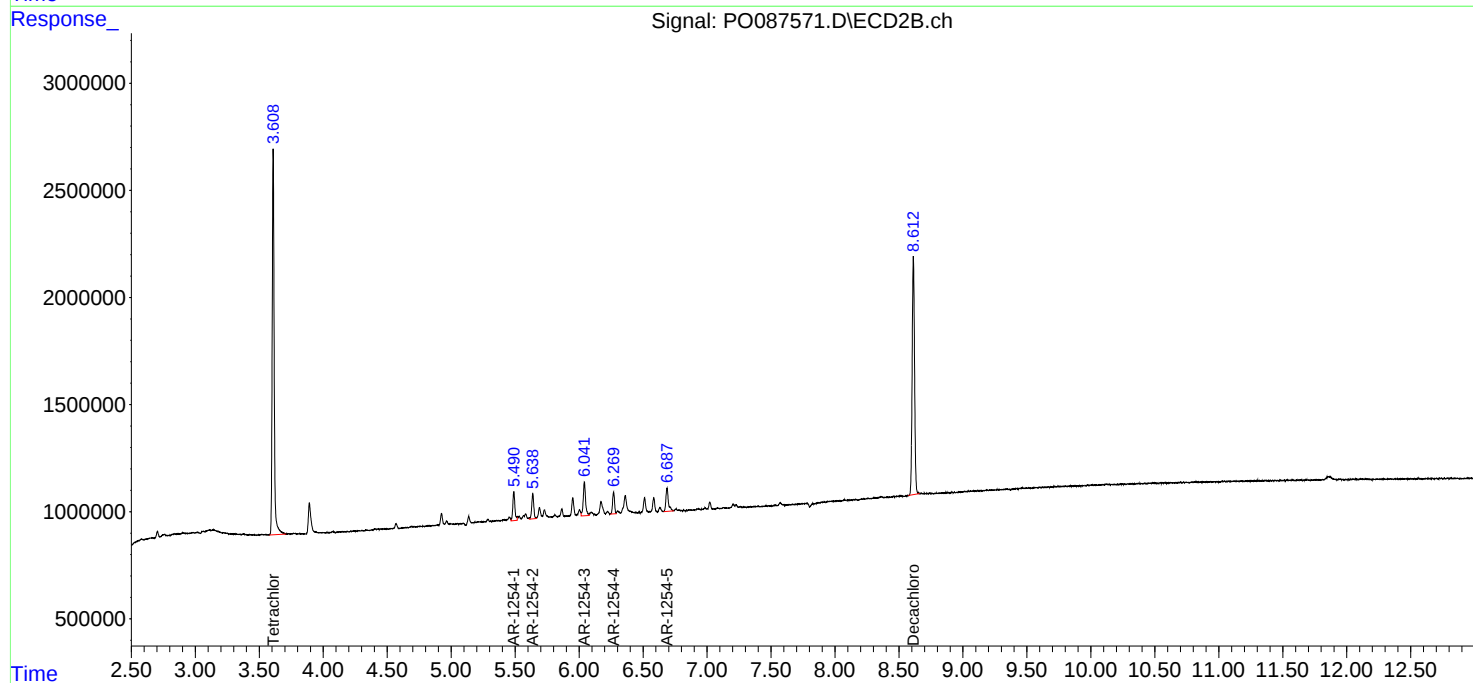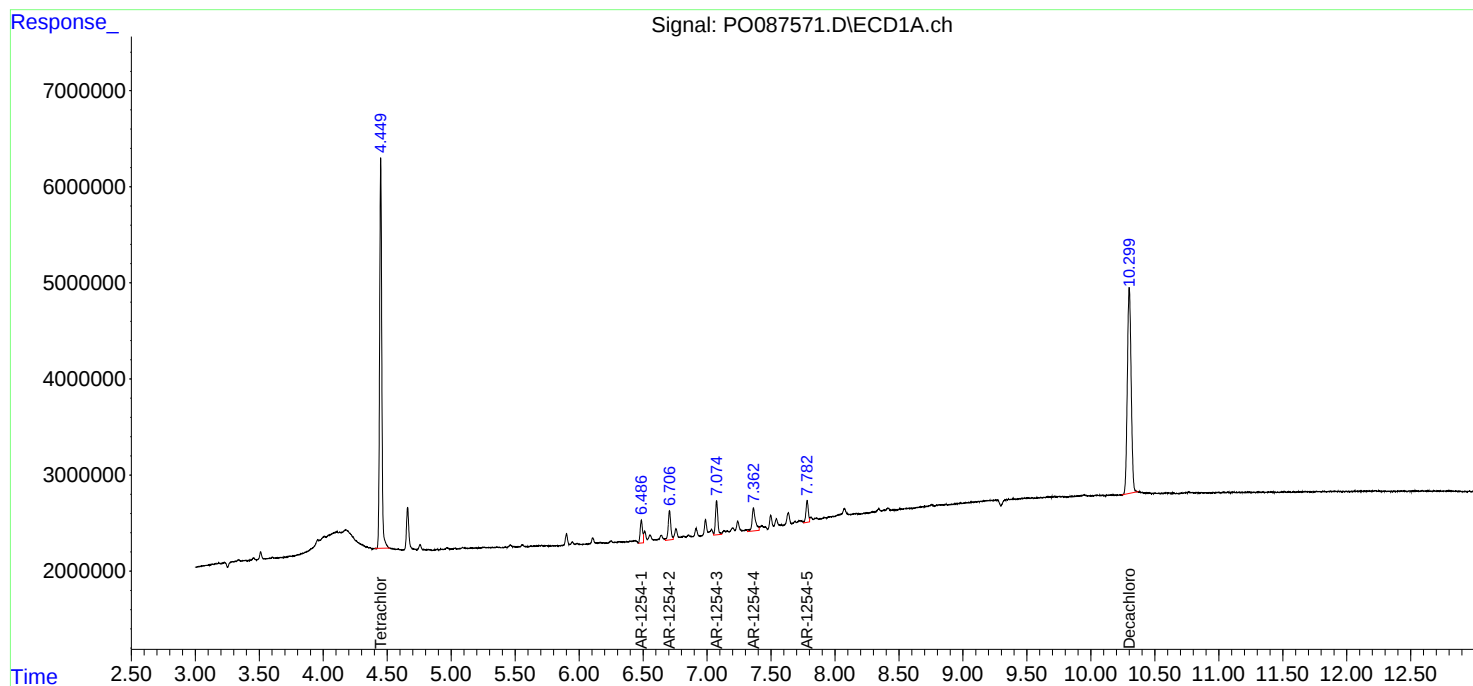


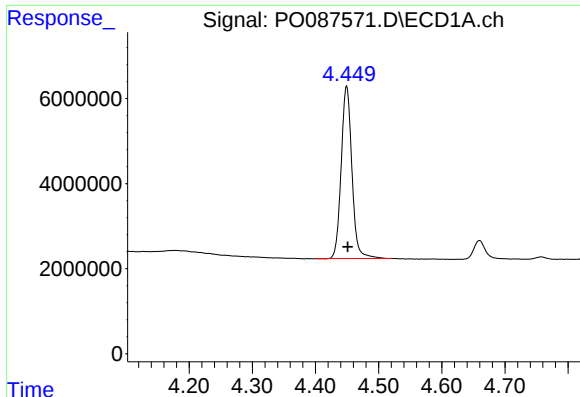

#1 Tetrachloro-m-xylene


R.T.: 4.449 min
Delta R.T.: -0.002 min
Response: 47940865
Conc: 18.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

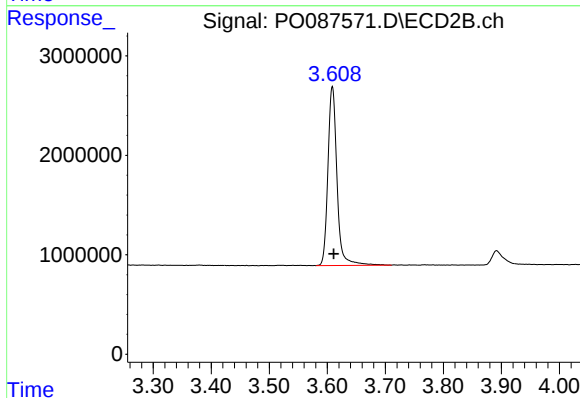


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: -0.002 min
Response: 19427180
Conc: 19.74 ng/ml

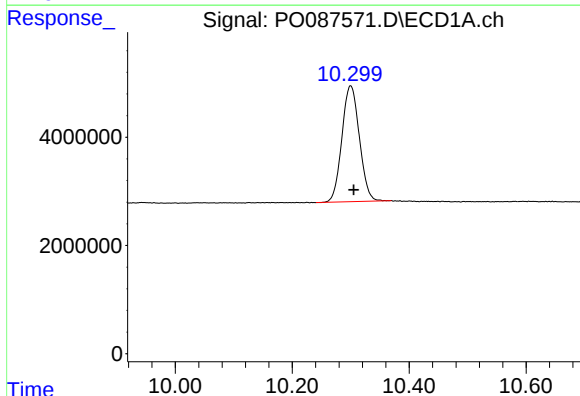


#2 Decachlorobiphenyl

R.T.: 10.300 min
Delta R.T.: -0.006 min
Response: 44463700
Conc: 21.77 ng/ml

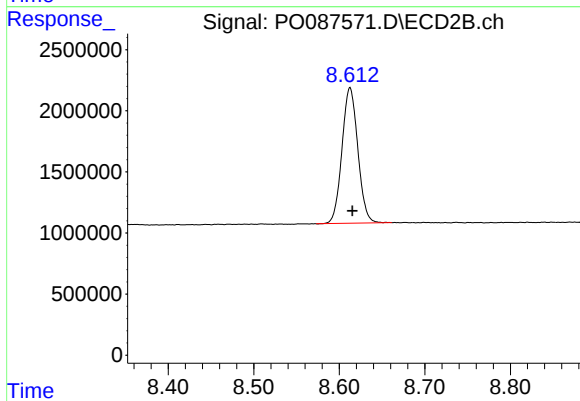

#2 Decachlorobiphenyl


R.T.: 8.613 min
Delta R.T.: -0.003 min
Response: 14299827
Conc: 17.64 ng/ml

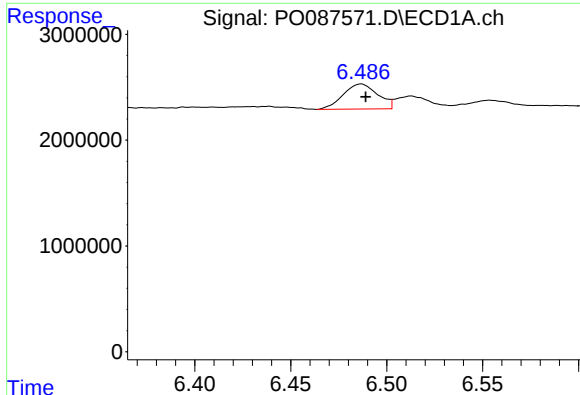

#26 AR-1254-1


R.T.: 6.487 min
Delta R.T.: -0.002 min
Response: 2982800
Conc: 29.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

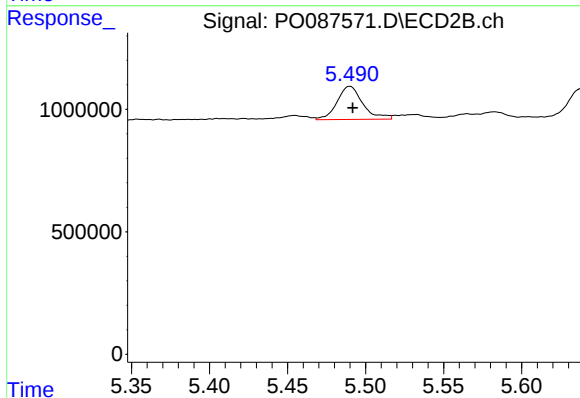


#26 AR-1254-1

R.T.: 5.490 min
Delta R.T.: -0.002 min
Response: 1557366
Conc: 28.17 ng/ml

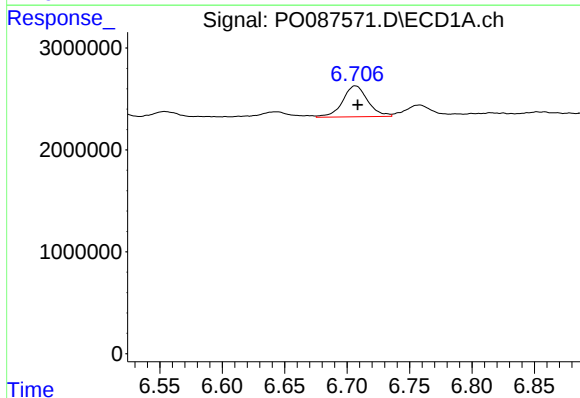


#27 AR-1254-2

R.T.: 6.707 min
Delta R.T.: -0.002 min
Response: 4258604
Conc: 27.91 ng/ml

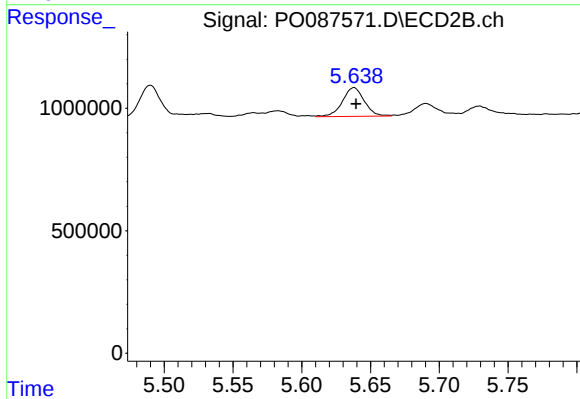

#27 AR-1254-2


R.T.: 5.638 min
Delta R.T.: -0.002 min
Response: 1304686
Conc: 26.67 ng/ml

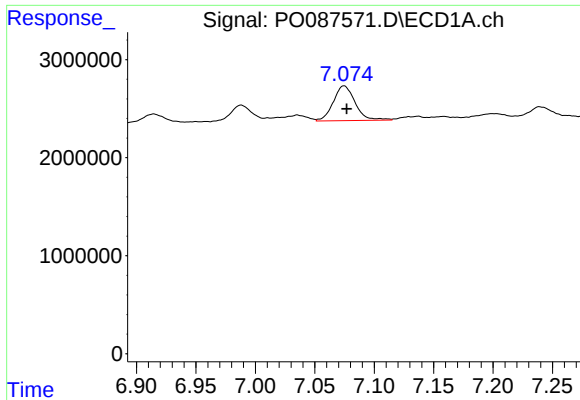

#28 AR-1254-3


R.T.: 7.075 min
Delta R.T.: -0.002 min
Response: 4551422
Conc: 29.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

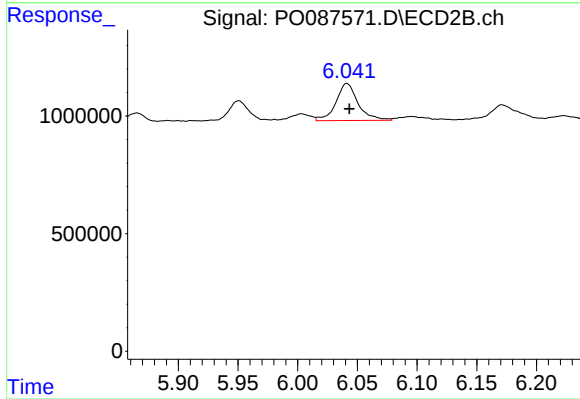


#28 AR-1254-3

R.T.: 6.041 min
Delta R.T.: -0.002 min
Response: 2027990
Conc: 26.73 ng/ml

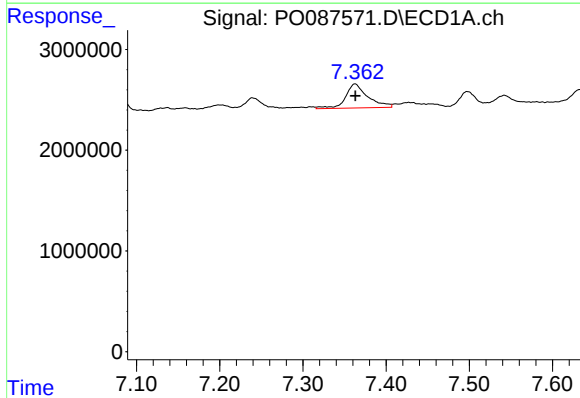


#29 AR-1254-4

R.T.: 7.363 min
Delta R.T.: 0.000 min
Response: 4449054
Conc: 40.42 ng/ml

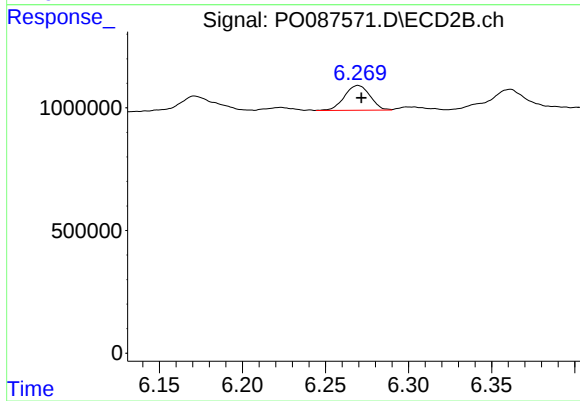

#29 AR-1254-4


R.T.: 6.270 min
Delta R.T.: -0.002 min
Response: 1085749
Conc: 23.92 ng/ml

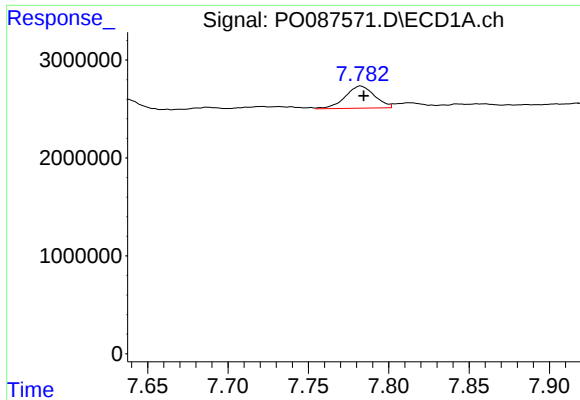

#30 AR-1254-5

R.T.: 7.782 min
Delta R.T.: -0.002 min
Response: 2891753
Conc: 24.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

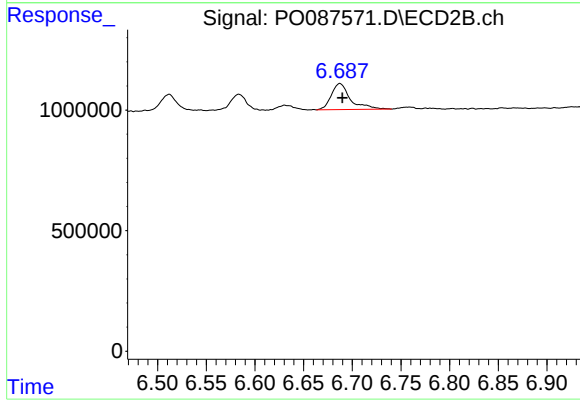

#30 AR-1254-5

R.T.: 6.687 min
Delta R.T.: -0.003 min
Response: 1485066
Conc: 23.23 ng/ml