

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062922\
 Data File : P0087588.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2022 22:00
 Operator : YP/AJ
 Sample : N3214-07
 Misc : AR1232 LOD 40 PPB
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 04:22:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.450	3.609	51744391	20878003	19.991	21.218
2) SA Decachlor...	10.302	8.613	47775123	15311454	23.389	18.888
Target Compounds						
11) L3 AR-1232-1	4.822	3.982	2363363	1008956	36.104	38.867
12) L3 AR-1232-2	5.161	4.708	1191348	862935	36.894	35.389
13) L3 AR-1232-3	5.649	4.883	2076294	431639	34.429	34.756
14) L3 AR-1232-4	5.810	4.967	1013440	434563	34.613	38.327
15) L3 AR-1232-5	5.901	5.137	982618	488165	39.848	38.901



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062922\
Data File : PO087588.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2022 22:00
Operator : YP/AJ
Sample : N3214-07
Misc : AR1232 LOD 40 PPB
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 04:22:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

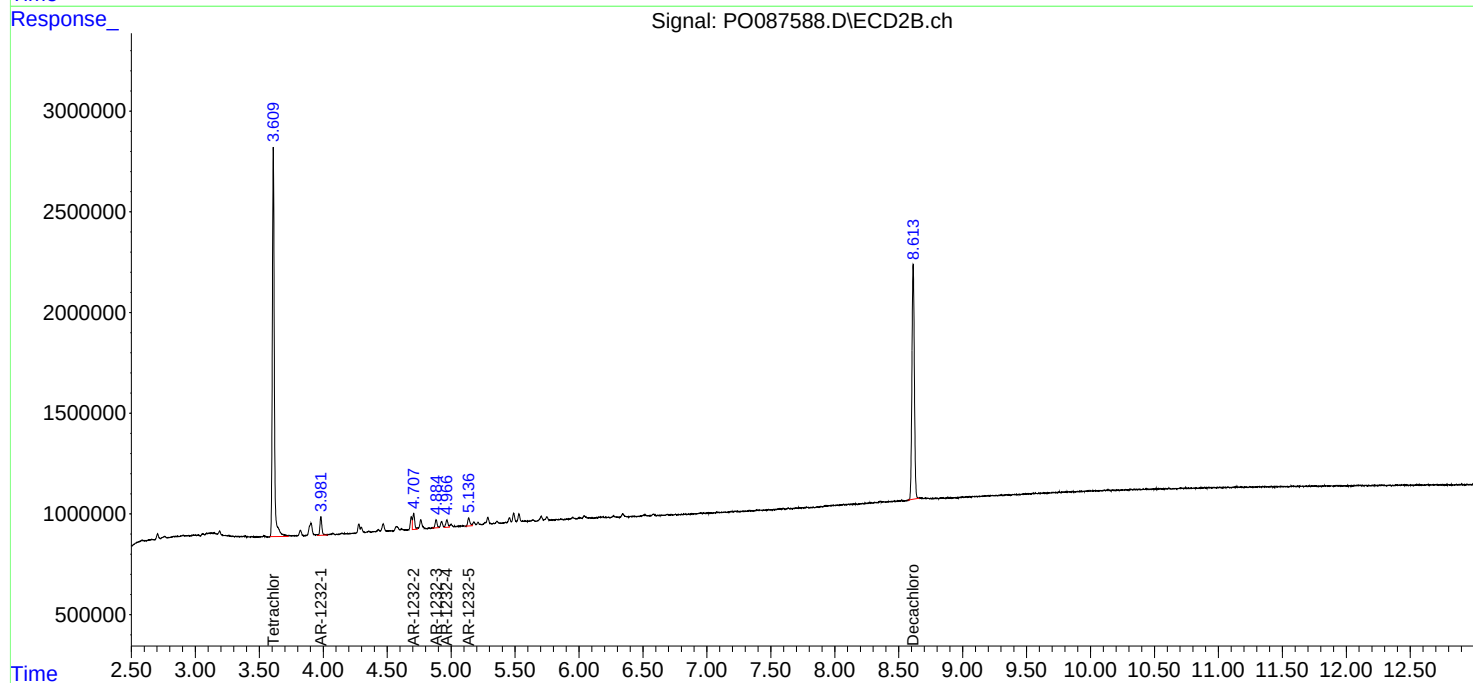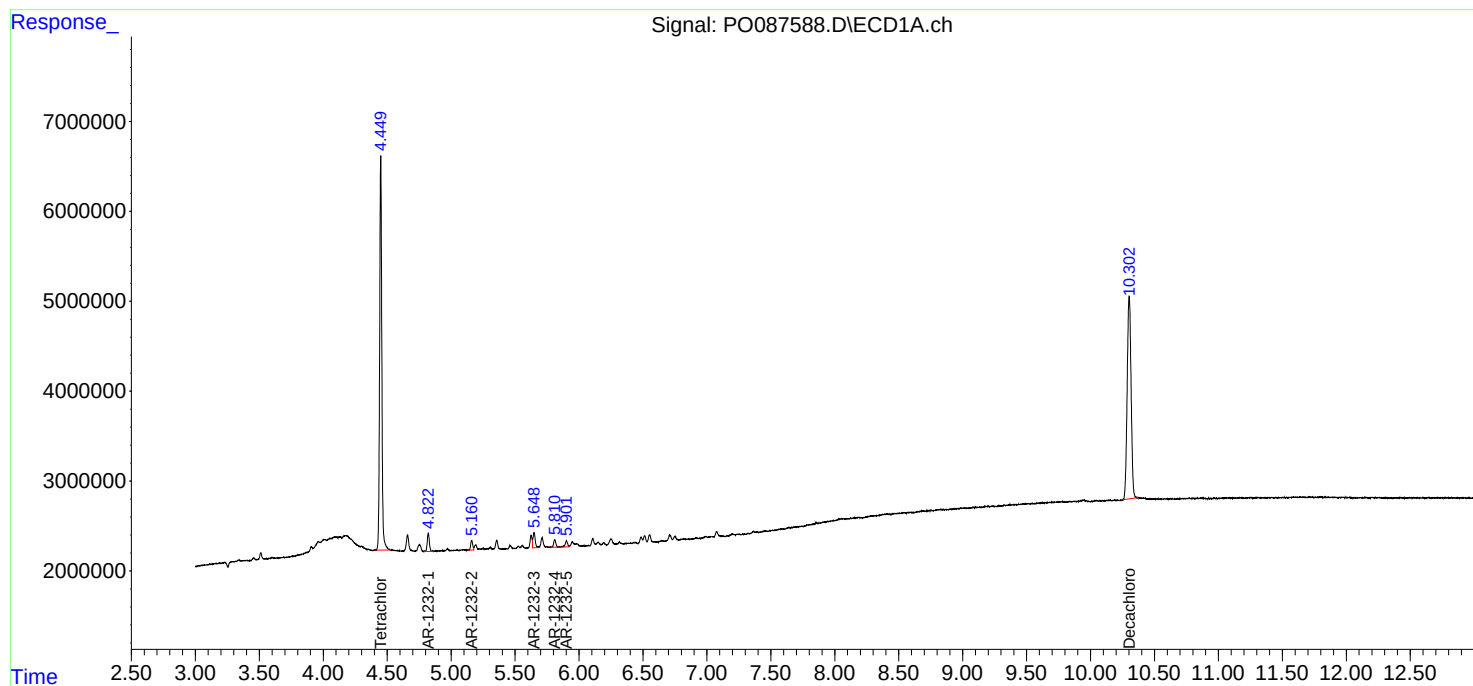


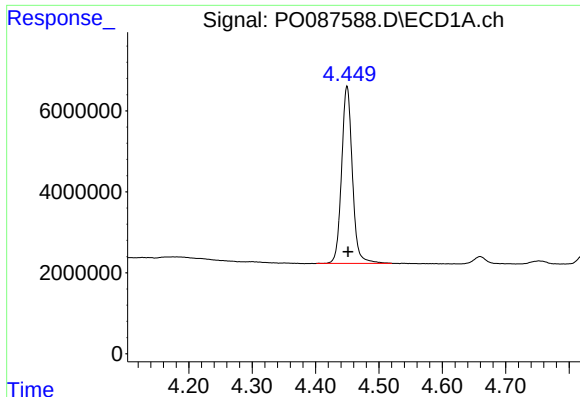

#1 Tetrachloro-m-xylene


R.T.: 4.450 min
Delta R.T.: -0.001 min
Response: 51744391
Conc: 19.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

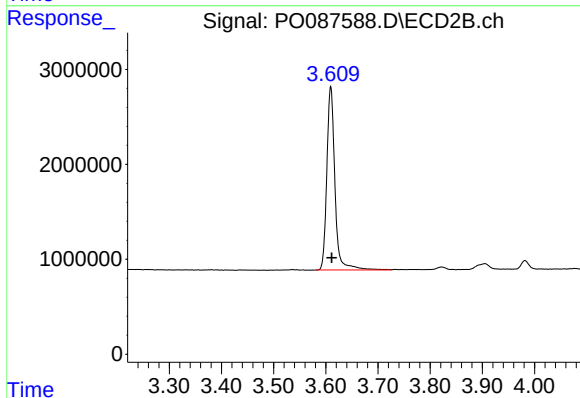


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: -0.002 min
Response: 20878003
Conc: 21.22 ng/ml

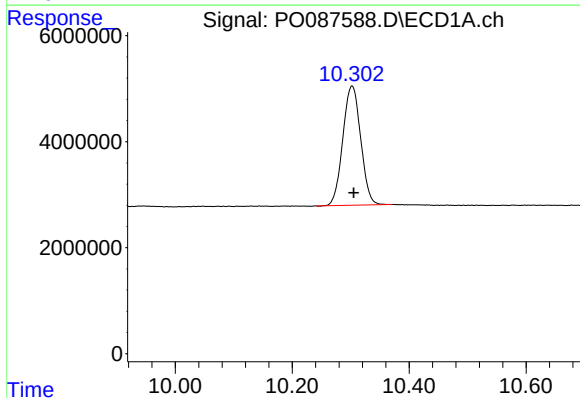


#2 Decachlorobiphenyl

R.T.: 10.302 min
Delta R.T.: -0.003 min
Response: 47775123
Conc: 23.39 ng/ml

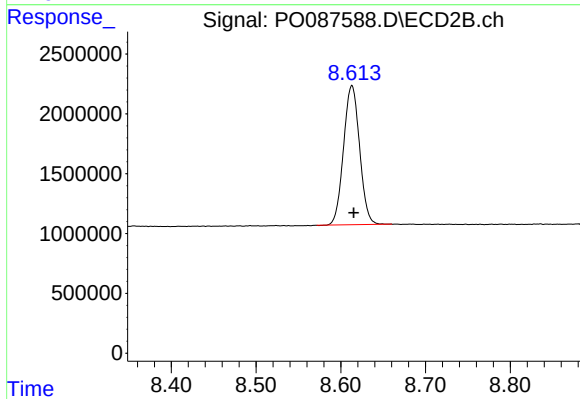

#2 Decachlorobiphenyl


R.T.: 8.613 min
Delta R.T.: -0.002 min
Response: 15311454
Conc: 18.89 ng/ml

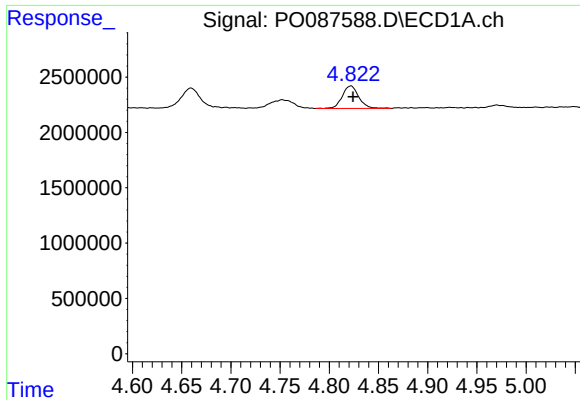

#11 AR-1232-1


R.T.: 4.822 min
Delta R.T.: -0.002 min
Response: 2363363
Conc: 36.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

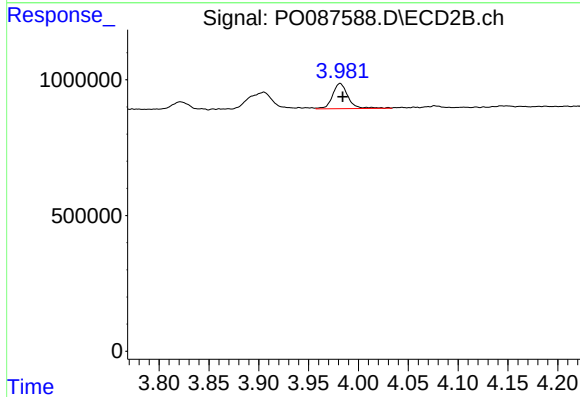


#11 AR-1232-1

R.T.: 3.982 min
Delta R.T.: -0.003 min
Response: 1008956
Conc: 38.87 ng/ml

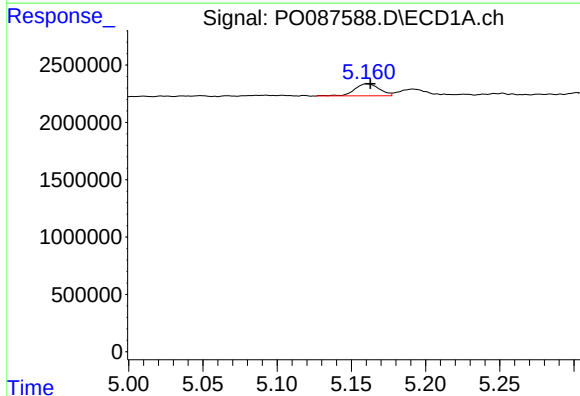


#12 AR-1232-2

R.T.: 5.161 min
Delta R.T.: -0.002 min
Response: 1191348
Conc: 36.89 ng/ml

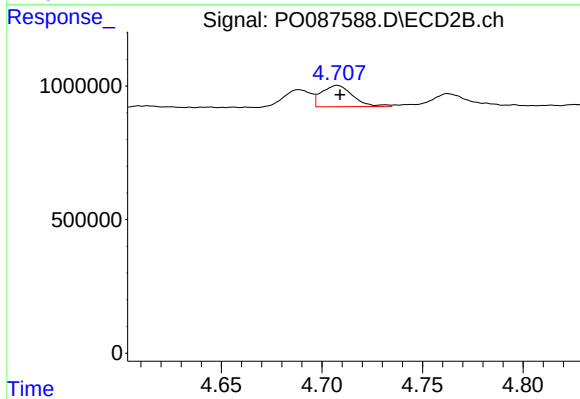

#12 AR-1232-2


R.T.: 4.708 min
Delta R.T.: -0.001 min
Response: 862935
Conc: 35.39 ng/ml

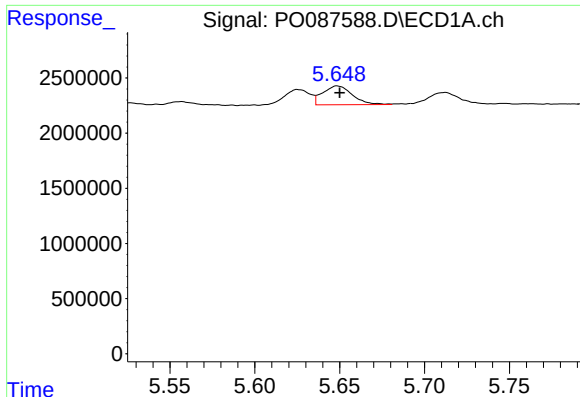

#13 AR-1232-3


R.T.: 5.649 min
Delta R.T.: -0.001 min
Response: 2076294
Conc: 34.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

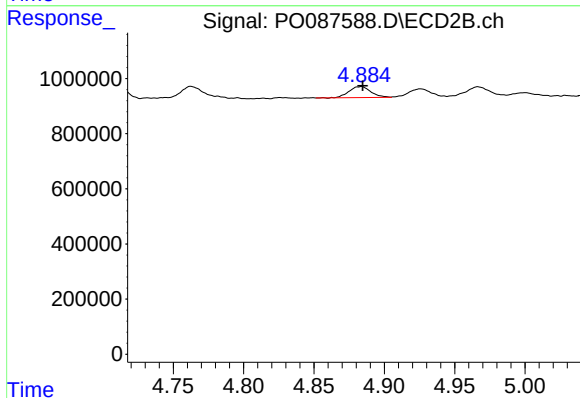


#13 AR-1232-3

R.T.: 4.883 min
Delta R.T.: -0.001 min
Response: 431639
Conc: 34.76 ng/ml

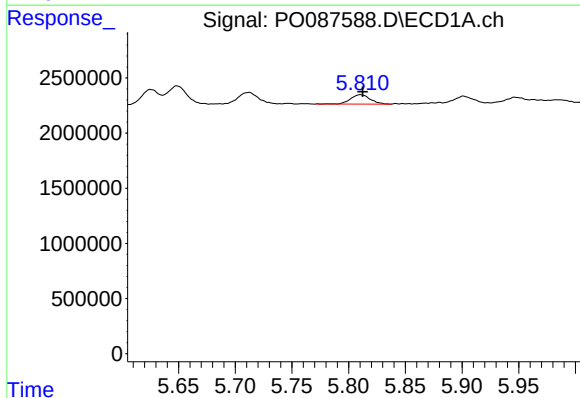


#14 AR-1232-4

R.T.: 5.810 min
Delta R.T.: -0.002 min
Response: 1013440
Conc: 34.61 ng/ml

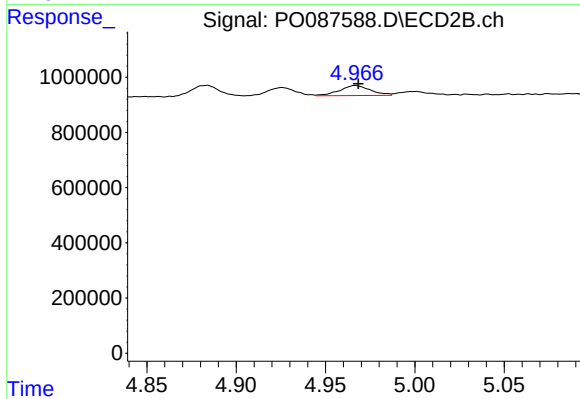

#14 AR-1232-4


R.T.: 4.967 min
Delta R.T.: -0.002 min
Response: 434563
Conc: 38.33 ng/ml

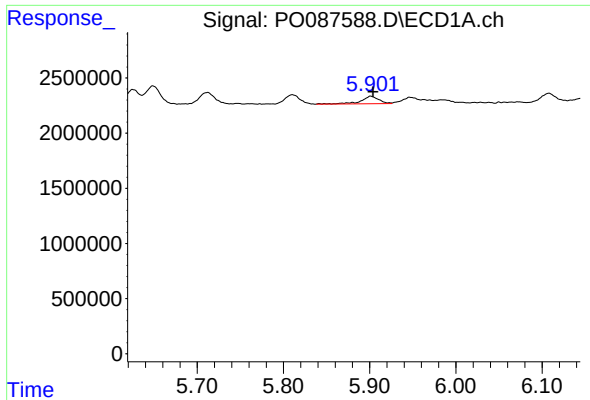

#15 AR-1232-5

R.T.: 5.901 min
Delta R.T.: -0.003 min
Response: 982618
Conc: 39.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2022

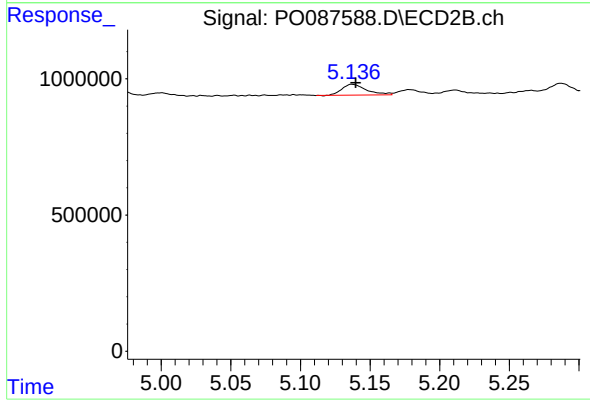

#15 AR-1232-5

R.T.: 5.137 min
Delta R.T.: -0.002 min
Response: 488165
Conc: 38.90 ng/ml