

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062922\
 Data File : P0087617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 06:46
 Operator : YP/AJ
 Sample : N3526-03
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PUMPHOUSE-SIDE-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 07:48:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.607	50539824	22080985	19.526	22.440
2) SA Decachlor...	10.298	8.610	47543125	18358133	23.275	22.646m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0062922\
Data File : P0087617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 06:46
Operator : YP/AJ
Sample : N3526-03
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
PUMPHOUSE-SIDE-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 07:48:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

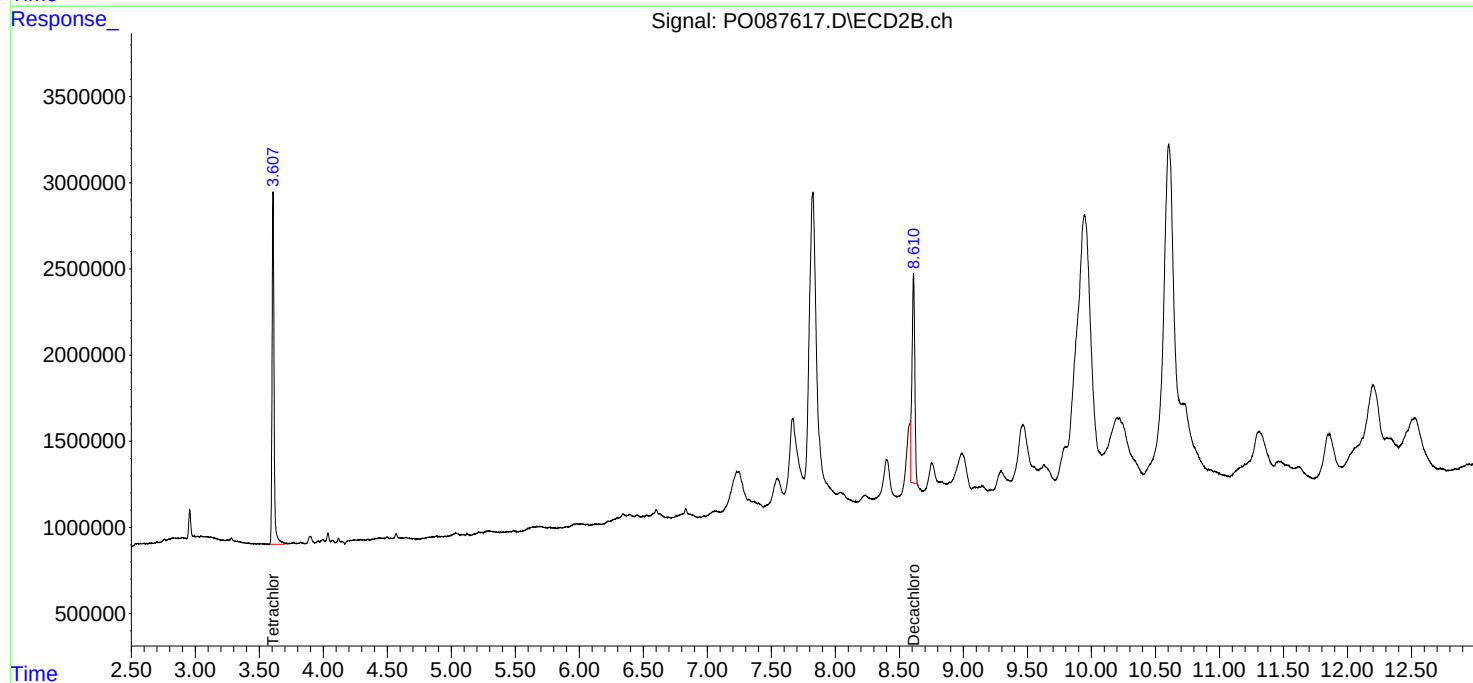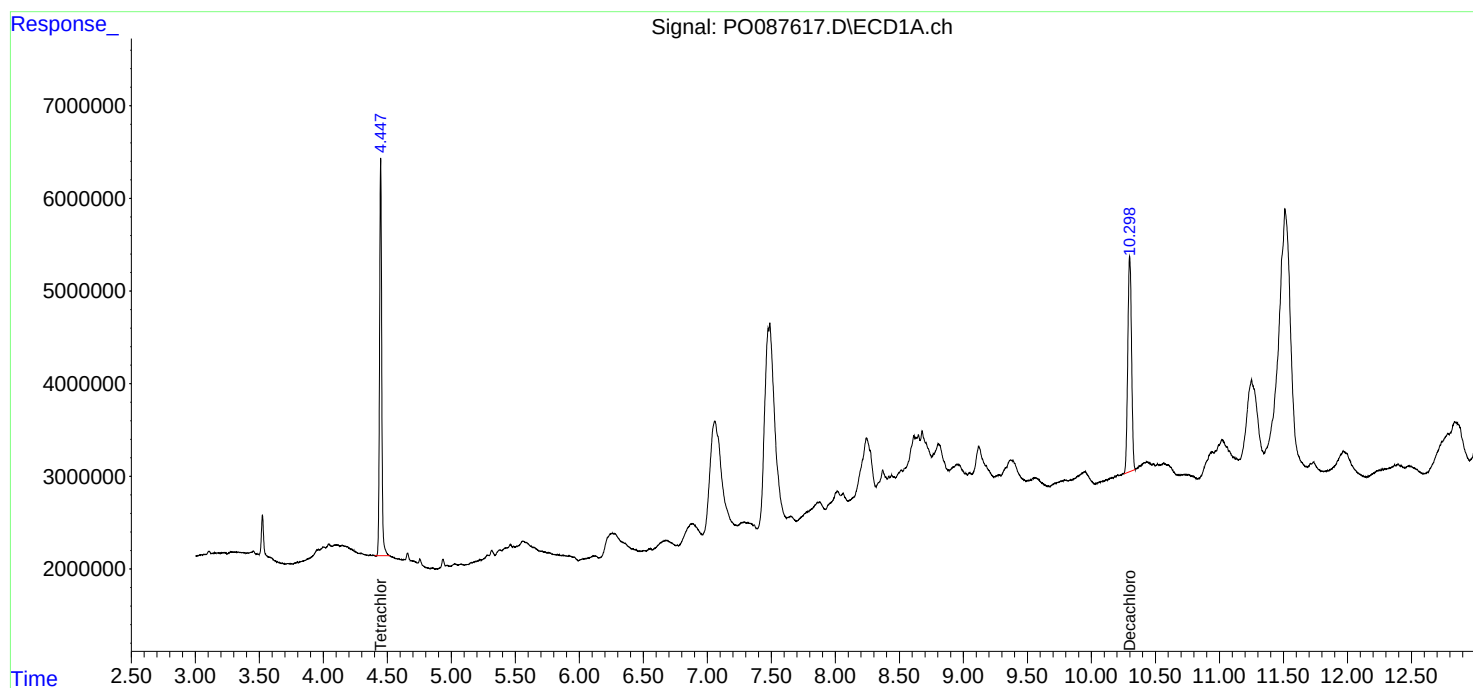


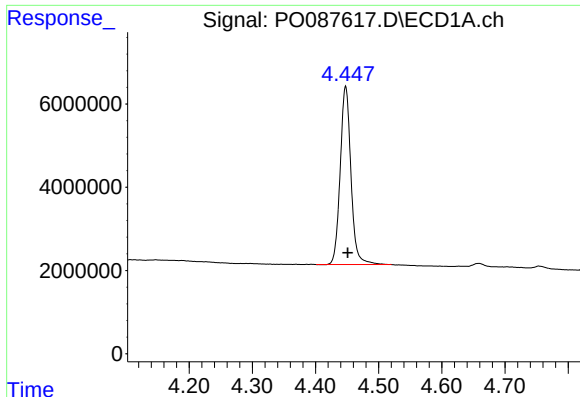

#1 Tetrachloro-m-xylene


R.T.: 4.448 min
Delta R.T.: -0.003 min
Response: 50539824
Conc: 19.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
PUMPHOUSE-SIDE-2

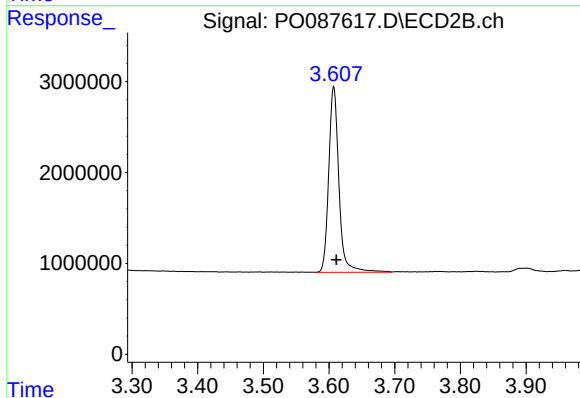


#1 Tetrachloro-m-xylene

R.T.: 3.607 min
Delta R.T.: -0.004 min
Response: 22080985
Conc: 22.44 ng/ml

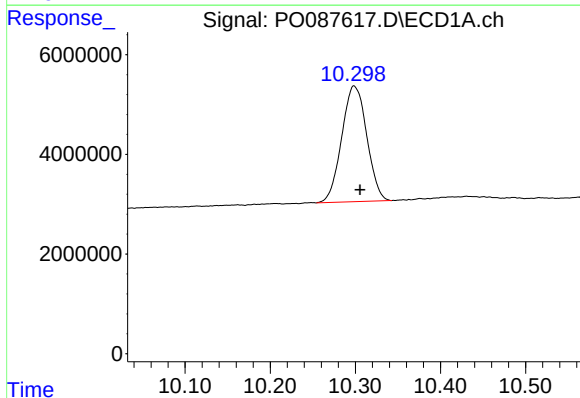

#2 Decachlorobiphenyl

R.T.: 10.298 min
Delta R.T.: -0.007 min
Response: 47543125
Conc: 23.28 ng/ml

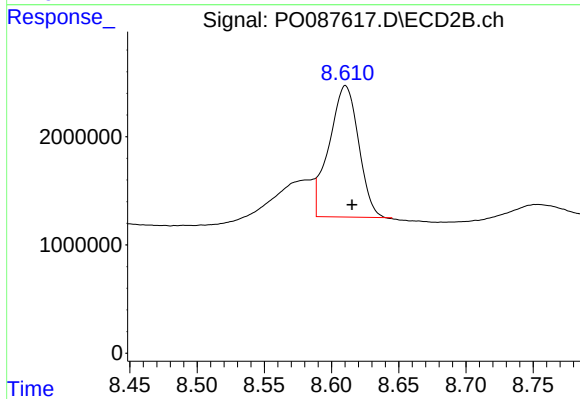

#2 Decachlorobiphenyl

R.T.: 8.610 min
Delta R.T.: -0.005 min
Response: 18358133
Conc: 22.65 ng/ml m