

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062923\
 Data File : P0096073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2023 16:27
 Operator : YP/AJ
 Sample : 03466-02 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC283069-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/30/2023
 Supervised By :Ankita Jodhani 06/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 20:53:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 21 13:08:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.420	3.636	4063610	1996897	1.397	1.471m
2) SA Decachlor...	10.250	8.672	4224085	2403532	2.039	1.960

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062923\
Data File : P0096073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2023 16:27
Operator : YP/AJ
Sample : 03466-02 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC283069-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/30/2023
Supervised By :Ankita Jodhani 06/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 20:53:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 21 13:08:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

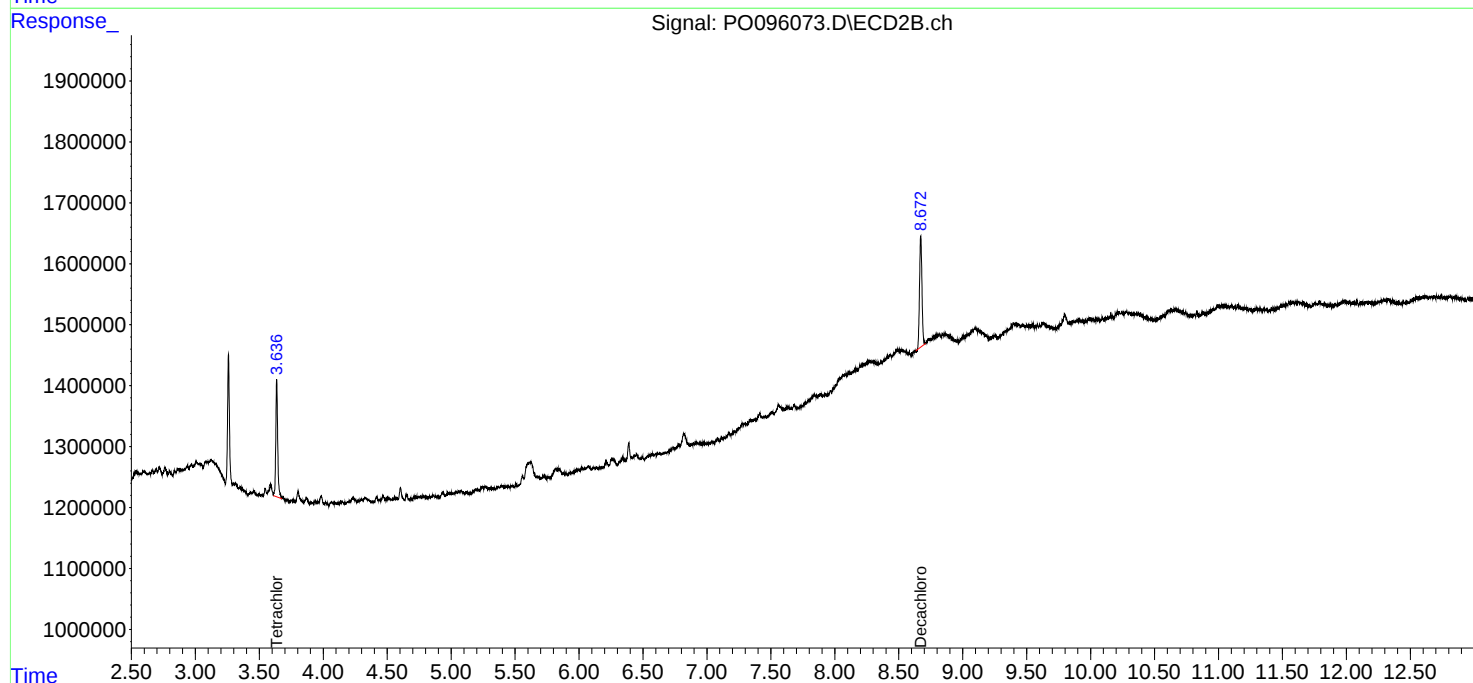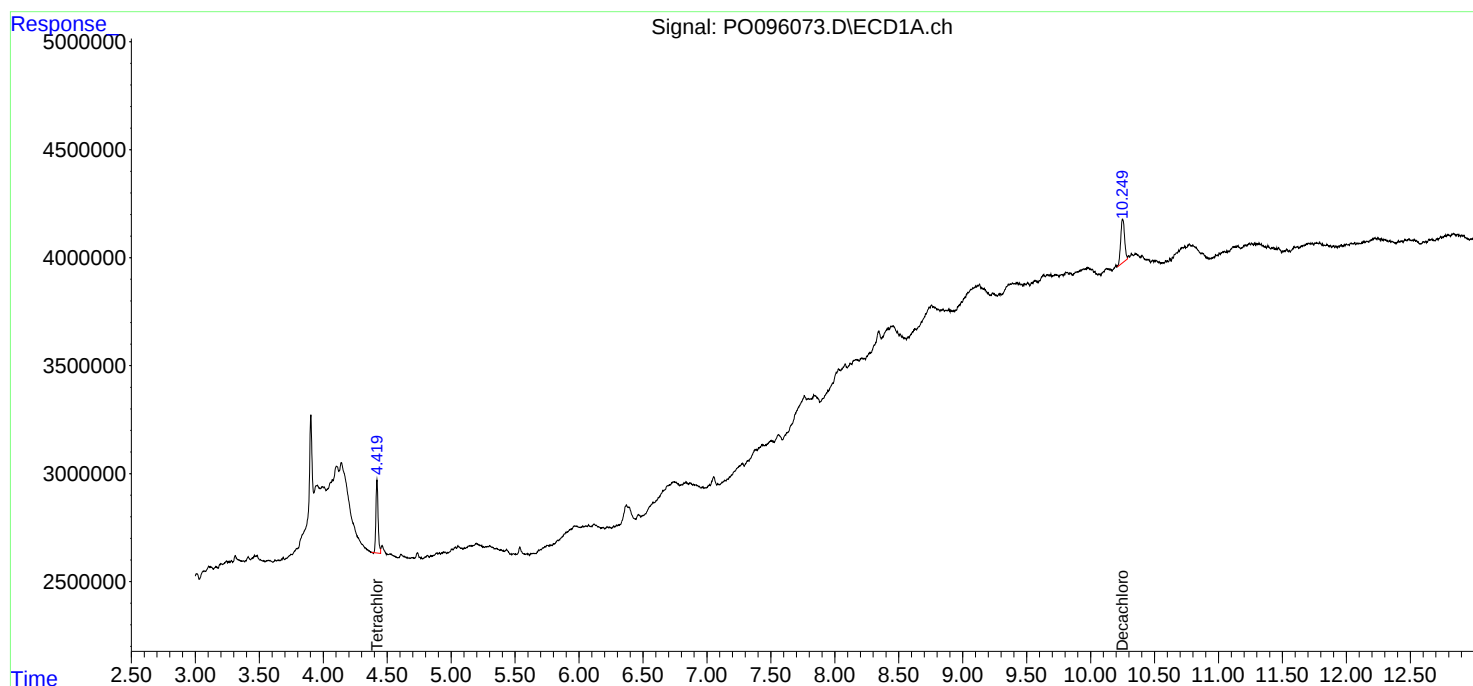

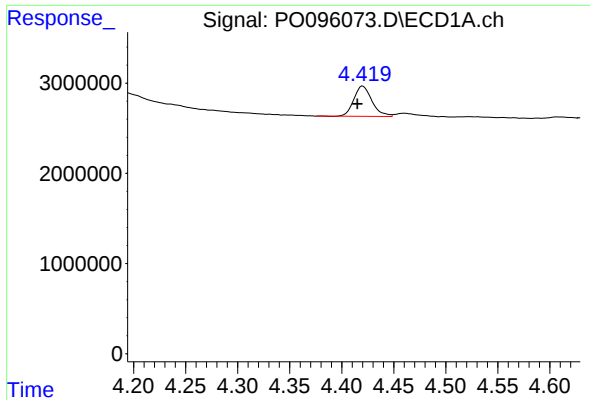


#1 Tetrachloro-m-xylene

R.T.: 4.420 min
Delta R.T.: 0.005 min
Response: 4063610
Conc: 1.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC283069-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/30/2023
Supervised By :Ankita Jodhani 06/30/2023

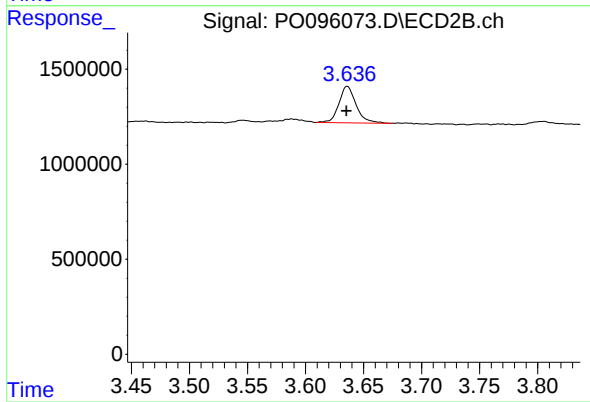


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: 0.000 min
Response: 1996897
Conc: 1.47 ng/ml m

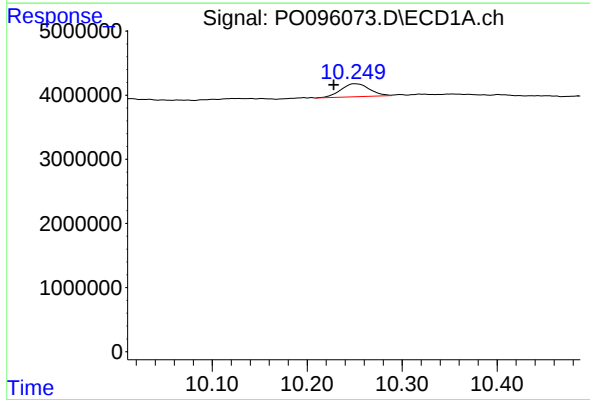

#2 Decachlorobiphenyl

R.T.: 10.250 min
Delta R.T.: 0.022 min
Response: 4224085
Conc: 2.04 ng/ml

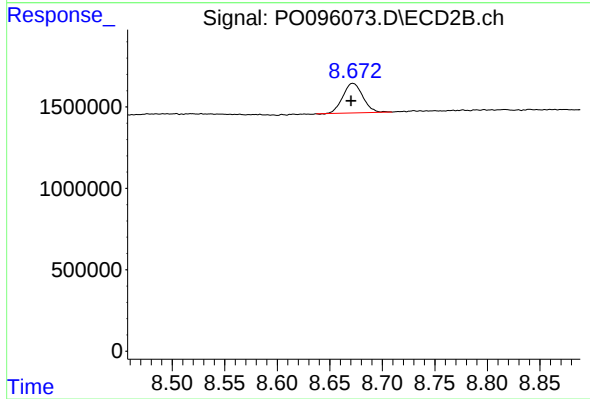

#2 Decachlorobiphenyl

R.T.: 8.672 min
Delta R.T.: 0.002 min
Response: 2403532
Conc: 1.96 ng/ml