

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063020\
 Data File : P0069336.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jun 2020 20:16
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 06:40:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.399	3.566	727170	813843	24.581	21.145
2)	SA Decachlor...	10.062	8.774	990943	1009462	20.864	18.544
Target Compounds							
26)	L6 AR-1254-1	6.549	0.000	89332	0	60.822	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063020\
Data File : P0069336.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jun 2020 20:16
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 06:40:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

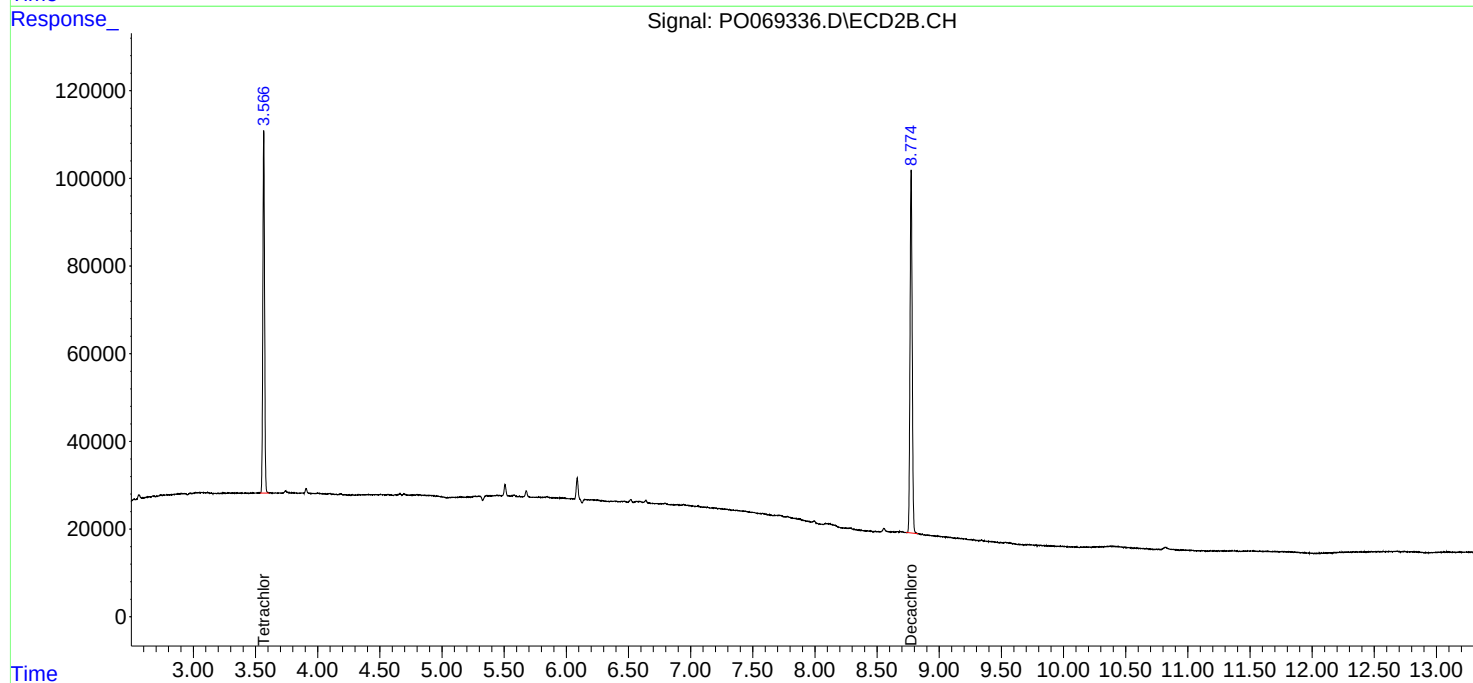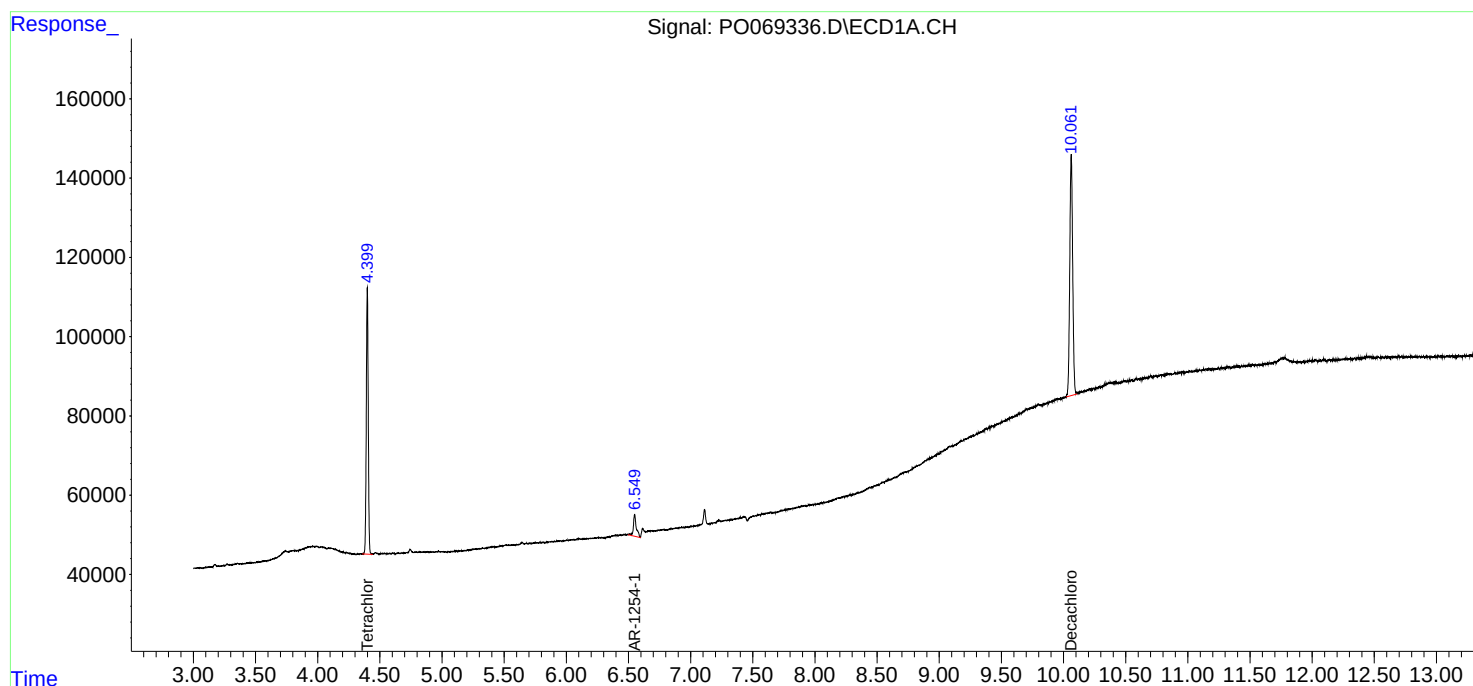


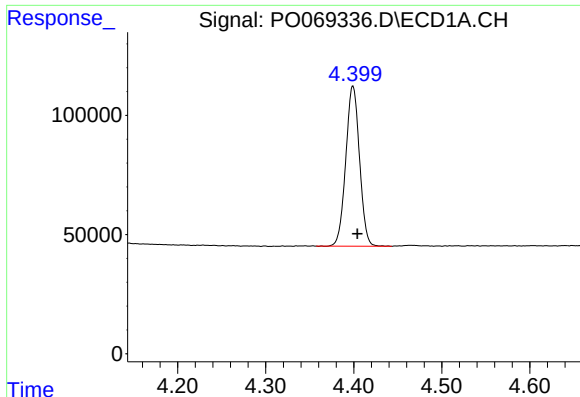

#1 Tetrachloro-m-xylene


R.T.: 4.399 min
Delta R.T.: -0.005 min
Response: 727170
Conc: 24.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

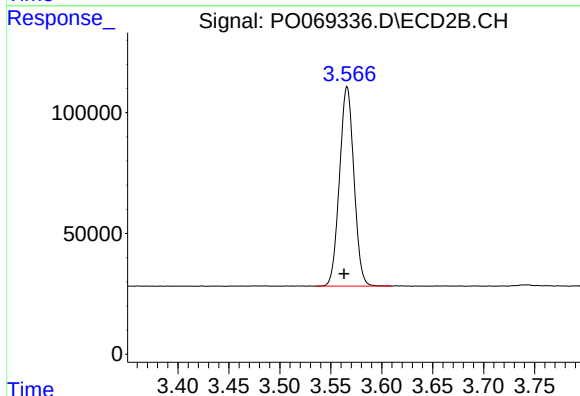


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.003 min
Response: 813843
Conc: 21.14 ng/ml

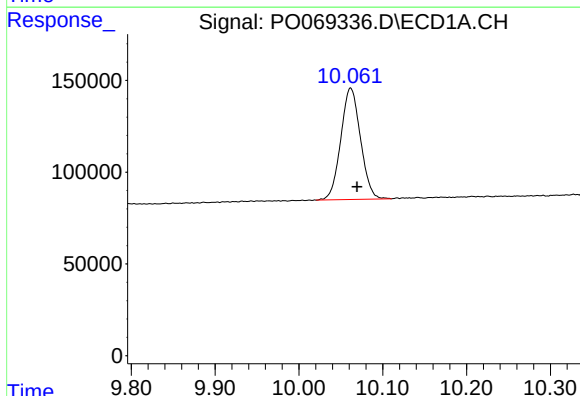


#2 Decachlorobiphenyl

R.T.: 10.062 min
Delta R.T.: -0.008 min
Response: 990943
Conc: 20.86 ng/ml

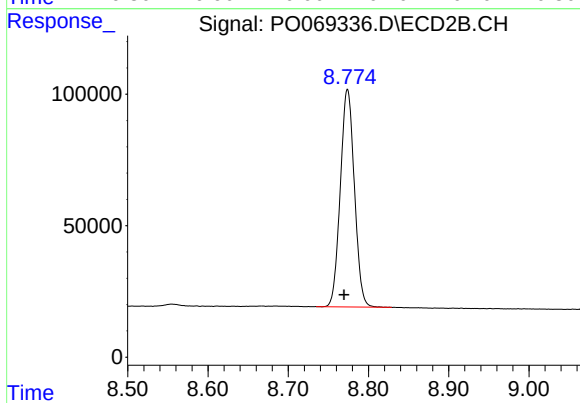

#2 Decachlorobiphenyl


R.T.: 8.774 min
Delta R.T.: 0.005 min
Response: 1009462
Conc: 18.54 ng/ml

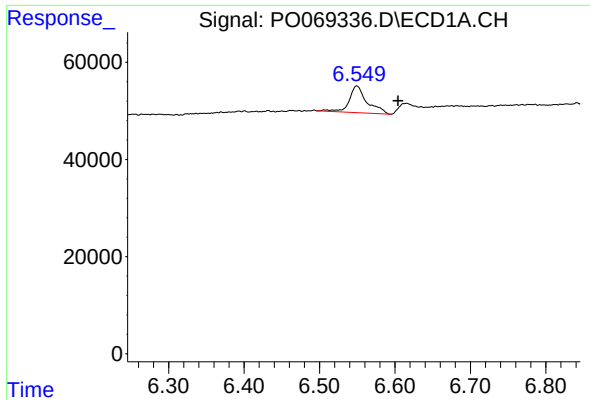

#26 AR-1254-1

R.T.: 6.549 min
Delta R.T.: -0.055 min
Response: 89332
Conc: 60.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

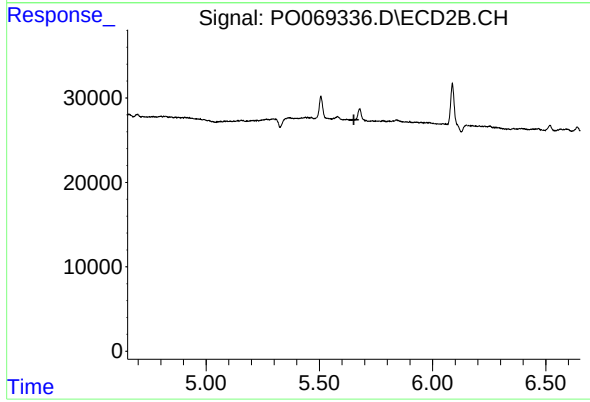

#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.653 min
Response: 0
Conc: N.D.