

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063020\
 Data File : P0069323.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jun 2020 16:32
 Operator : DD\AJ
 Sample : L3153-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP1-C

Manual Integrations
 APPROVED

Ankita
 7/1/2020 12:10:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 06:35:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.400	3.566	890308	1132136	30.095	29.414m
2) SA Decachlor...	10.063	8.774	957953	1005891	20.169	18.479

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063020\
Data File : P0069323.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jun 2020 16:32
Operator : DD\AJ
Sample : L3153-07
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SP1-C


Manual Integrations
APPROVED

Ankita
7/1/2020 12:10:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 06:35:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

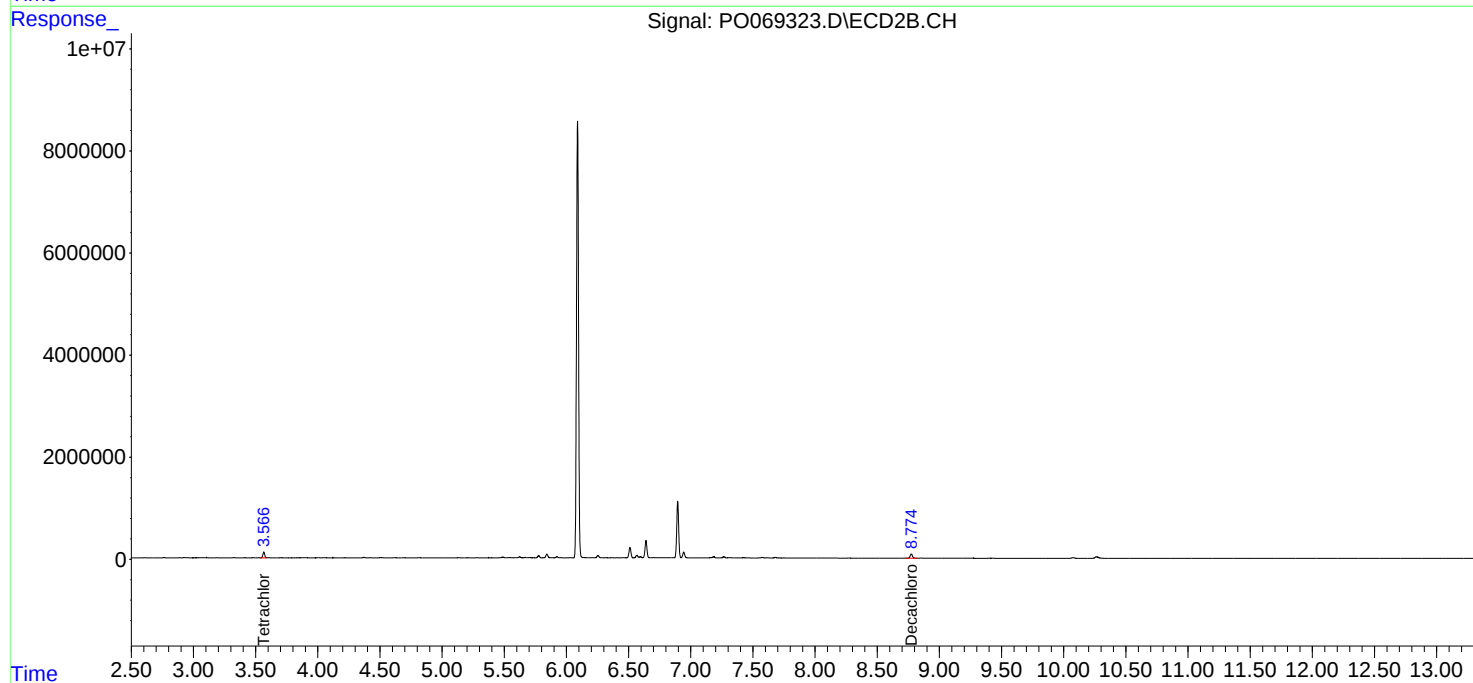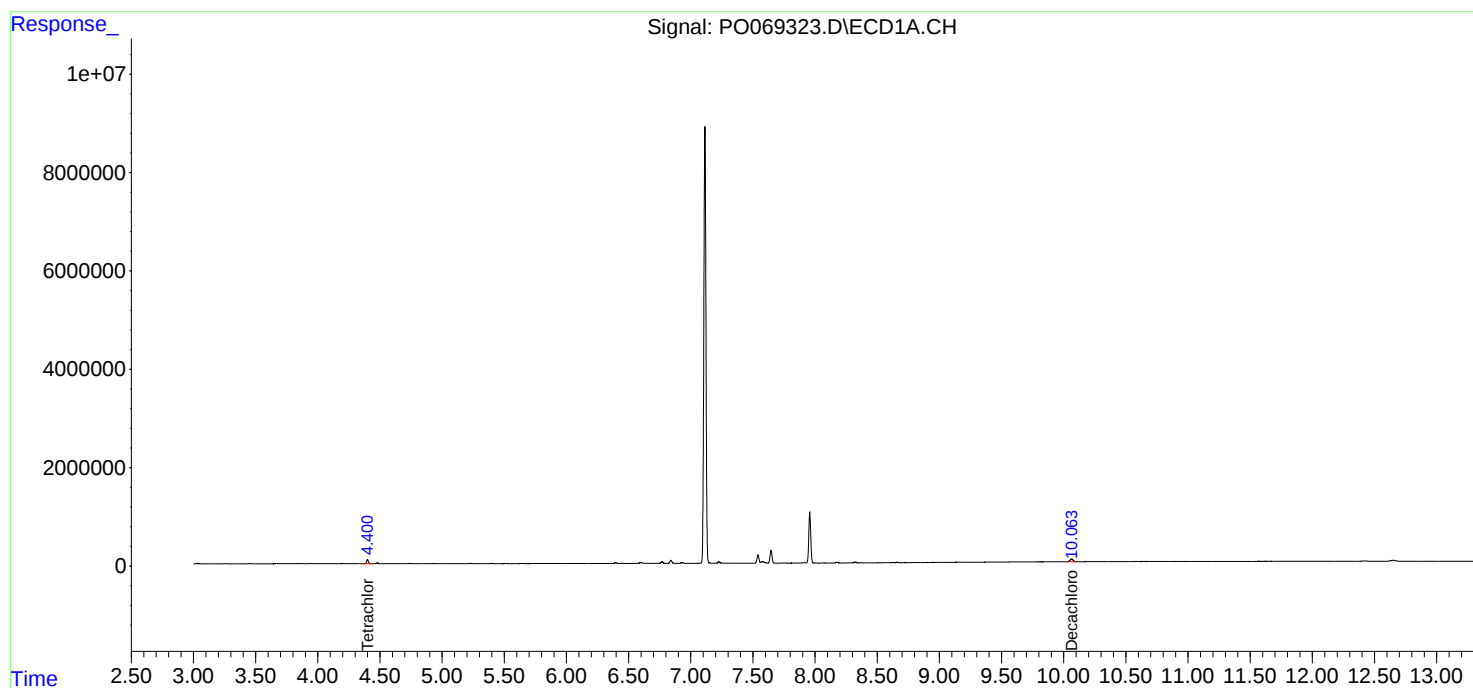

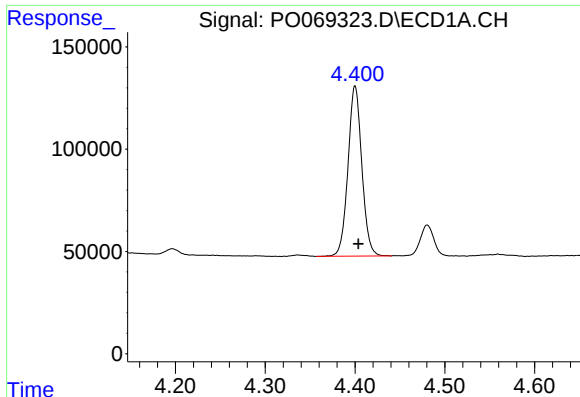


#1 Tetrachloro-m-xylene

R.T.: 4.400 min
Delta R.T.: -0.004 min
Response: 890308
Conc: 30.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP1-C


Manual Integrations
APPROVED

Ankita
7/1/2020 12:10:10 PM

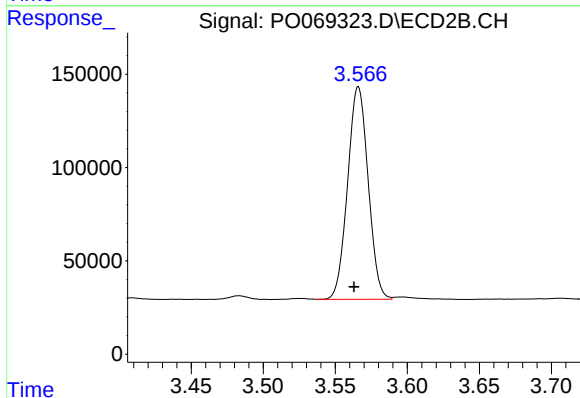


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.003 min
Response: 1132136
Conc: 29.41 ng/ml m

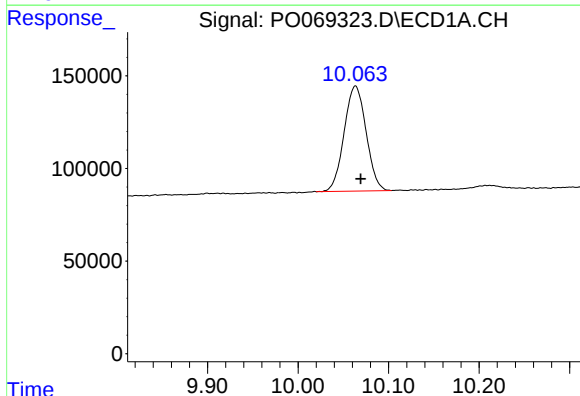

#2 Decachlorobiphenyl

R.T.: 10.063 min
Delta R.T.: -0.006 min
Response: 957953
Conc: 20.17 ng/ml

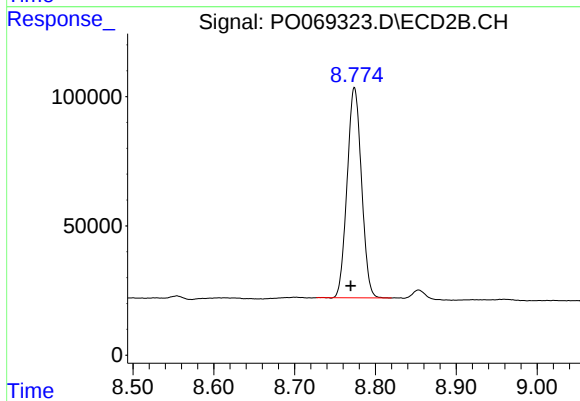

#2 Decachlorobiphenyl

R.T.: 8.774 min
Delta R.T.: 0.005 min
Response: 1005891
Conc: 18.48 ng/ml