

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063020\
 Data File : P0069326.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jun 2020 17:24
 Operator : DD\AJ
 Sample : L3153-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP2-C

Manual Integrations
 APPROVED

Ankita
 7/1/2020 12:10:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 06:36:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.400	3.566	917803	1111305	31.025m	28.873
2) SA Decachlor...	10.063	8.776	965168	980580	20.321	18.014

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063020\
Data File : P0069326.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jun 2020 17:24
Operator : DD\AJ
Sample : L3153-16
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SP2-C


Manual Integrations
APPROVED

Ankita
7/1/2020 12:10:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 06:36:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

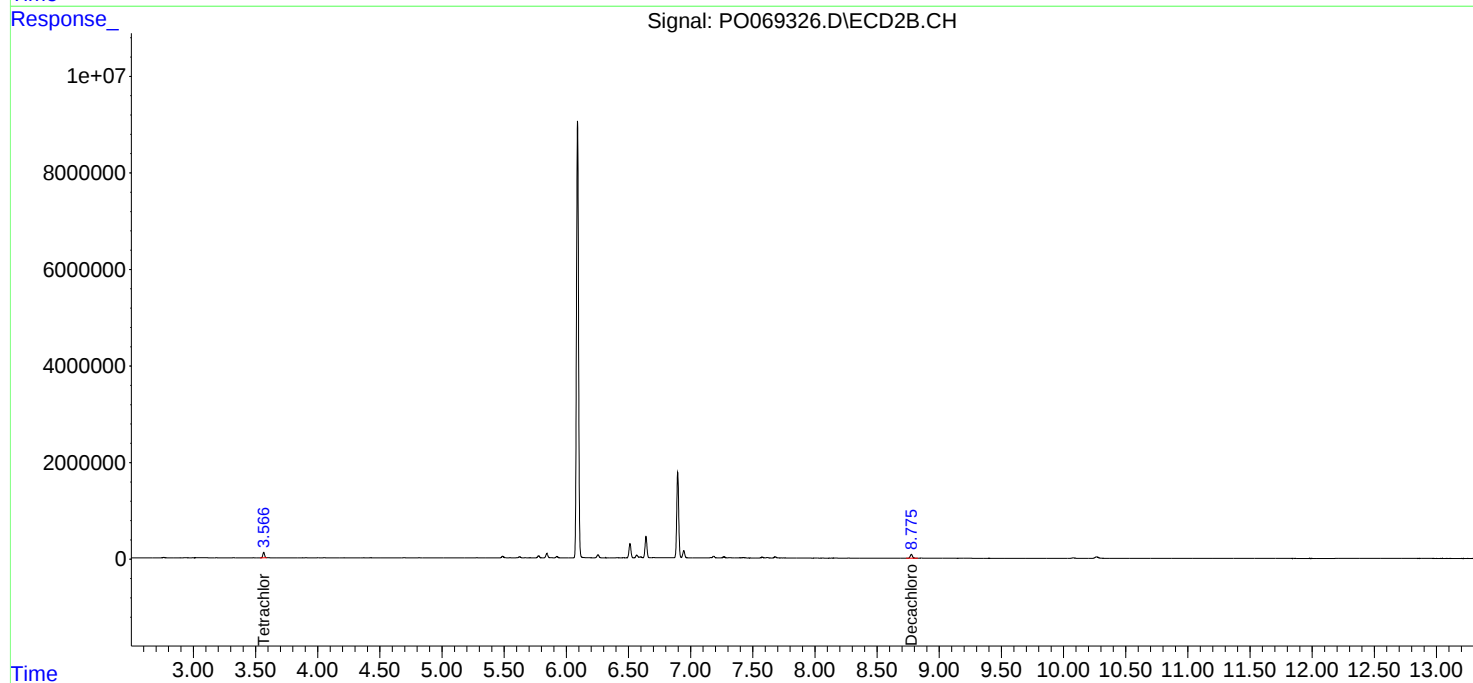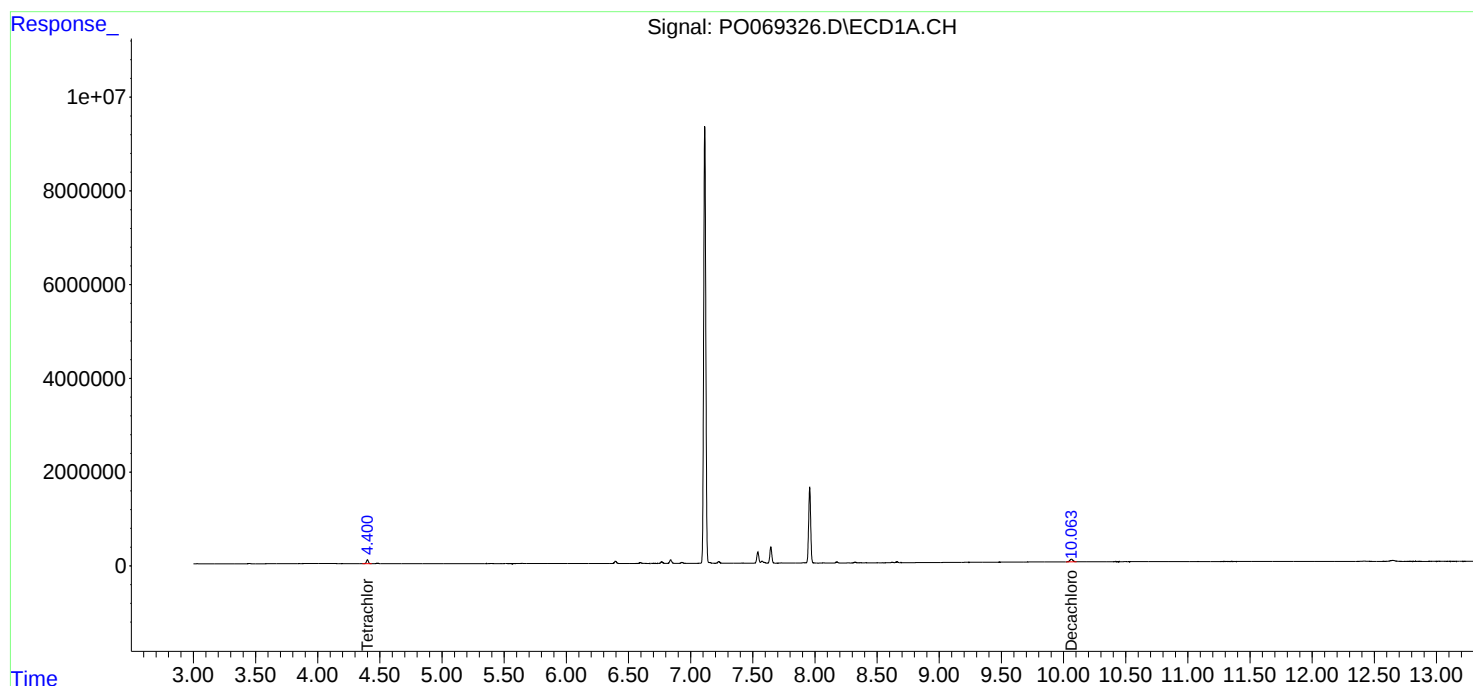

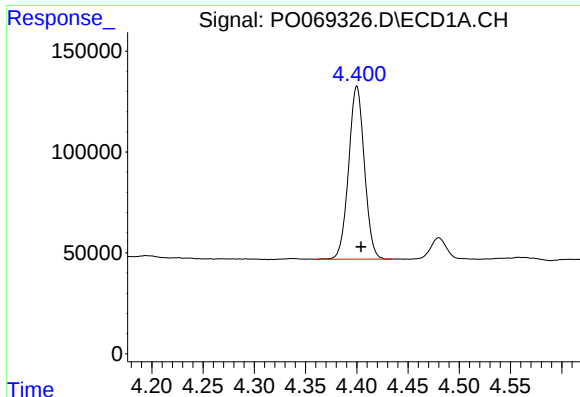

#1 Tetrachloro-m-xylene

R.T.: 4.400 min

Delta R.T.: -0.004 min


Response: 917803

Conc: 31.02 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SP2-C

Manual Integrations
APPROVED

Ankita
7/1/2020 12:10:15 PM

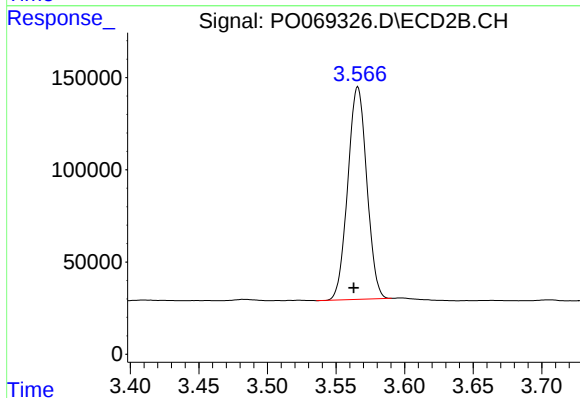


#1 Tetrachloro-m-xylene

R.T.: 3.566 min

Delta R.T.: 0.003 min

Response: 1111305

Conc: 28.87 ng/ml

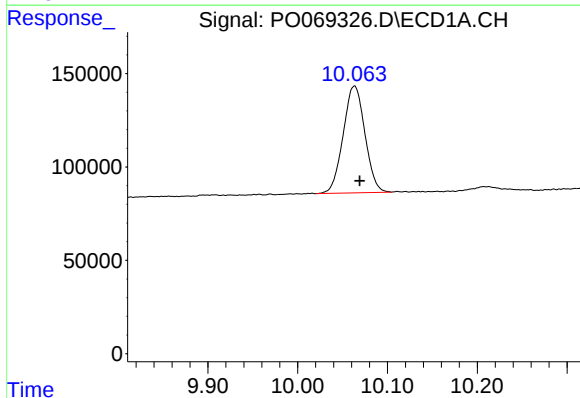


#2 Decachlorobiphenyl

R.T.: 10.063 min

Delta R.T.: -0.006 min

Response: 965168

Conc: 20.32 ng/ml

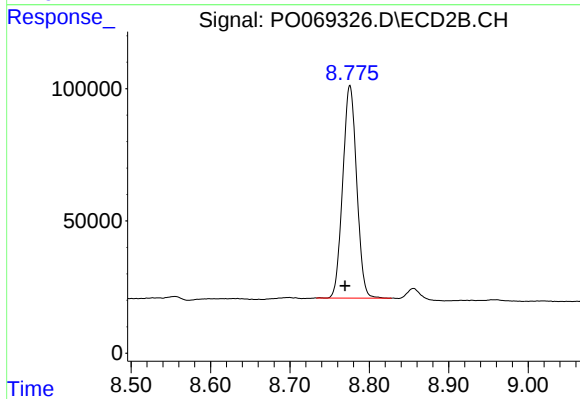

#2 Decachlorobiphenyl

R.T.: 8.776 min

Delta R.T.: 0.006 min

Response: 980580

Conc: 18.01 ng/ml