

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0063022\
 Data File : P0087660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 19:01
 Operator : YP/AJ
 Sample : N3214-09
 Misc : AR1260 MDL 25 PPB
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 03:04:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.450	3.608	49092221	18952296	18.967	19.261
2) SA Decachlor...	10.300	8.613	46364260	15051252	22.698	18.567
Target Compounds						
3) L1 AR-1016-1	5.625	4.688	2347853	860973	26.159	21.529
4) L1 AR-1016-2	5.648	4.706	2938721	1153572	23.383	20.692
5) L1 AR-1016-3	5.711	4.882	1868650	663152	24.009	22.525
6) L1 AR-1016-4	5.810	4.924	1302864	545947	21.315	22.718
7) L1 AR-1016-5	6.107	5.137	1392639	729644	23.237	23.854
31) L7 AR-1260-1	7.240	6.170	2846232	1213469	25.389	21.494
32) L7 AR-1260-2	7.498	6.359	3418056	1582081	25.082	23.384
33) L7 AR-1260-3	7.860	6.511	2529588	1317615	27.006	20.859
34) L7 AR-1260-4	8.086	6.984	2671290	960665	25.536	20.657
35) L7 AR-1260-5	8.415	7.226	5471250	2392955	27.736	22.199



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063022\
Data File : P0087660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 19:01
Operator : YP/AJ
Sample : N3214-09
Misc : AR1260 MDL 25 PPB
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 03:04:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

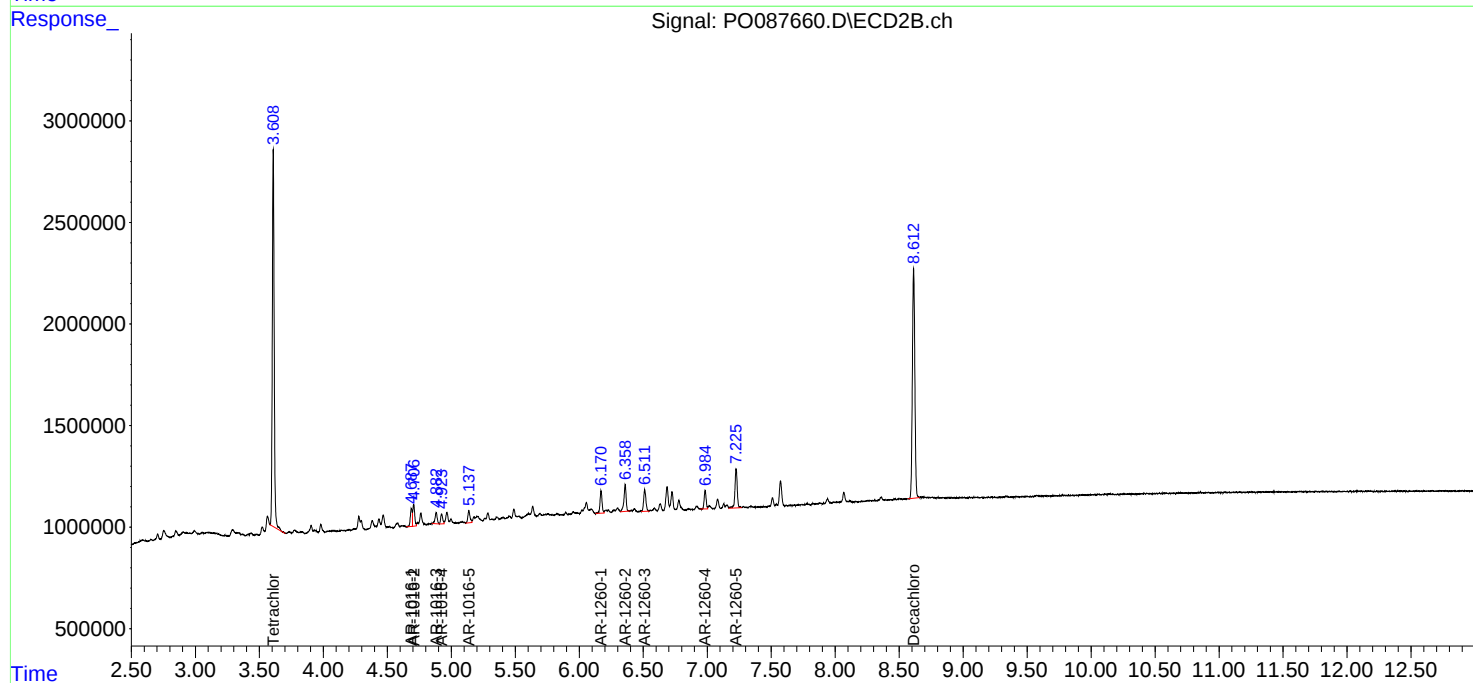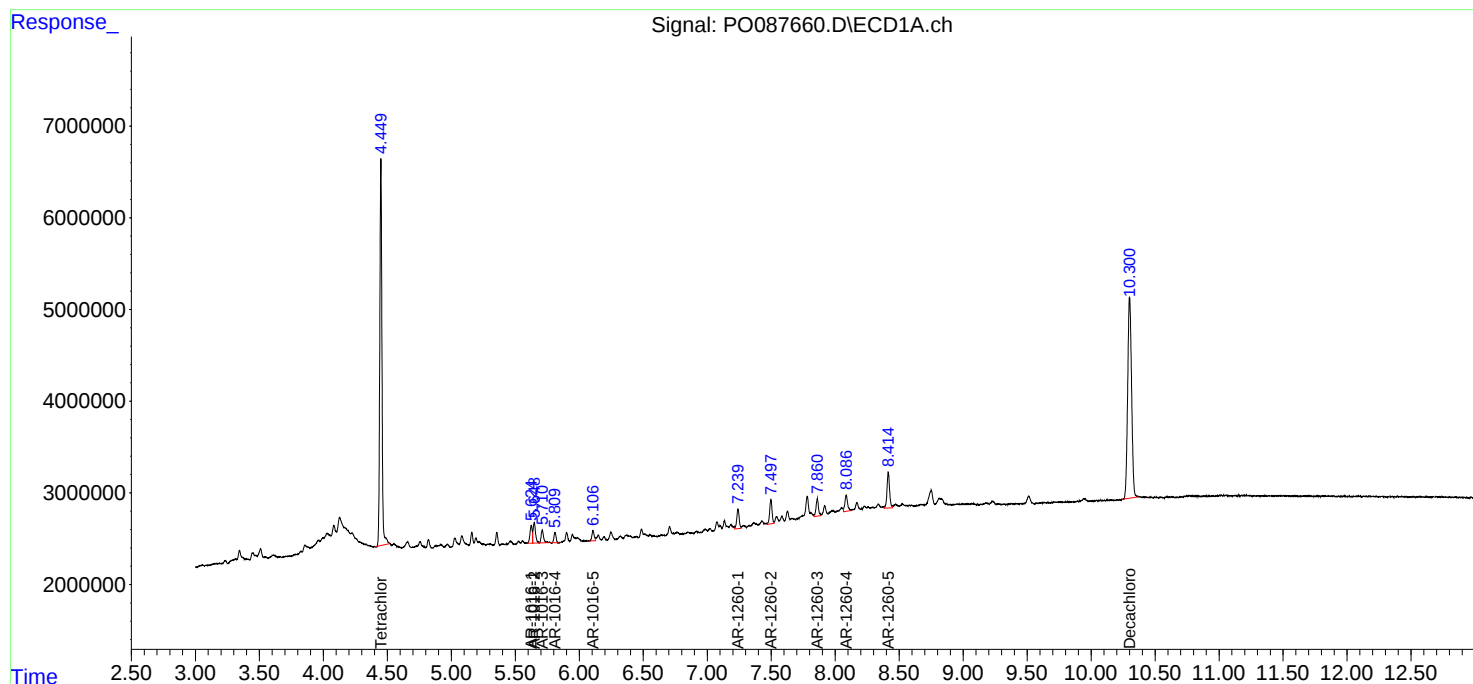


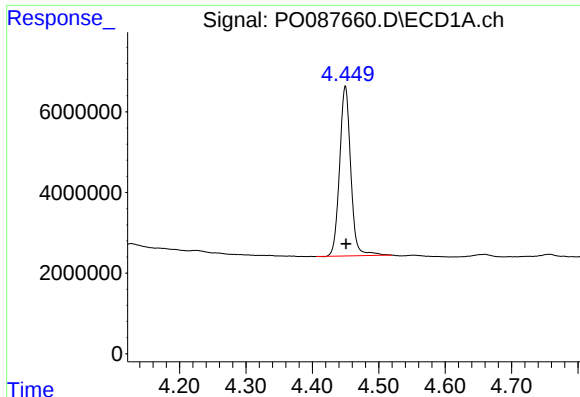

#1 Tetrachloro-m-xylene


R.T.: 4.450 min
Delta R.T.: -0.001 min
Response: 49092221
Conc: 18.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

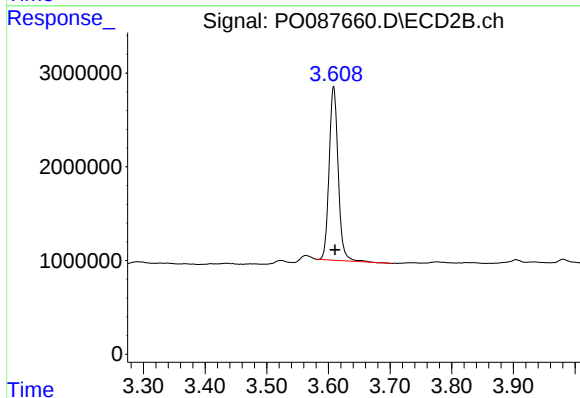


#1 Tetrachloro-m-xylene

R.T.: 3.608 min
Delta R.T.: -0.003 min
Response: 18952296
Conc: 19.26 ng/ml

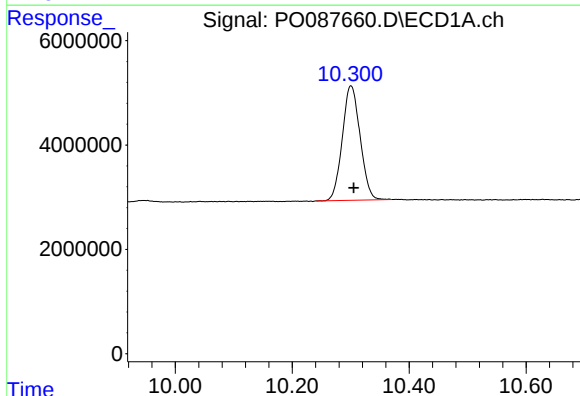


#2 Decachlorobiphenyl

R.T.: 10.300 min
Delta R.T.: -0.005 min
Response: 46364260
Conc: 22.70 ng/ml

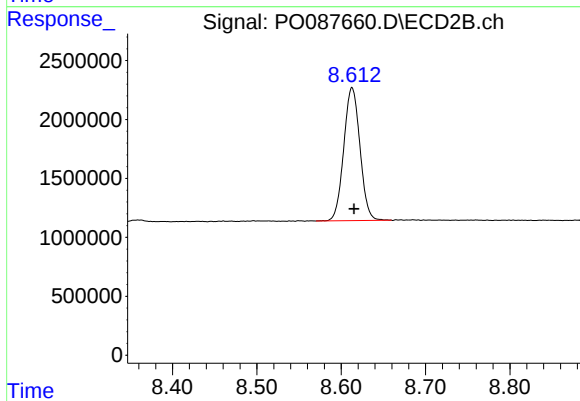

#2 Decachlorobiphenyl


R.T.: 8.613 min
Delta R.T.: -0.002 min
Response: 15051252
Conc: 18.57 ng/ml

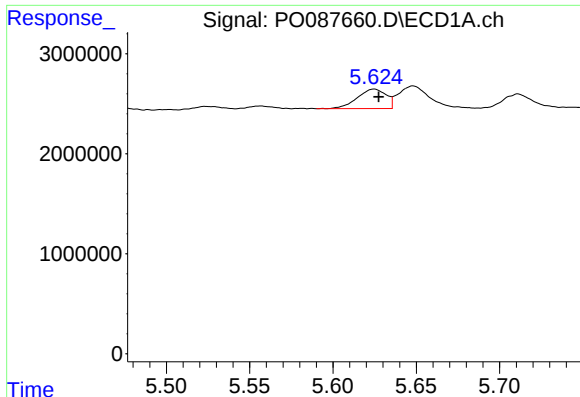

#3 AR-1016-1


R.T.: 5.625 min
Delta R.T.: -0.003 min
Response: 2347853
Conc: 26.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

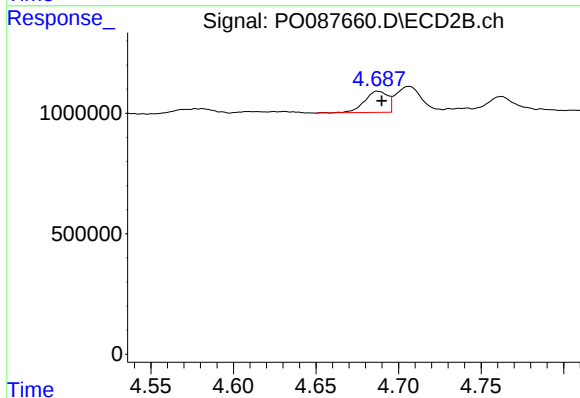


#3 AR-1016-1

R.T.: 4.688 min
Delta R.T.: -0.002 min
Response: 860973
Conc: 21.53 ng/ml

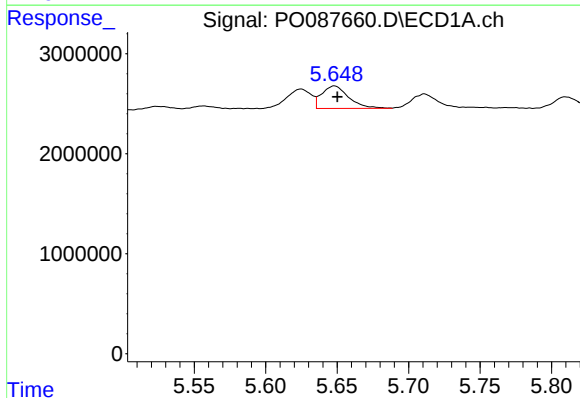


#4 AR-1016-2

R.T.: 5.648 min
Delta R.T.: -0.002 min
Response: 2938721
Conc: 23.38 ng/ml

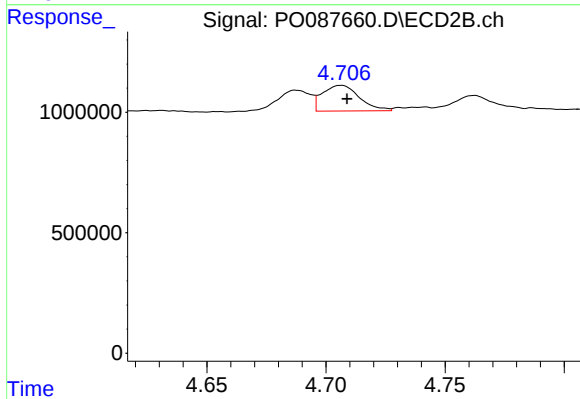

#4 AR-1016-2


R.T.: 4.706 min
Delta R.T.: -0.002 min
Response: 1153572
Conc: 20.69 ng/ml

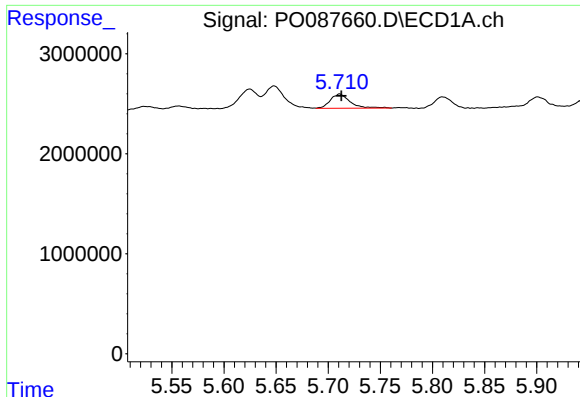

#5 AR-1016-3


R.T.: 5.711 min
Delta R.T.: -0.002 min
Response: 1868650
Conc: 24.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

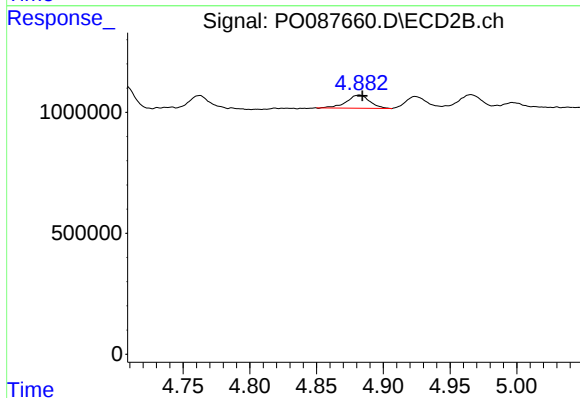


#5 AR-1016-3

R.T.: 4.882 min
Delta R.T.: -0.002 min
Response: 663152
Conc: 22.53 ng/ml

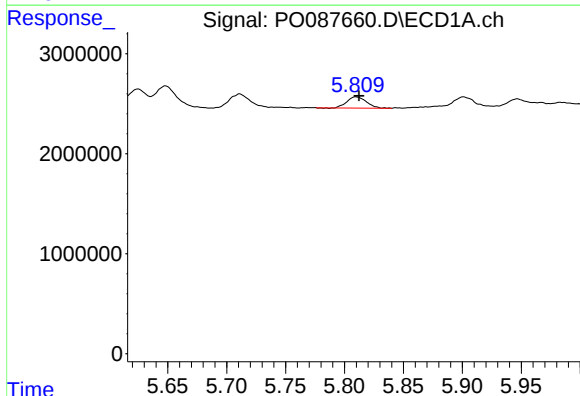


#6 AR-1016-4

R.T.: 5.810 min
Delta R.T.: -0.002 min
Response: 1302864
Conc: 21.32 ng/ml

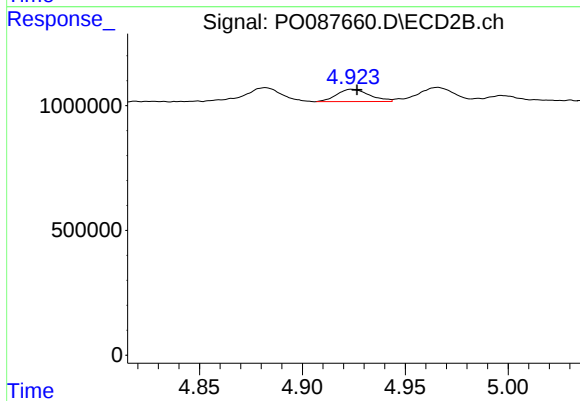

#6 AR-1016-4


R.T.: 4.924 min
Delta R.T.: -0.002 min
Response: 545947
Conc: 22.72 ng/ml

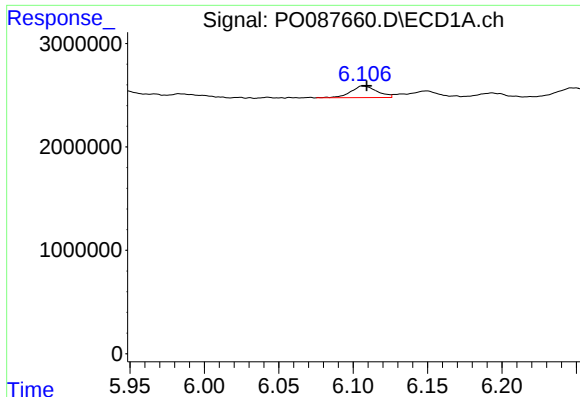

#7 AR-1016-5


R.T.: 6.107 min
Delta R.T.: -0.002 min
Response: 1392639
Conc: 23.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

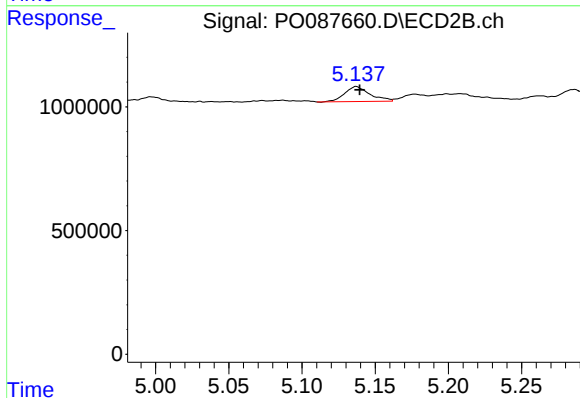


#7 AR-1016-5

R.T.: 5.137 min
Delta R.T.: -0.002 min
Response: 729644
Conc: 23.85 ng/ml

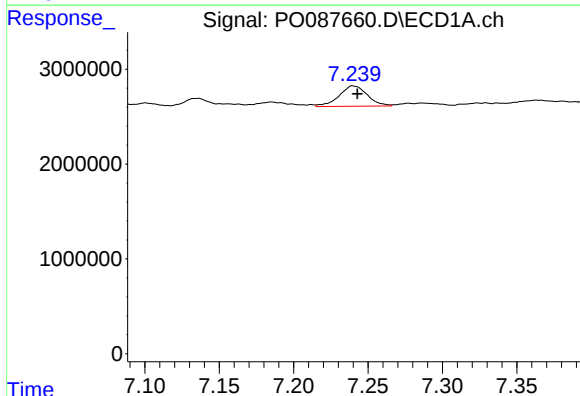


#31 AR-1260-1

R.T.: 7.240 min
Delta R.T.: -0.003 min
Response: 2846232
Conc: 25.39 ng/ml

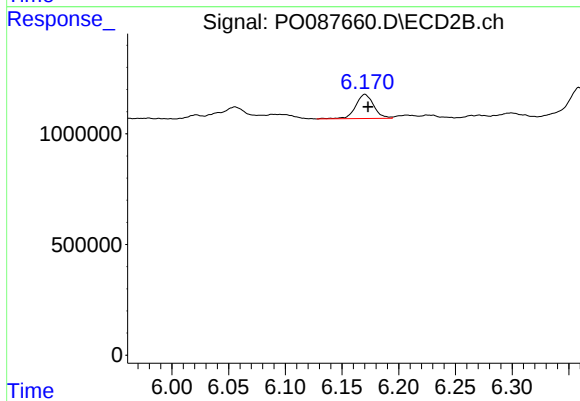

#31 AR-1260-1


R.T.: 6.170 min
Delta R.T.: -0.003 min
Response: 1213469
Conc: 21.49 ng/ml

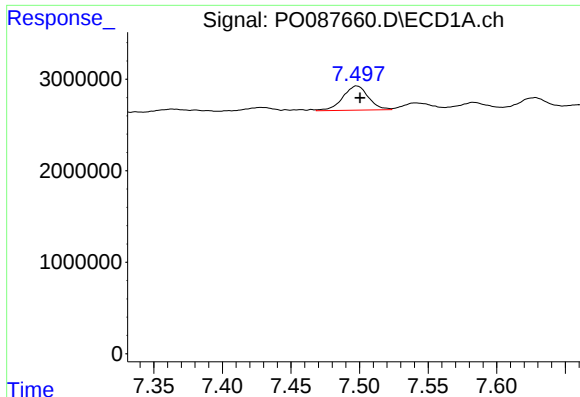

#32 AR-1260-2


R.T.: 7.498 min
Delta R.T.: -0.002 min
Response: 3418056
Conc: 25.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

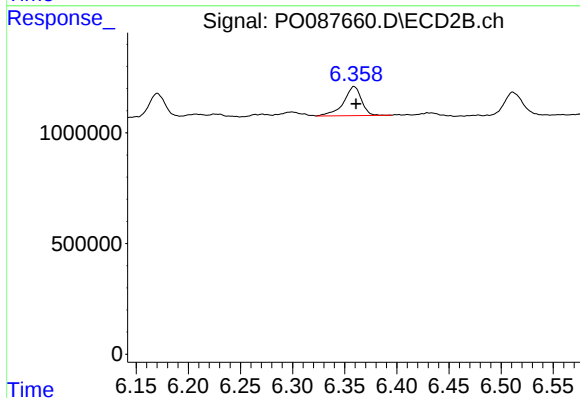


#32 AR-1260-2

R.T.: 6.359 min
Delta R.T.: -0.002 min
Response: 1582081
Conc: 23.38 ng/ml

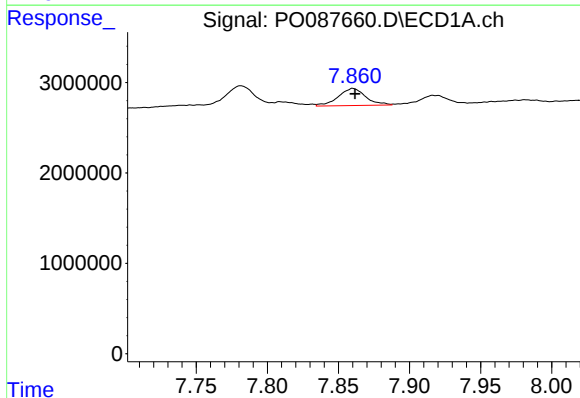


#33 AR-1260-3

R.T.: 7.860 min
Delta R.T.: -0.001 min
Response: 2529588
Conc: 27.01 ng/ml

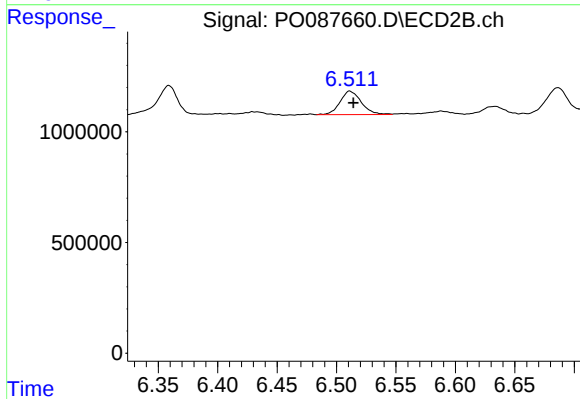

#33 AR-1260-3


R.T.: 6.511 min
Delta R.T.: -0.003 min
Response: 1317615
Conc: 20.86 ng/ml

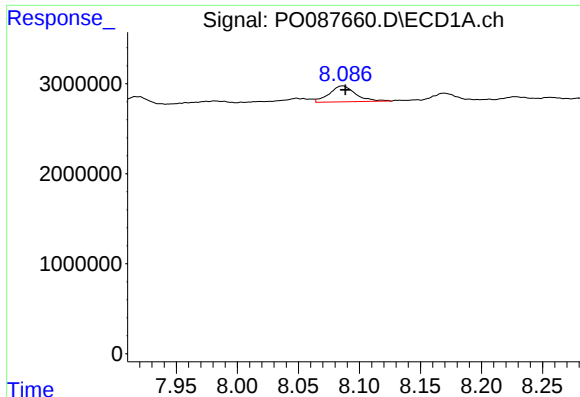

#34 AR-1260-4


R.T.: 8.086 min
Delta R.T.: -0.002 min
Response: 2671290
Conc: 25.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

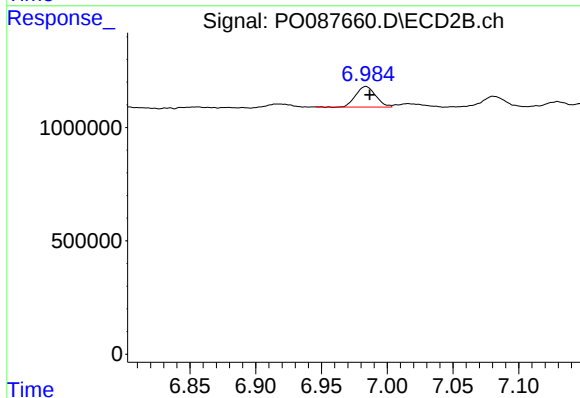


#34 AR-1260-4

R.T.: 6.984 min
Delta R.T.: -0.003 min
Response: 960665
Conc: 20.66 ng/ml

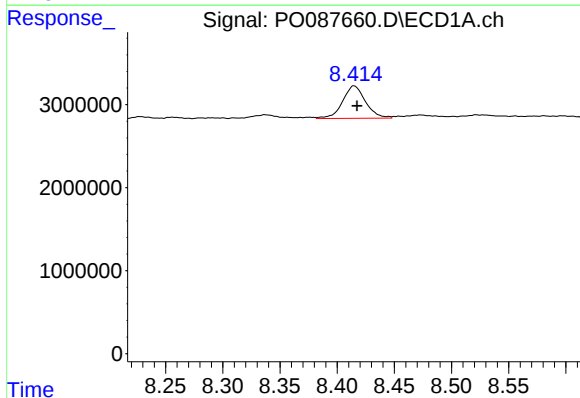

#35 AR-1260-5

R.T.: 8.415 min
Delta R.T.: -0.003 min
Response: 5471250
Conc: 27.74 ng/ml

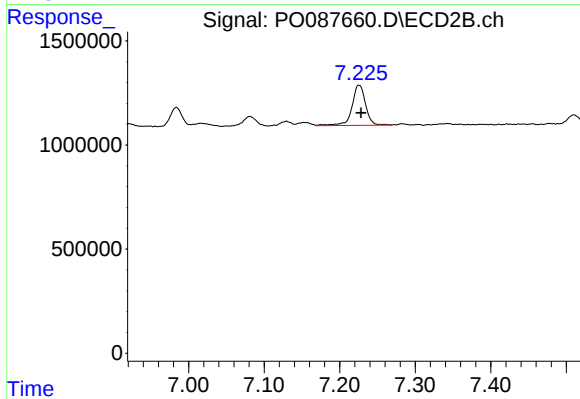

#35 AR-1260-5

R.T.: 7.226 min
Delta R.T.: -0.002 min
Response: 2392955
Conc: 22.20 ng/ml