

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063022\
 Data File : P0087662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 19:35
 Operator : YP/AJ
 Sample : N3214-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 03:05:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.449	3.609	48127758	19426992	18.594	19.743
2) SA Decachlor...	10.302	8.612	44763257	14597774	21.914	18.007
Target Compounds						
11) L3 AR-1232-1	4.821	3.981	1361933	543020	20.806	20.918
12) L3 AR-1232-2	5.160	4.707	913157	491200	28.279	20.144 #
13) L3 AR-1232-3	5.649	4.883	1229649	256276	20.390	20.636
14) L3 AR-1232-4	5.810	4.966	504326	222498	17.225	19.624
15) L3 AR-1232-5	5.900	5.137	578612	350490	23.464	27.930



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO063022\
Data File : PO087662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 19:35
Operator : YP/AJ
Sample : N3214-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 03:05:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

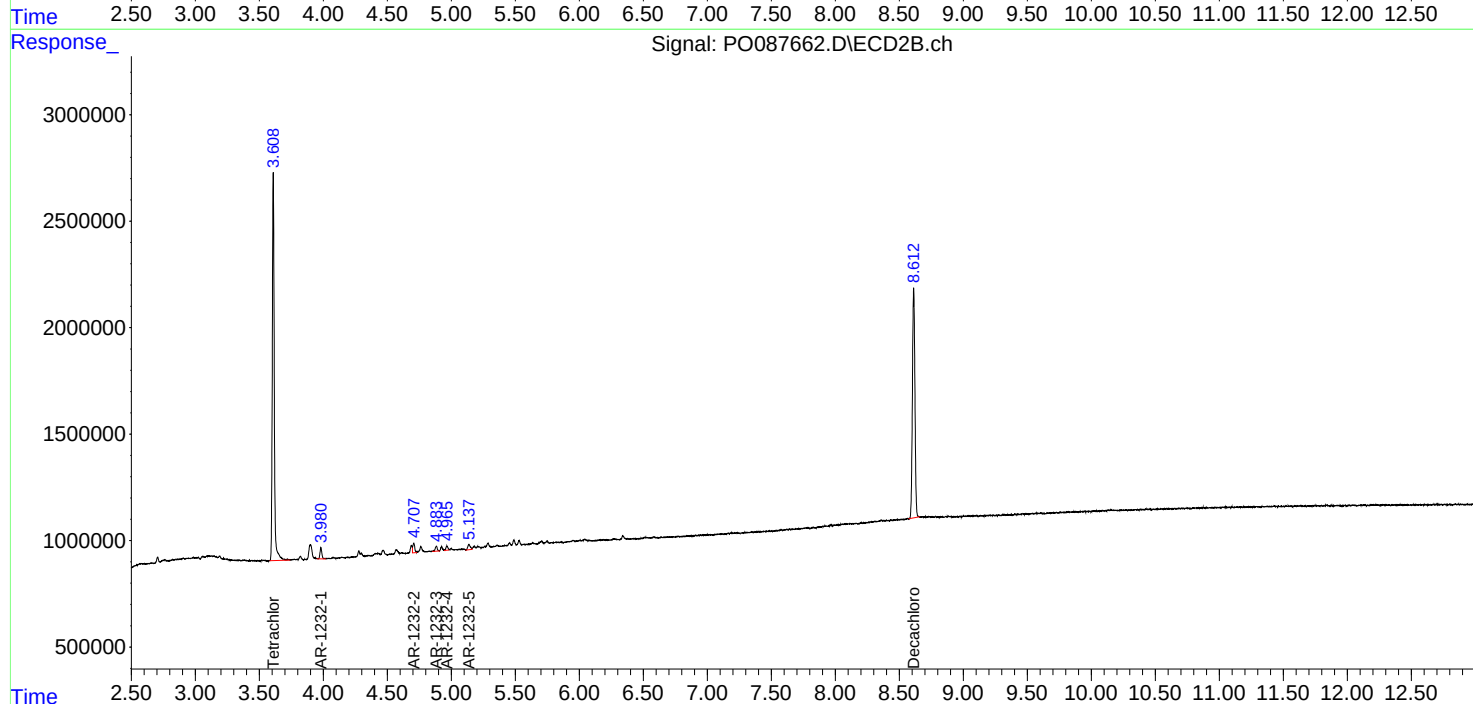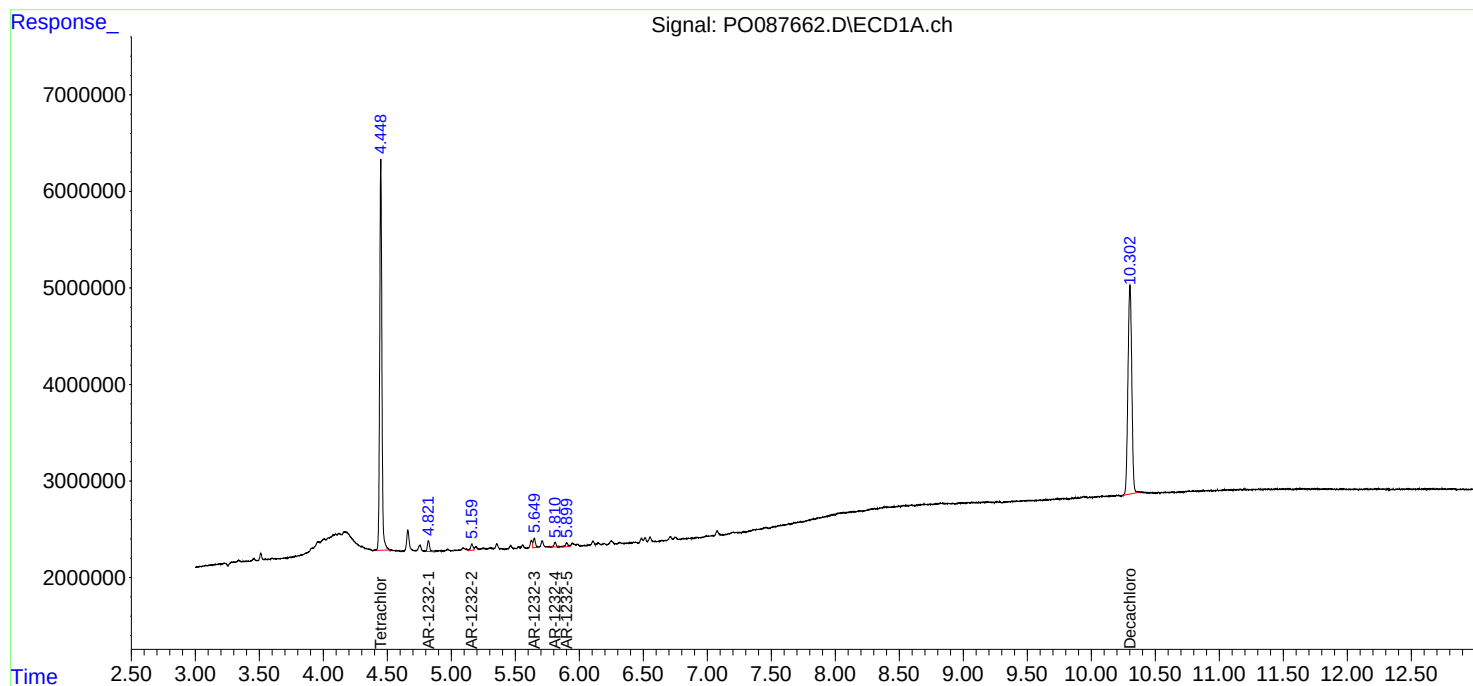


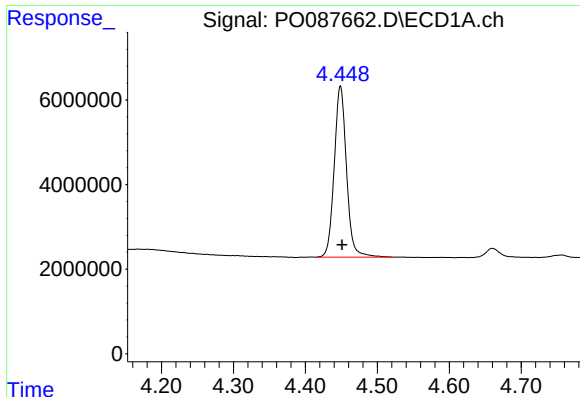

#1 Tetrachloro-m-xylene


R.T.: 4.449 min
Delta R.T.: -0.002 min
Response: 48127758
Conc: 18.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

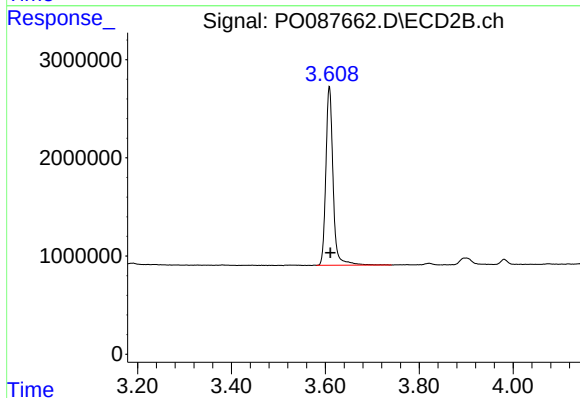


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: -0.002 min
Response: 19426992
Conc: 19.74 ng/ml

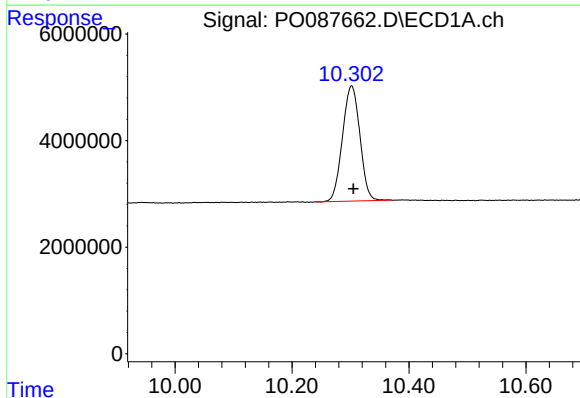


#2 Decachlorobiphenyl

R.T.: 10.302 min
Delta R.T.: -0.004 min
Response: 44763257
Conc: 21.91 ng/ml

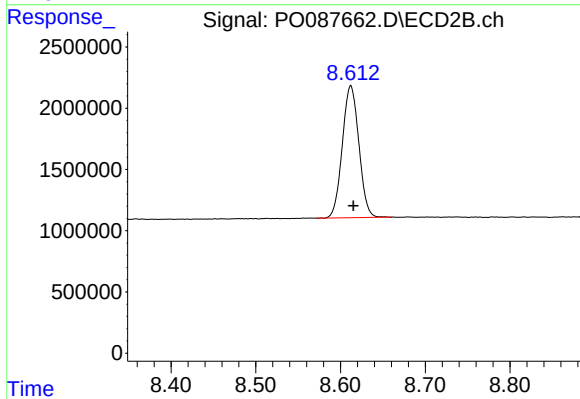

#2 Decachlorobiphenyl


R.T.: 8.612 min
Delta R.T.: -0.003 min
Response: 14597774
Conc: 18.01 ng/ml

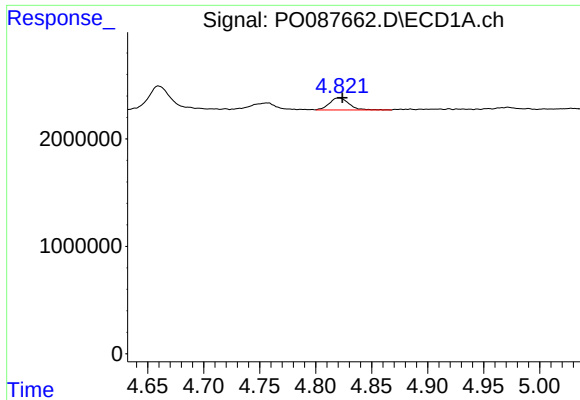

#11 AR-1232-1


R.T.: 4.821 min
Delta R.T.: -0.003 min
Response: 1361933
Conc: 20.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

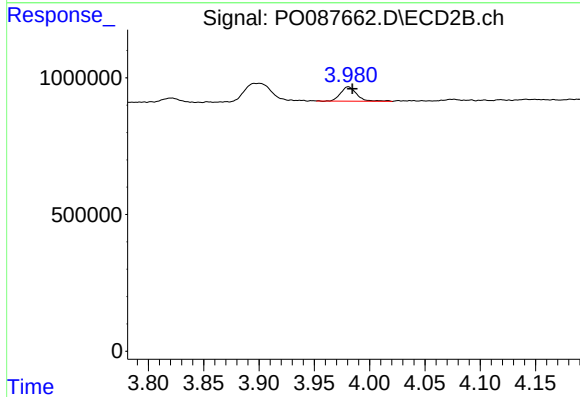


#11 AR-1232-1

R.T.: 3.981 min
Delta R.T.: -0.004 min
Response: 543020
Conc: 20.92 ng/ml

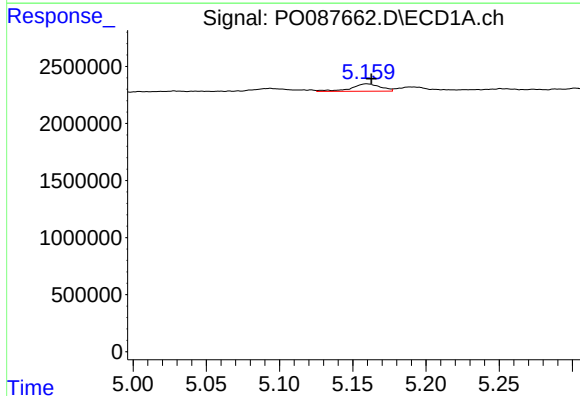


#12 AR-1232-2

R.T.: 5.160 min
Delta R.T.: -0.003 min
Response: 913157
Conc: 28.28 ng/ml

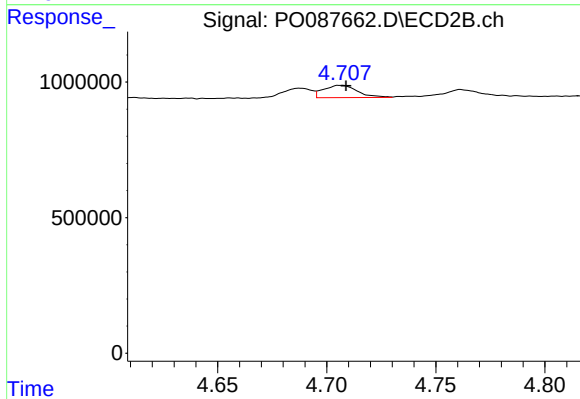

#12 AR-1232-2


R.T.: 4.707 min
Delta R.T.: -0.002 min
Response: 491200
Conc: 20.14 ng/ml

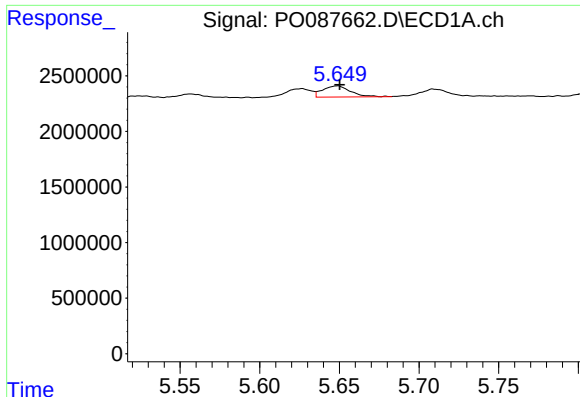

#13 AR-1232-3


R.T.: 5.649 min
Delta R.T.: -0.002 min
Response: 1229649
Conc: 20.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

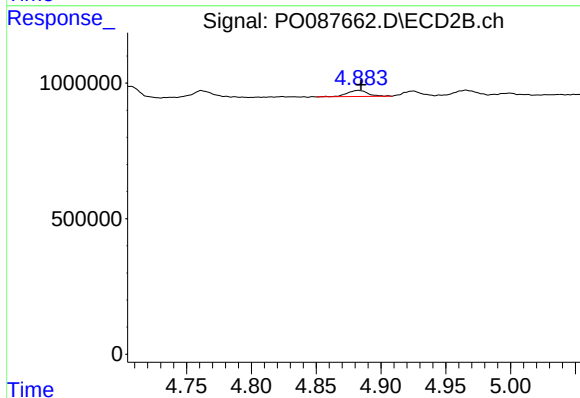


#13 AR-1232-3

R.T.: 4.883 min
Delta R.T.: -0.002 min
Response: 256276
Conc: 20.64 ng/ml

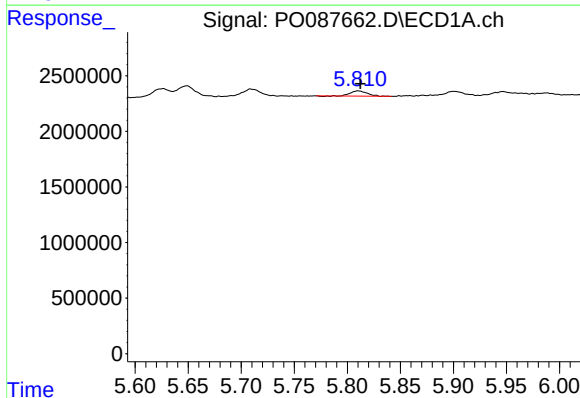


#14 AR-1232-4

R.T.: 5.810 min
Delta R.T.: -0.002 min
Response: 504326
Conc: 17.22 ng/ml

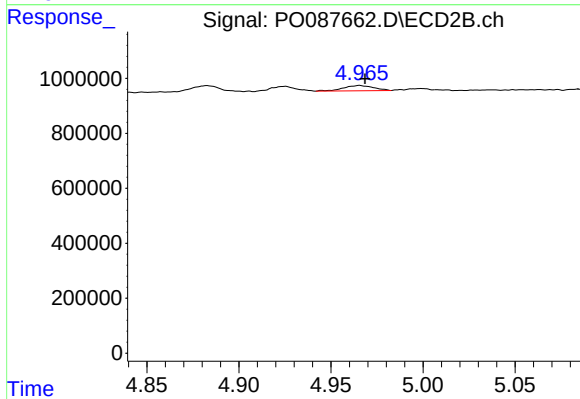

#14 AR-1232-4


R.T.: 4.966 min
Delta R.T.: -0.003 min
Response: 222498
Conc: 19.62 ng/ml

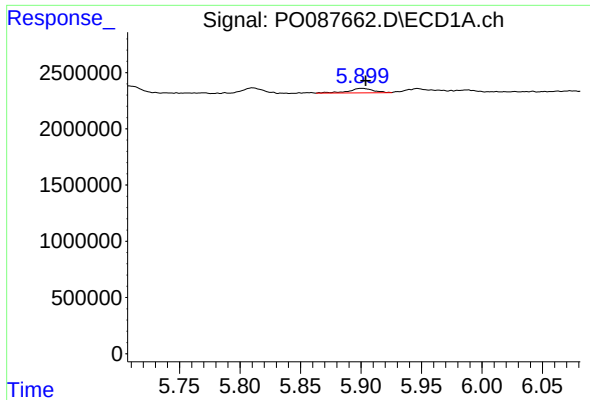

#15 AR-1232-5

R.T.: 5.900 min
Delta R.T.: -0.003 min
Response: 578612
Conc: 23.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

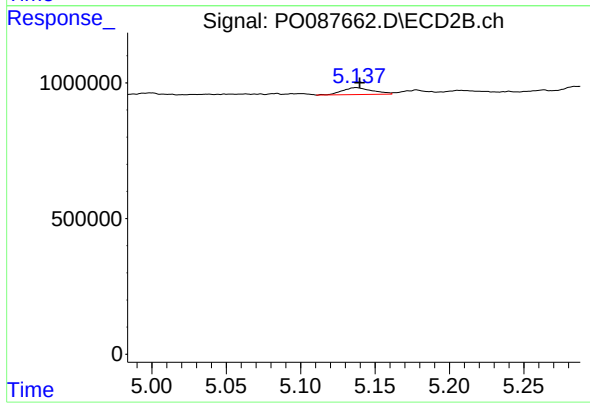

#15 AR-1232-5

R.T.: 5.137 min
Delta R.T.: -0.002 min
Response: 350490
Conc: 27.93 ng/ml