

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063022\
 Data File : P0087664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 20:08
 Operator : YP/AJ
 Sample : N3214-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 03:06:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.448	3.608	47555691	19296464	18.373	19.610
2)	SA Decachlor...	10.300	8.611	44787691	14389325	21.926	17.750
Target Compounds							
21)	L5 AR-1248-1	5.625	4.687	1208396	474726	21.049	20.457
22)	L5 AR-1248-2	5.900	4.924	1912573	747908	22.940	23.796
23)	L5 AR-1248-3	6.106	4.965	1882753	769546	21.015	23.709
24)	L5 AR-1248-4	6.512	5.136	2239798	929839	22.770	24.102
25)	L5 AR-1248-5	6.552	5.529	2158149	854260	22.452	23.435



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO063022\
Data File : PO087664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 20:08
Operator : YP/AJ
Sample : N3214-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 03:06:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

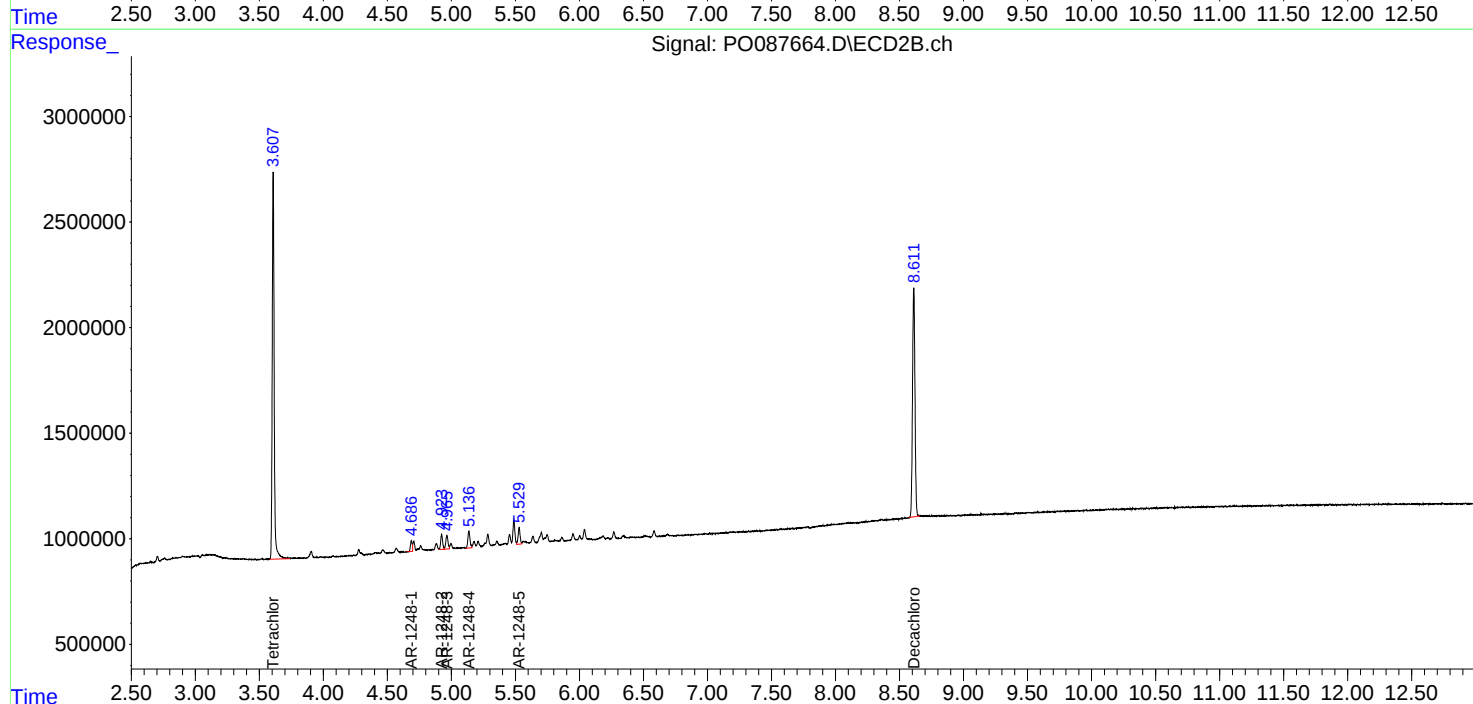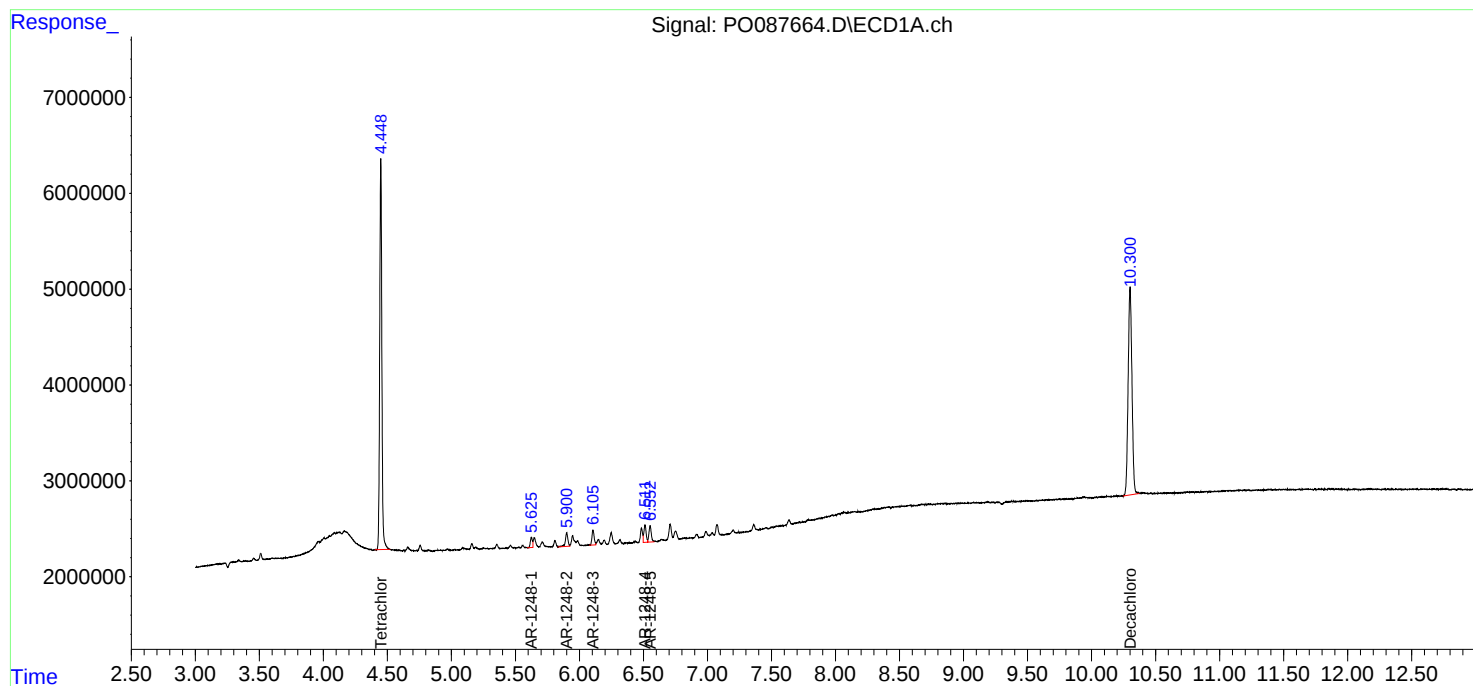


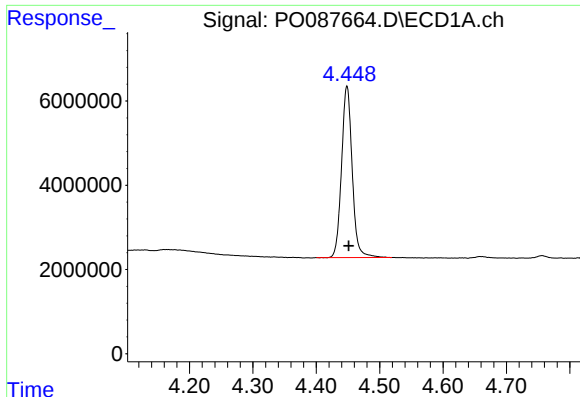

#1 Tetrachloro-m-xylene


R.T.: 4.448 min
Delta R.T.: -0.003 min
Response: 47555691
Conc: 18.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

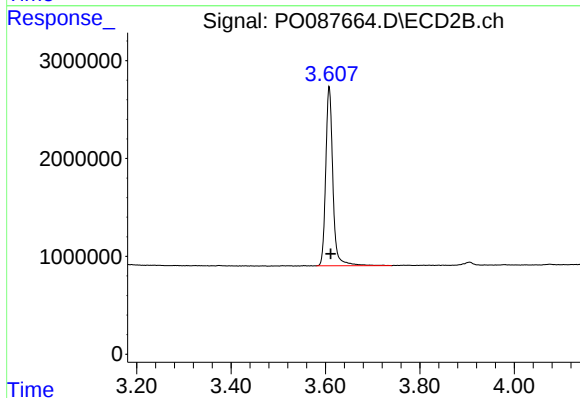


#1 Tetrachloro-m-xylene

R.T.: 3.608 min
Delta R.T.: -0.003 min
Response: 19296464
Conc: 19.61 ng/ml

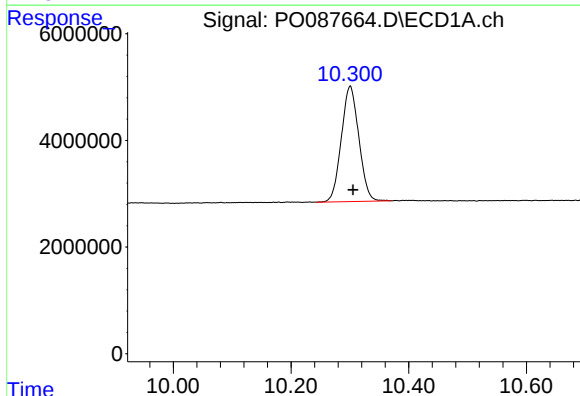


#2 Decachlorobiphenyl

R.T.: 10.300 min
Delta R.T.: -0.005 min
Response: 44787691
Conc: 21.93 ng/ml

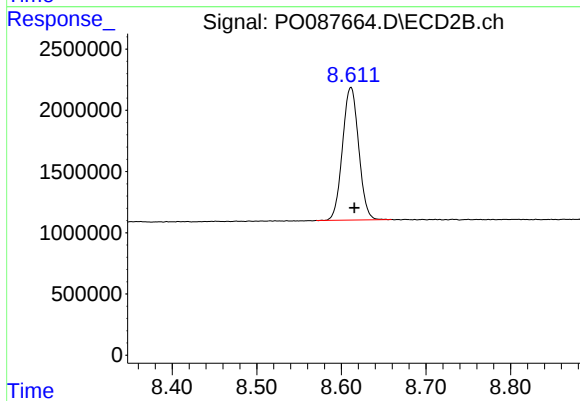

#2 Decachlorobiphenyl


R.T.: 8.611 min
Delta R.T.: -0.004 min
Response: 14389325
Conc: 17.75 ng/ml

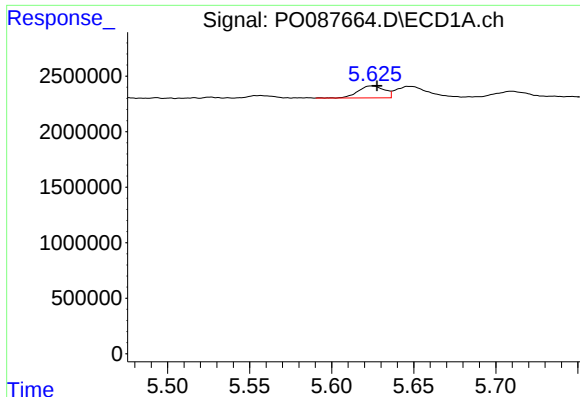

#21 AR-1248-1


R.T.: 5.625 min
Delta R.T.: -0.003 min
Response: 1208396
Conc: 21.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

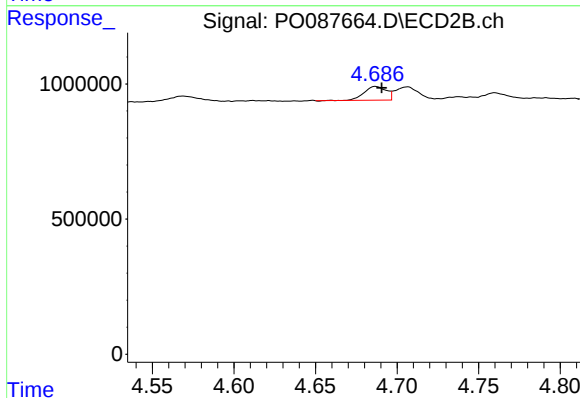


#21 AR-1248-1

R.T.: 4.687 min
Delta R.T.: -0.003 min
Response: 474726
Conc: 20.46 ng/ml

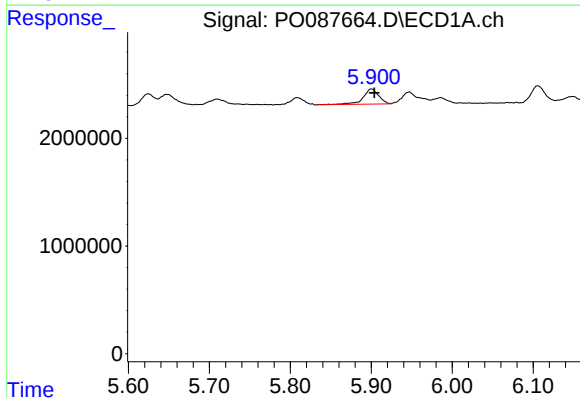


#22 AR-1248-2

R.T.: 5.900 min
Delta R.T.: -0.003 min
Response: 1912573
Conc: 22.94 ng/ml

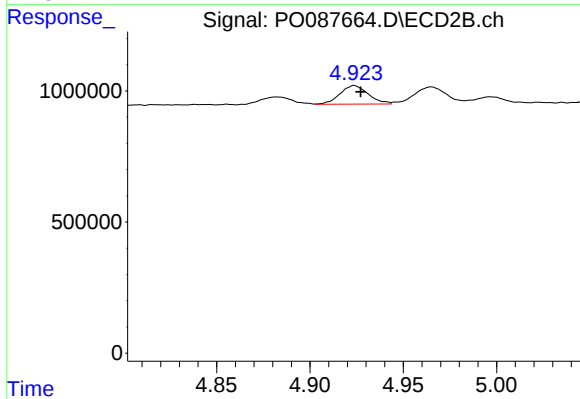

#22 AR-1248-2


R.T.: 4.924 min
Delta R.T.: -0.003 min
Response: 747908
Conc: 23.80 ng/ml

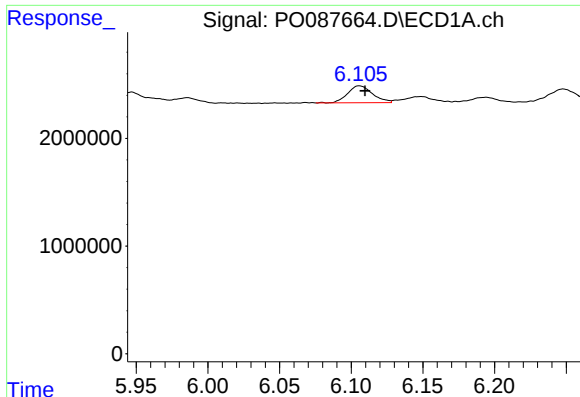

#23 AR-1248-3


R.T.: 6.106 min
Delta R.T.: -0.004 min
Response: 1882753
Conc: 21.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

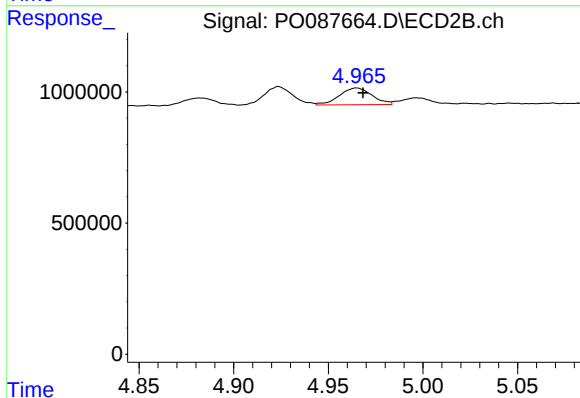


#23 AR-1248-3

R.T.: 4.965 min
Delta R.T.: -0.003 min
Response: 769546
Conc: 23.71 ng/ml

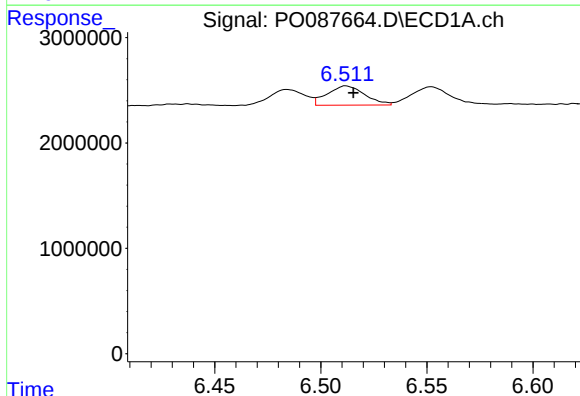


#24 AR-1248-4

R.T.: 6.512 min
Delta R.T.: -0.003 min
Response: 2239798
Conc: 22.77 ng/ml

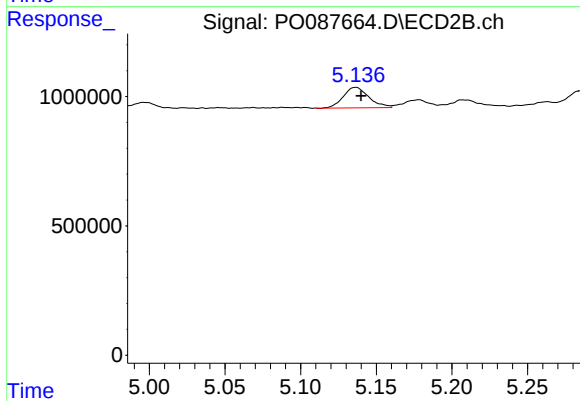

#24 AR-1248-4


R.T.: 5.136 min
Delta R.T.: -0.004 min
Response: 929839
Conc: 24.10 ng/ml

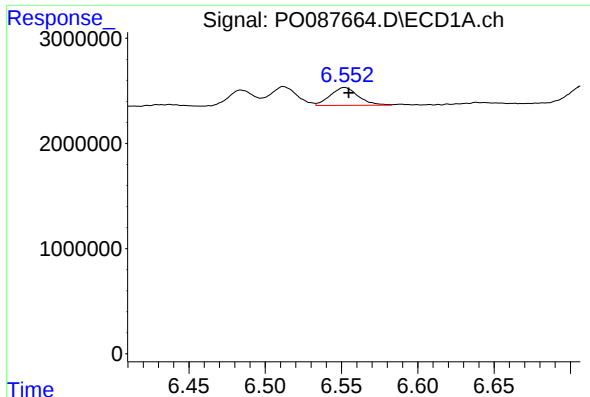

#25 AR-1248-5

R.T.: 6.552 min
Delta R.T.: -0.003 min
Response: 2158149
Conc: 22.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

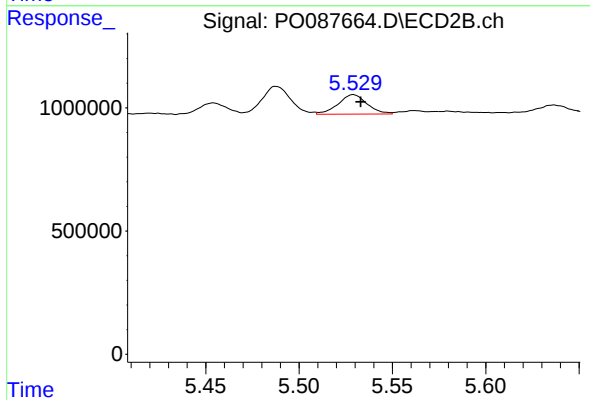

#25 AR-1248-5

R.T.: 5.529 min
Delta R.T.: -0.004 min
Response: 854260
Conc: 23.44 ng/ml