

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063022\
 Data File : P0087665.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 20:25
 Operator : YP/AJ
 Sample : N3214-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 03:07:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.449	3.608	49328965	19714356	19.058	20.035
2) SA Decachlor...	10.302	8.611	45706922	14870376	22.376	18.343
Target Compounds						
26) L6 AR-1254-1	6.487	5.489	2691177	1429114	26.848	25.853
27) L6 AR-1254-2	6.706	5.636	3982178	1282099	26.095	26.207
28) L6 AR-1254-3	7.075	6.039	4144213	2019391	27.209	26.612
29) L6 AR-1254-4	7.362	6.268	2799047	1144160	25.429	25.202
30) L6 AR-1254-5	7.783	6.686	2855920	1531610	23.793	23.958



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO063022\
Data File : PO087665.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 20:25
Operator : YP/AJ
Sample : N3214-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 03:07:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

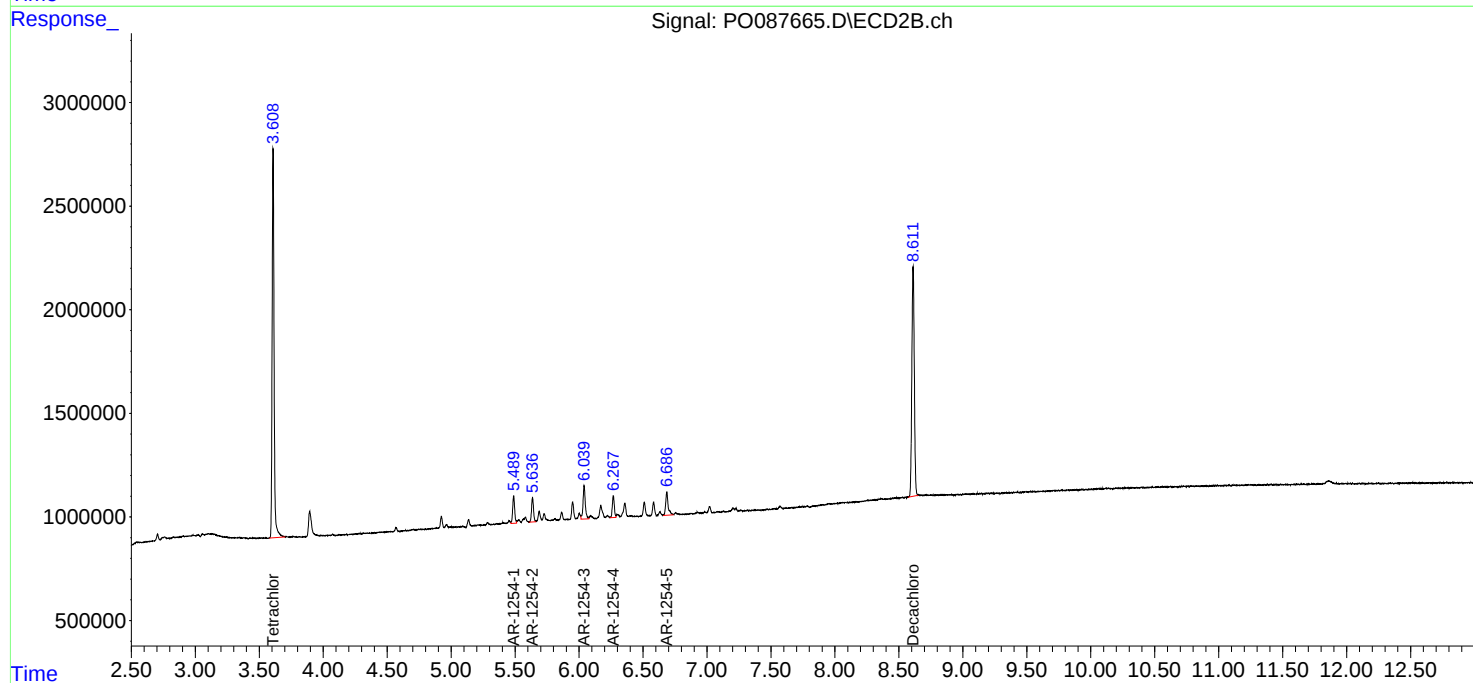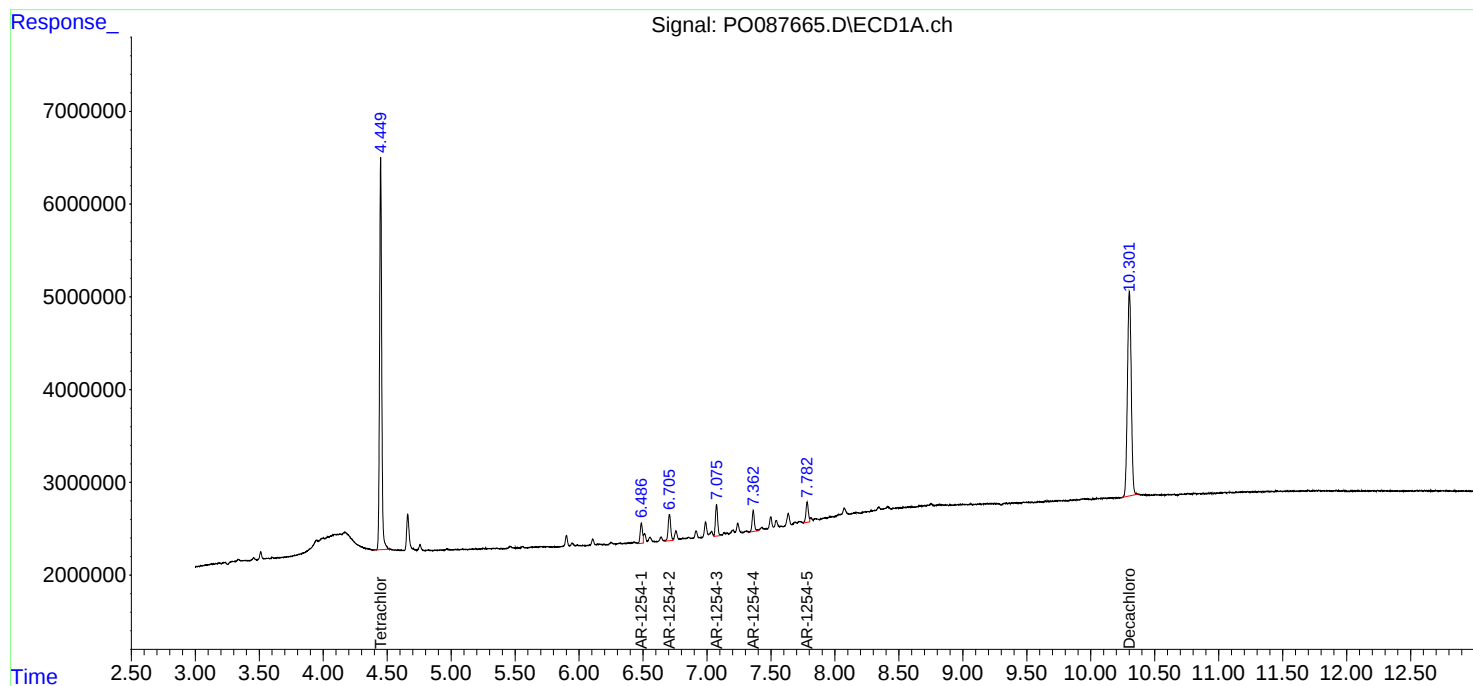


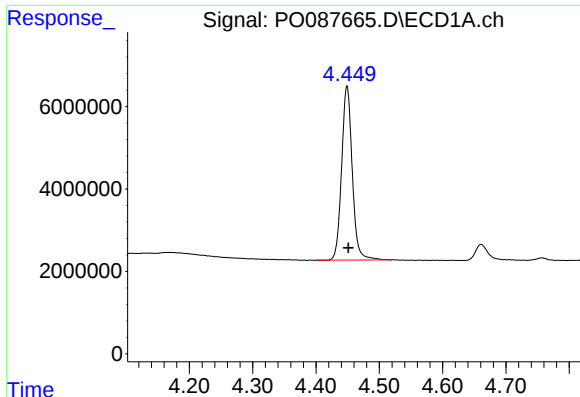

#1 Tetrachloro-m-xylene


R.T.: 4.449 min
Delta R.T.: -0.002 min
Response: 49328965
Conc: 19.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

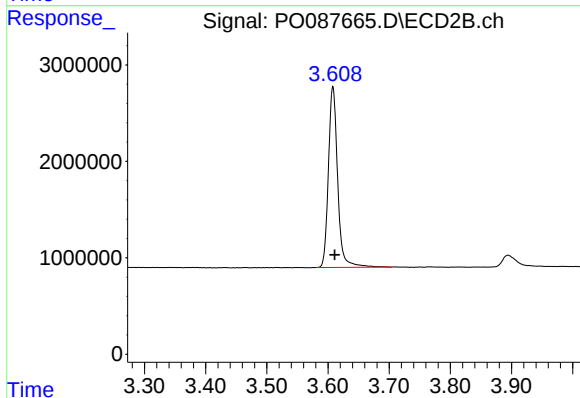


#1 Tetrachloro-m-xylene

R.T.: 3.608 min
Delta R.T.: -0.003 min
Response: 19714356
Conc: 20.04 ng/ml

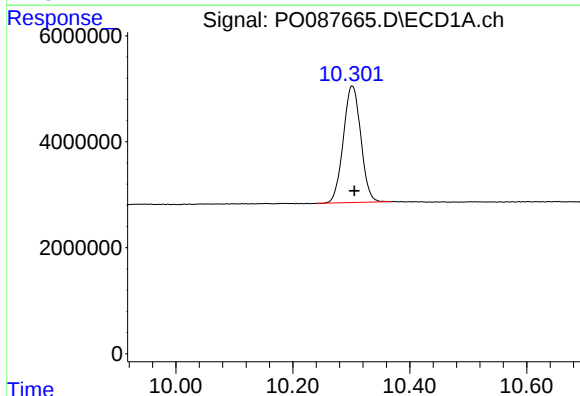


#2 Decachlorobiphenyl

R.T.: 10.302 min
Delta R.T.: -0.004 min
Response: 45706922
Conc: 22.38 ng/ml

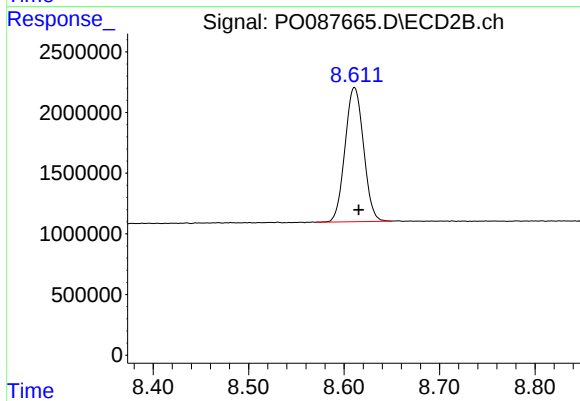

#2 Decachlorobiphenyl


R.T.: 8.611 min
Delta R.T.: -0.004 min
Response: 14870376
Conc: 18.34 ng/ml

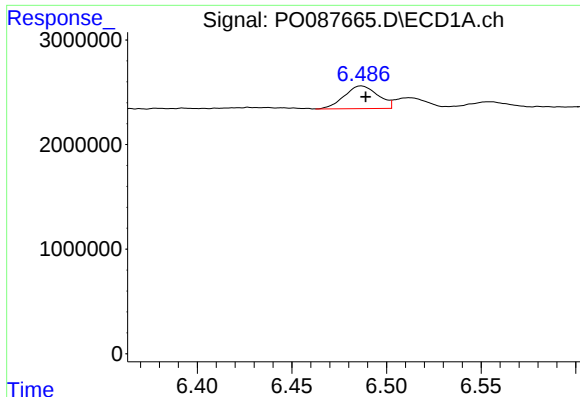

#26 AR-1254-1


R.T.: 6.487 min
Delta R.T.: -0.002 min
Response: 2691177
Conc: 26.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

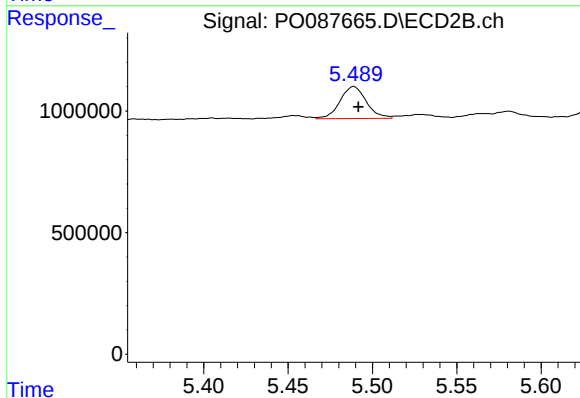


#26 AR-1254-1

R.T.: 5.489 min
Delta R.T.: -0.003 min
Response: 1429114
Conc: 25.85 ng/ml

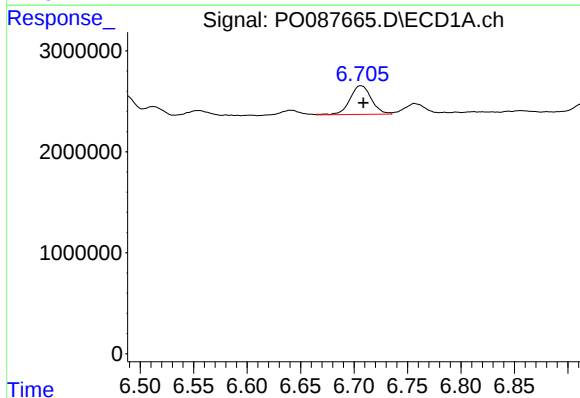


#27 AR-1254-2

R.T.: 6.706 min
Delta R.T.: -0.002 min
Response: 3982178
Conc: 26.10 ng/ml

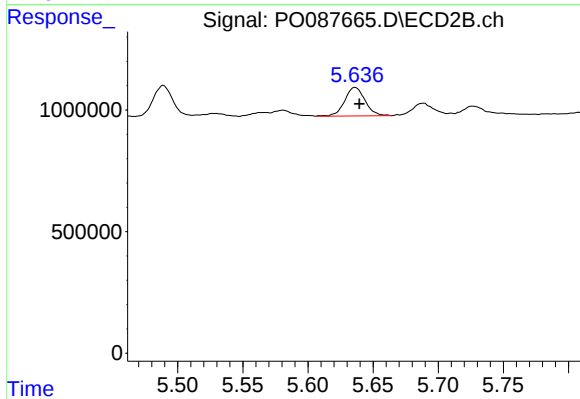

#27 AR-1254-2


R.T.: 5.636 min
Delta R.T.: -0.003 min
Response: 1282099
Conc: 26.21 ng/ml

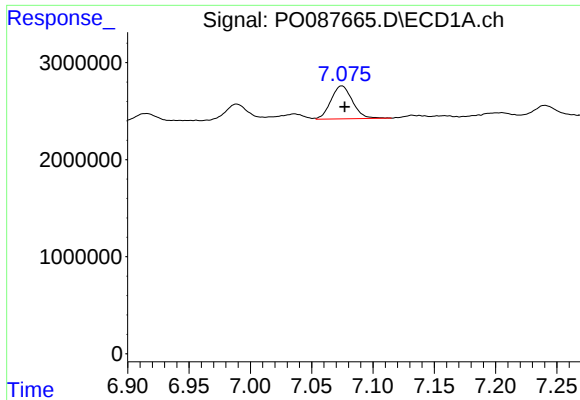

#28 AR-1254-3


R.T.: 7.075 min
Delta R.T.: -0.002 min
Response: 4144213
Conc: 27.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

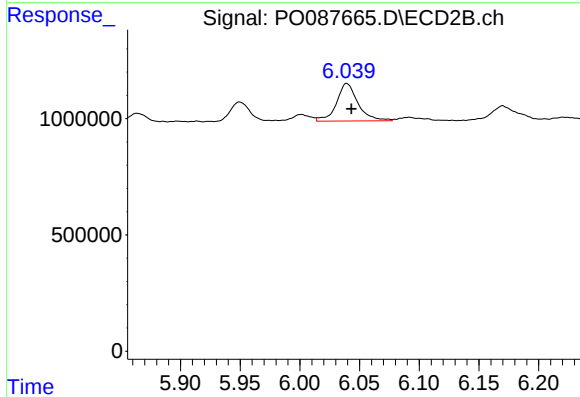


#28 AR-1254-3

R.T.: 6.039 min
Delta R.T.: -0.004 min
Response: 2019391
Conc: 26.61 ng/ml

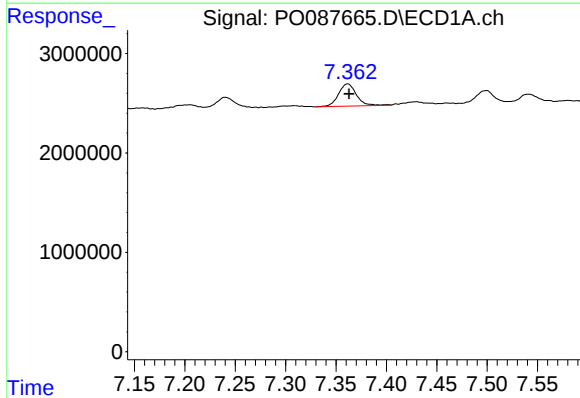


#29 AR-1254-4

R.T.: 7.362 min
Delta R.T.: -0.002 min
Response: 2799047
Conc: 25.43 ng/ml

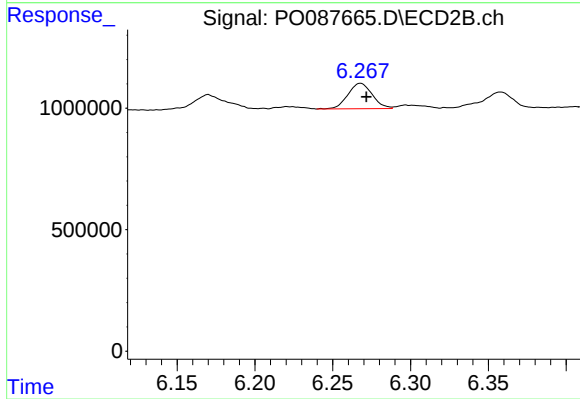

#29 AR-1254-4


R.T.: 6.268 min
Delta R.T.: -0.004 min
Response: 1144160
Conc: 25.20 ng/ml

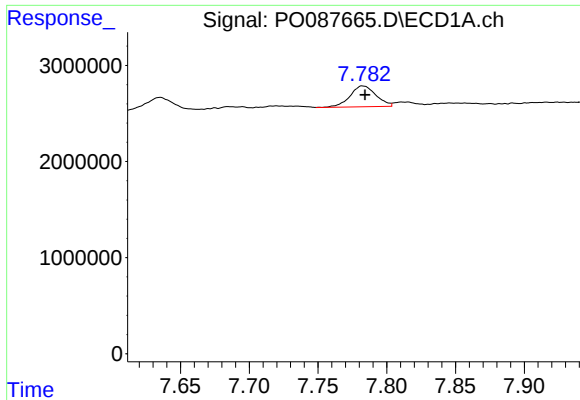

#30 AR-1254-5

R.T.: 7.783 min
Delta R.T.: -0.002 min
Response: 2855920
Conc: 23.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

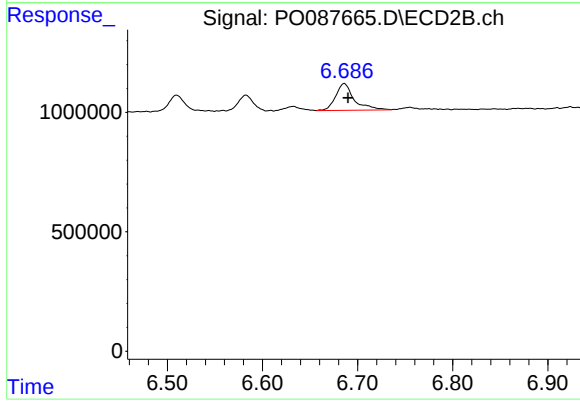

#30 AR-1254-5

R.T.: 6.686 min
Delta R.T.: -0.004 min
Response: 1531610
Conc: 23.96 ng/ml