

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063022\
 Data File : P0087667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 20:58
 Operator : YP/AJ
 Sample : N3214-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 03:07:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.449	3.608	47513909	19130787	18.357	19.442
2) SA Decachlor...	10.301	8.612	47725401	15484127	23.364	19.101
Target Compounds						
41) L9 AR-1268-1	8.736	7.509	6959442	2953576	23.724	25.657
42) L9 AR-1268-2	8.832	7.574	6404082	2571908	23.800	25.053
43) L9 AR-1268-3	9.070	7.781	5770756	2121566	24.689	25.063
44) L9 AR-1268-4	9.511	8.067	3315260	892279	32.430	25.153
45) L9 AR-1268-5	9.945	8.357	18452582	6113657	24.438	24.412



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063022\
Data File : P0087667.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 20:58
Operator : YP/AJ
Sample : N3214-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 03:07:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

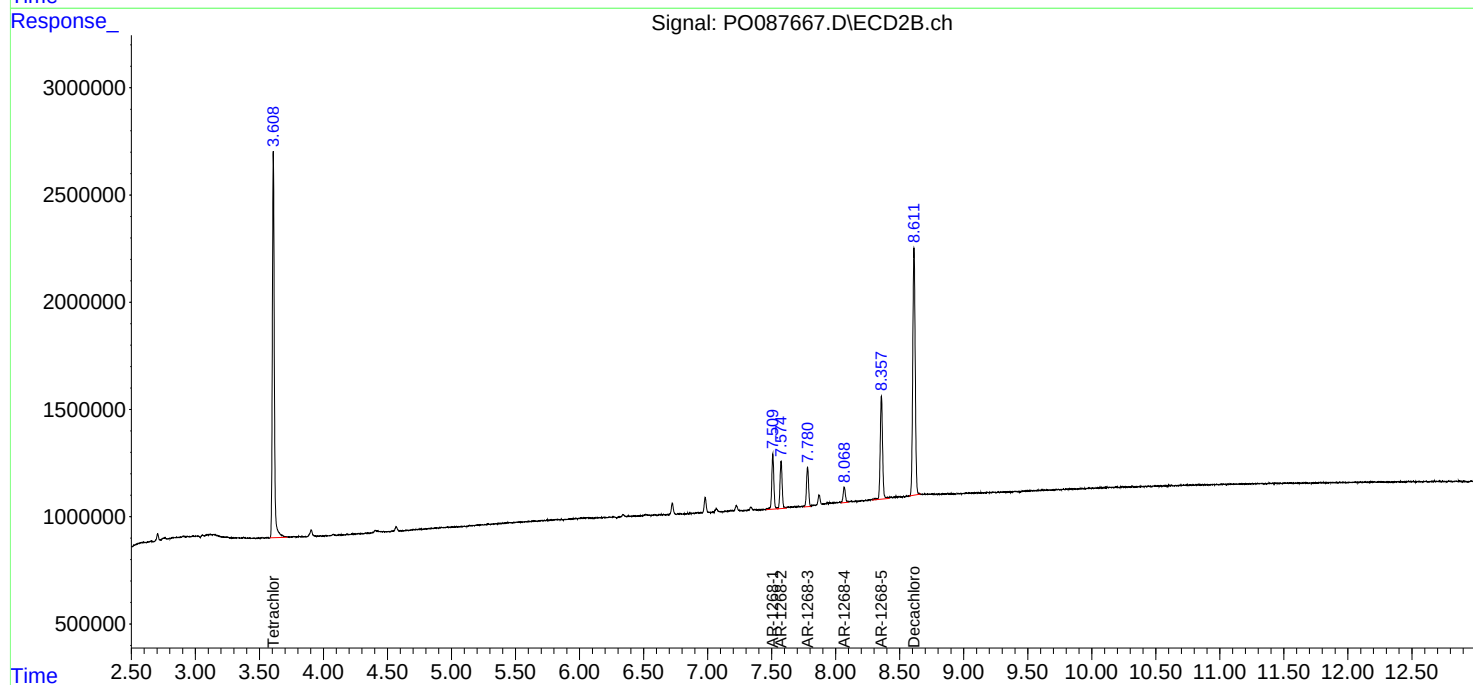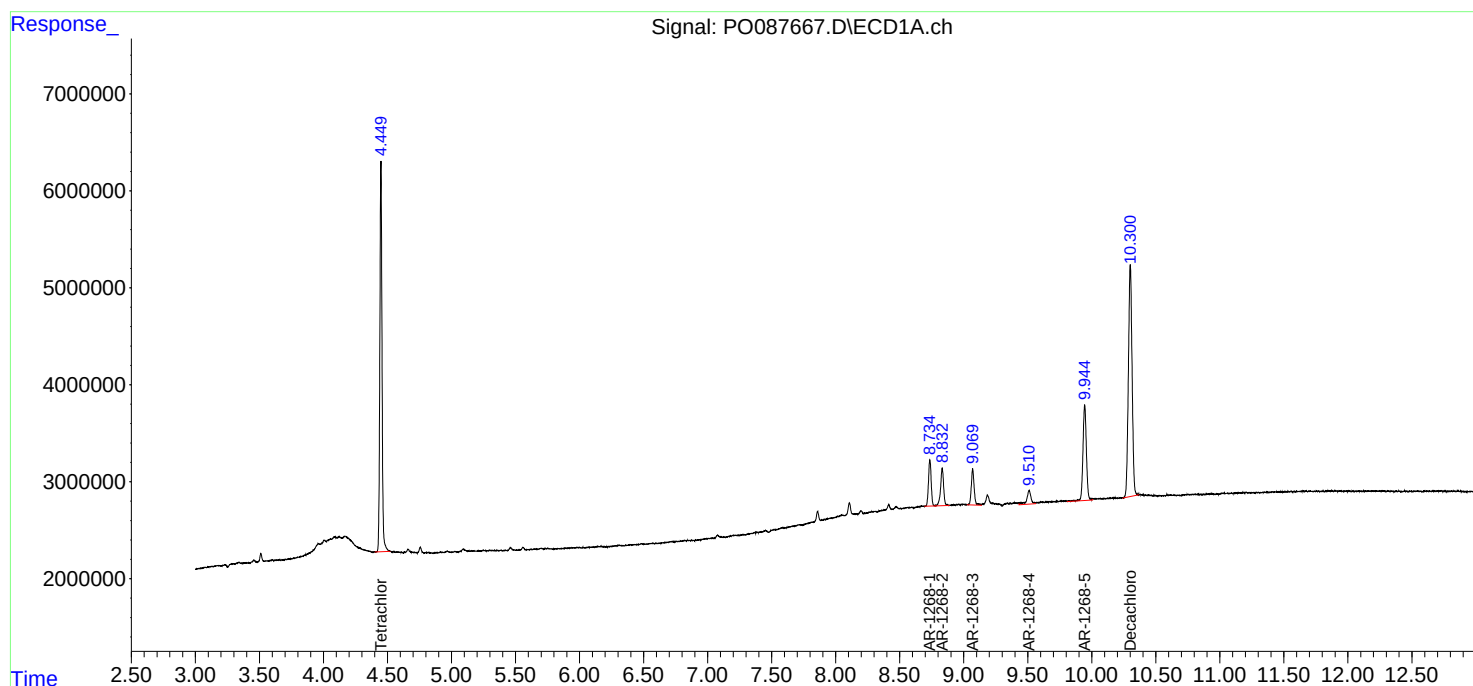


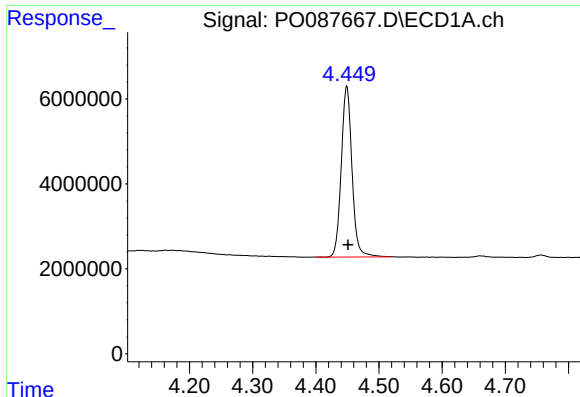

#1 Tetrachloro-m-xylene


R.T.: 4.449 min
Delta R.T.: -0.002 min
Response: 47513909
Conc: 18.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

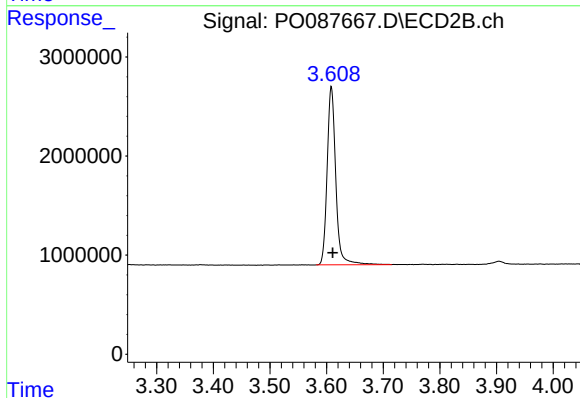


#1 Tetrachloro-m-xylene

R.T.: 3.608 min
Delta R.T.: -0.003 min
Response: 19130787
Conc: 19.44 ng/ml

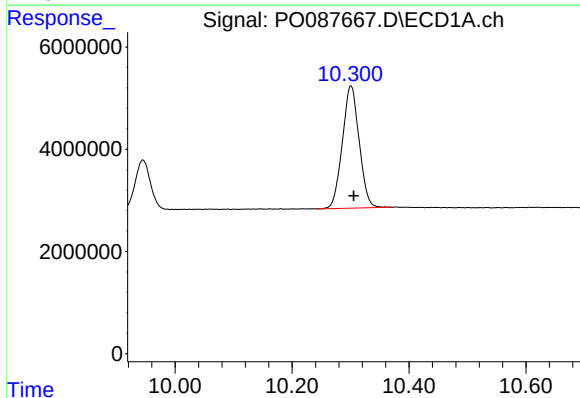


#2 Decachlorobiphenyl

R.T.: 10.301 min
Delta R.T.: -0.005 min
Response: 47725401
Conc: 23.36 ng/ml

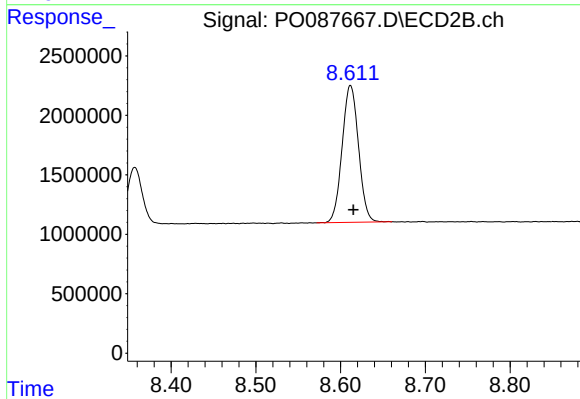

#2 Decachlorobiphenyl


R.T.: 8.612 min
Delta R.T.: -0.004 min
Response: 15484127
Conc: 19.10 ng/ml

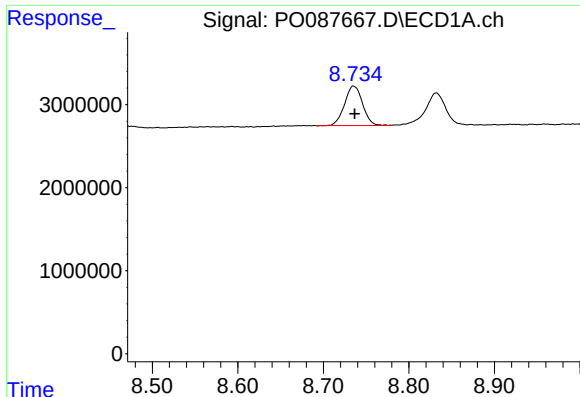

#41 AR-1268-1


R.T.: 8.736 min
Delta R.T.: -0.001 min
Response: 6959442
Conc: 23.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

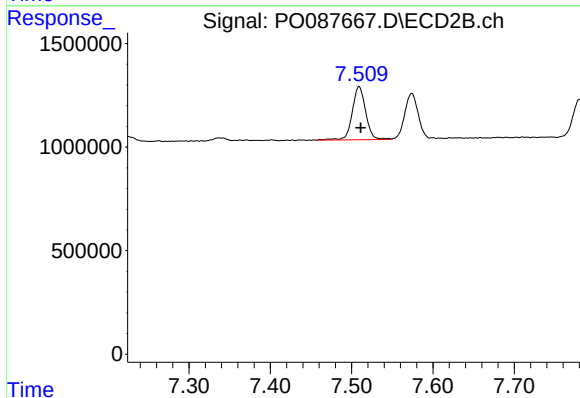


#41 AR-1268-1

R.T.: 7.509 min
Delta R.T.: -0.002 min
Response: 2953576
Conc: 25.66 ng/ml

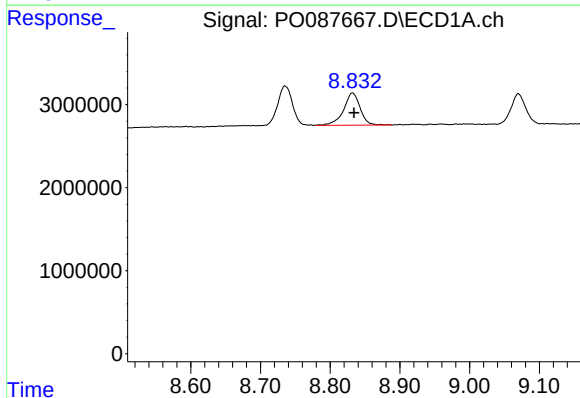


#42 AR-1268-2

R.T.: 8.832 min
Delta R.T.: -0.002 min
Response: 6404082
Conc: 23.80 ng/ml

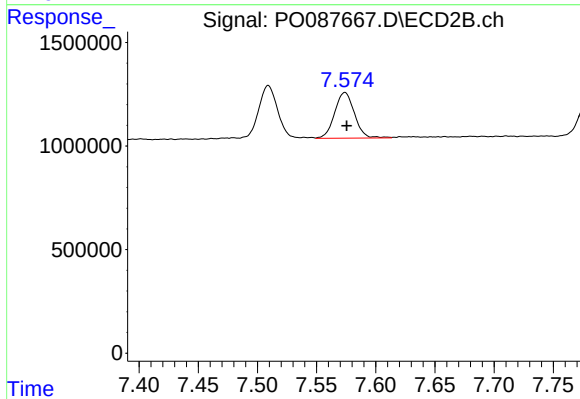

#42 AR-1268-2


R.T.: 7.574 min
Delta R.T.: -0.001 min
Response: 2571908
Conc: 25.05 ng/ml

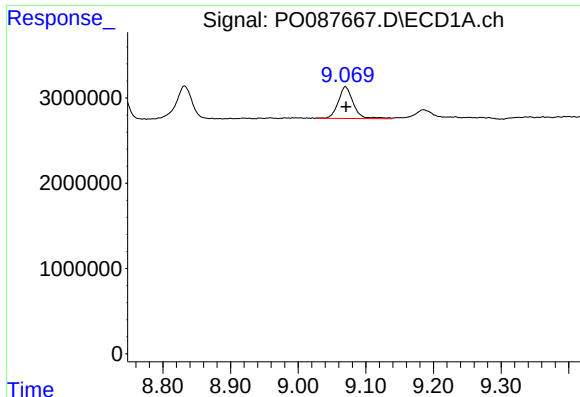

#43 AR-1268-3


R.T.: 9.070 min
Delta R.T.: 0.000 min
Response: 5770756
Conc: 24.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

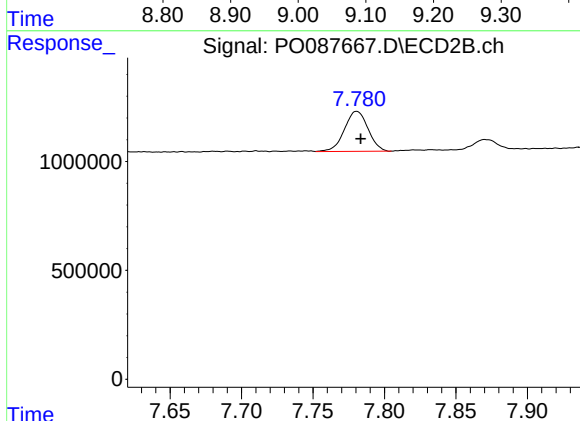


#43 AR-1268-3

R.T.: 7.781 min
Delta R.T.: -0.003 min
Response: 2121566
Conc: 25.06 ng/ml

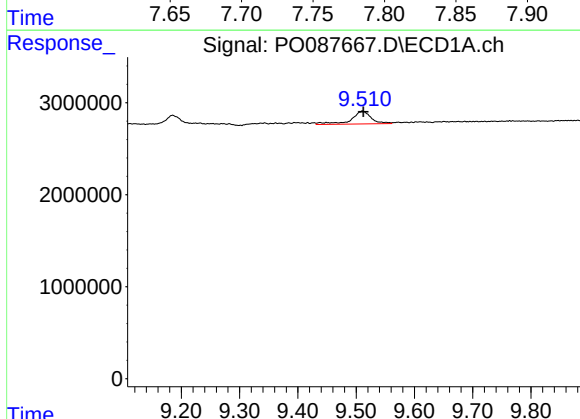


#44 AR-1268-4

R.T.: 9.511 min
Delta R.T.: -0.002 min
Response: 3315260
Conc: 32.43 ng/ml

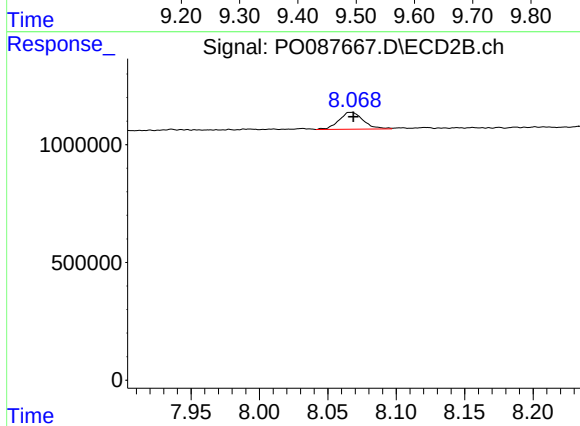

#44 AR-1268-4


R.T.: 8.067 min
Delta R.T.: -0.002 min
Response: 892279
Conc: 25.15 ng/ml

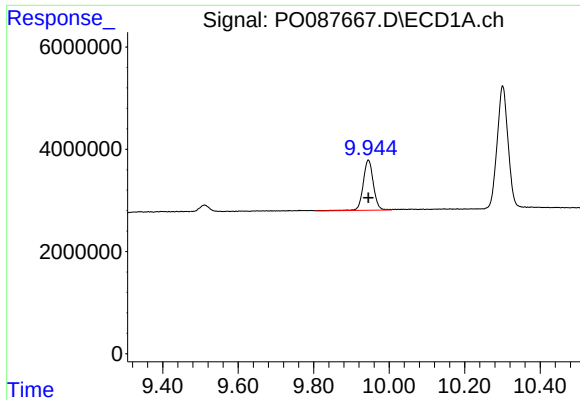

#45 AR-1268-5

R.T.: 9.945 min
Delta R.T.: 0.000 min
Response: 18452582
Conc: 24.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2022

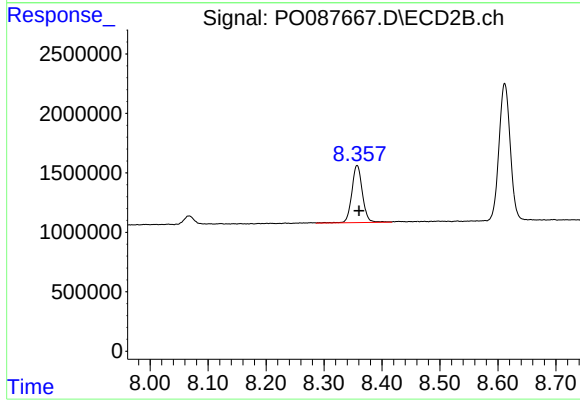

#45 AR-1268-5

R.T.: 8.357 min
Delta R.T.: -0.003 min
Response: 6113657
Conc: 24.41 ng/ml