

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063022\
 Data File : P0087688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2022 03:31
 Operator : YP/AJ
 Sample : N3559-07 10X
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMH459P-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/01/2022
 Supervised By :Ankita Jodhani 07/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 07:15:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.447	3.606	4530889	1859950	1.751m	1.890m
2) SA Decachlor...	10.297	8.611	5112794	1567826	2.503	1.934

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO063022\
Data File : PO087688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2022 03:31
Operator : YP/AJ
Sample : N3559-07 10X
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMH459P-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/01/2022
Supervised By :Ankita Jodhani 07/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 07:15:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

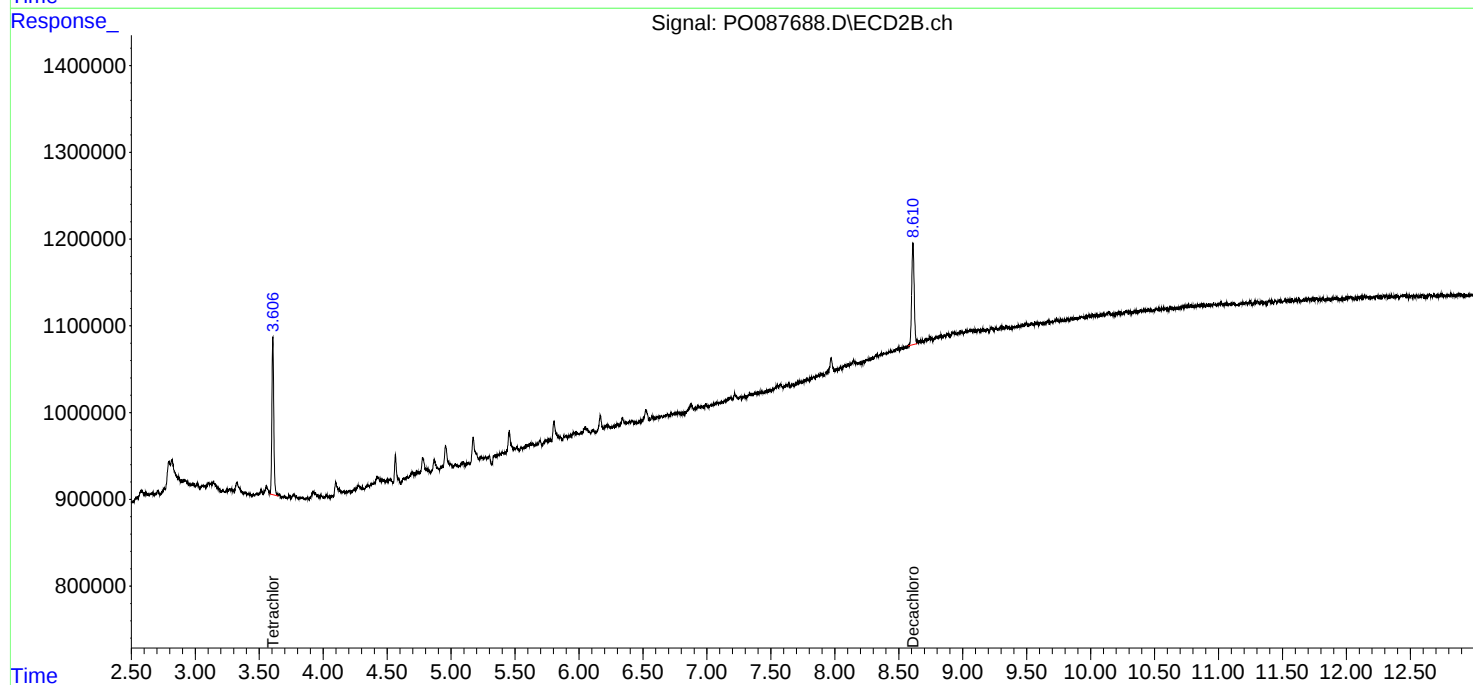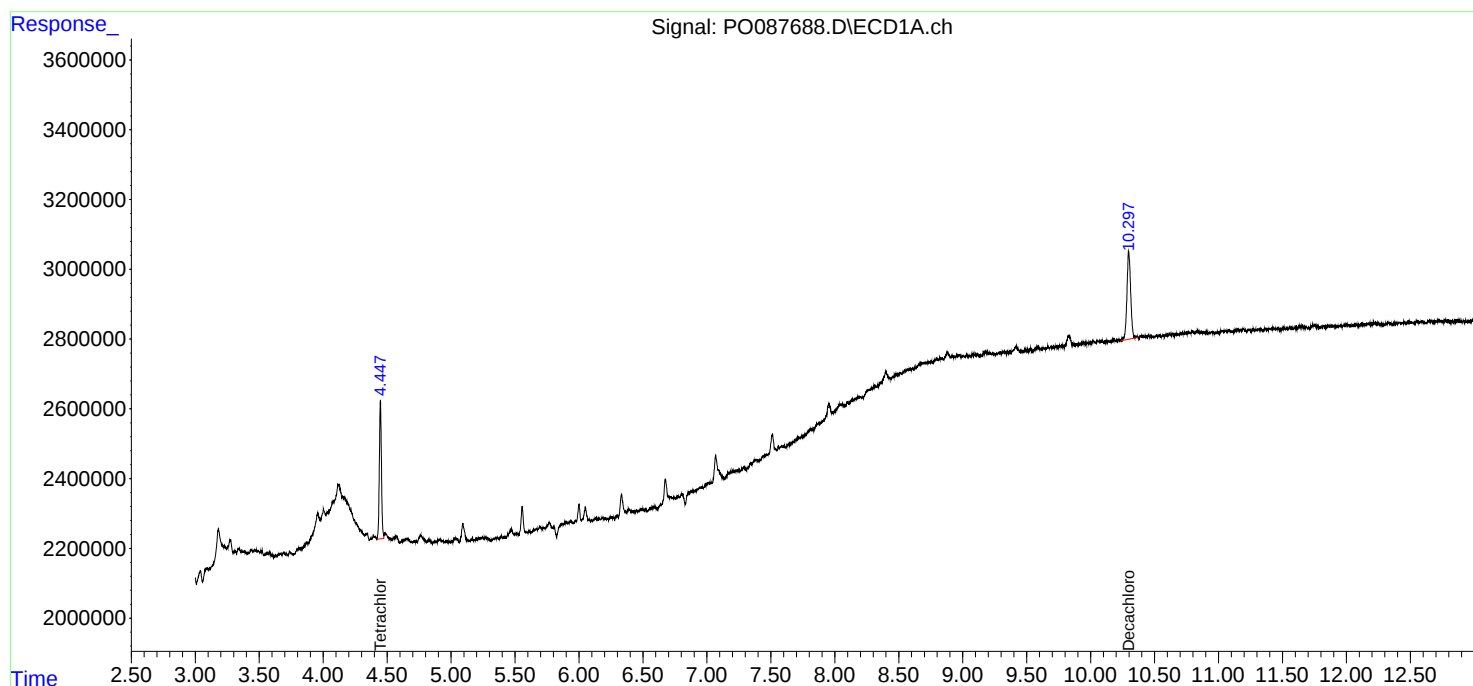

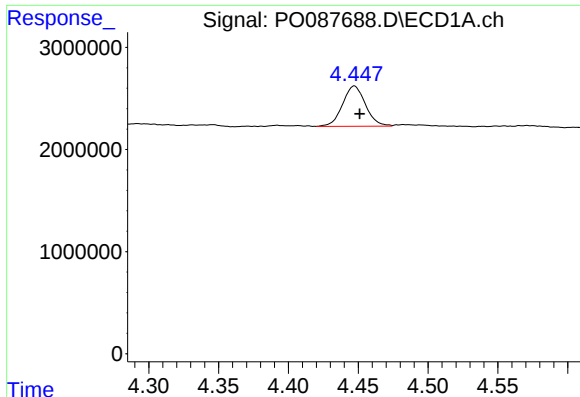


#1 Tetrachloro-m-xylene

R.T.: 4.447 min
Delta R.T.: -0.004 min
Response: 4530889
Conc: 1.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMH459P-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/01/2022
Supervised By :Ankita Jodhani 07/01/2022

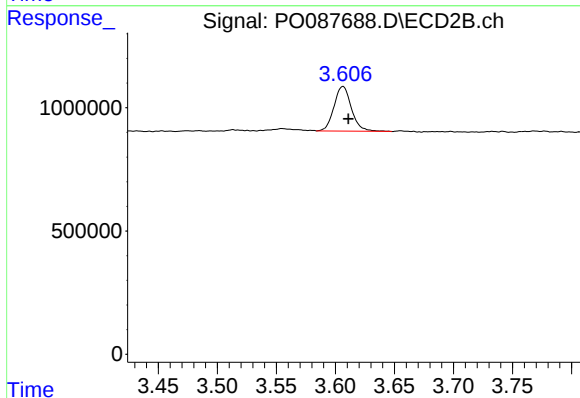


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: -0.005 min
Response: 1859950
Conc: 1.89 ng/ml m

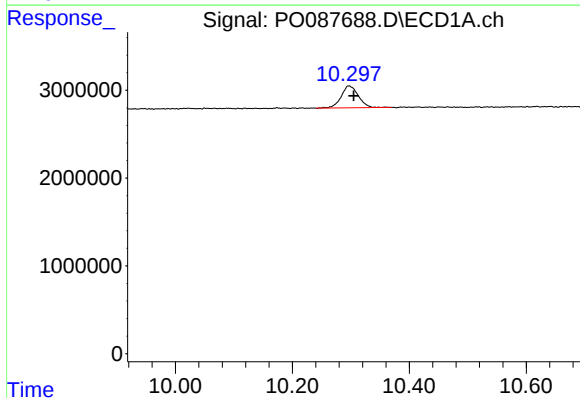

#2 Decachlorobiphenyl

R.T.: 10.297 min
Delta R.T.: -0.008 min
Response: 5112794
Conc: 2.50 ng/ml

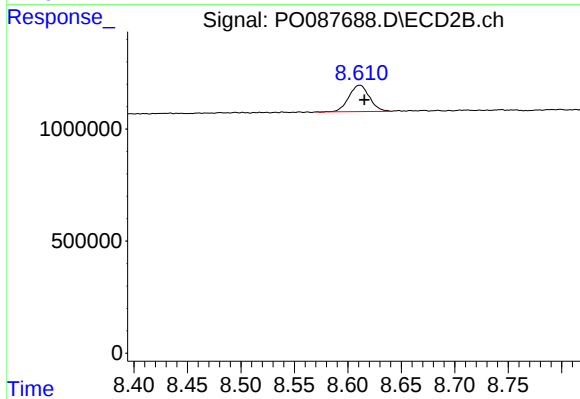

#2 Decachlorobiphenyl

R.T.: 8.611 min
Delta R.T.: -0.004 min
Response: 1567826
Conc: 1.93 ng/ml